

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044990.D
 Acq On : 07 Apr 2024 03:26
 Operator : MA/JU
 Sample : P2013-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	26	rBV2	20623	25953	0.64%	0.084%
2	3.616	87	90	103	rBV	108391	200982	4.95%	0.651%
3	3.905	135	139	145	rBV2	15550	20597	0.51%	0.067%
4	4.263	197	200	204	rBV5	3588	4994	0.12%	0.016%
5	5.175	352	355	359	rVB4	3988	4989	0.12%	0.016%
6	5.304	372	377	386	rBV5	10024	25183	0.62%	0.082%
7	5.669	434	439	446	rBV8	4944	9516	0.23%	0.031%
8	6.816	628	634	642	rBV	88508	159157	3.92%	0.515%
9	6.987	656	663	672	rBV	374616	599921	14.78%	1.942%
10	7.163	687	693	704	rBV	354619	604302	14.89%	1.956%
11	7.634	766	773	784	rBV	324107	542785	13.37%	1.757%
12	8.340	886	893	904	rBV	265083	471338	11.61%	1.526%
13	8.792	962	970	982	rBV	458386	777941	19.17%	2.518%
14	9.504	1084	1091	1102	rBV	387949	647404	15.95%	2.096%
15	10.034	1174	1181	1200	rBV	494313	930527	22.93%	3.012%
16	10.269	1216	1221	1224	rBV7	4563	7315	0.18%	0.024%
17	10.404	1235	1244	1256	rBV	490233	834363	20.56%	2.701%
18	10.563	1263	1271	1288	rBV	443375	876373	21.59%	2.837%
19	12.016	1514	1518	1526	rBV5	6896	13164	0.32%	0.043%
20	13.704	1797	1805	1815	rBV	1028113	1504163	37.06%	4.869%
21	13.975	1844	1851	1863	rBV	1329039	1948810	48.02%	6.308%
22	14.280	1895	1903	1912	rBV	816410	1185952	29.22%	3.839%
23	14.357	1912	1916	1926	rBV8	7917	20201	0.50%	0.065%
24	14.533	1940	1946	1972	rBV2	43926	151439	3.73%	0.490%
25	14.716	1972	1977	1981	rVV6	2652	4974	0.12%	0.016%
26	14.969	2016	2020	2024	rVB6	2710	4687	0.12%	0.015%
27	15.280	2067	2073	2082	rBV	1720802	2485885	61.25%	8.047%
28	15.421	2091	2097	2105	rBV	505838	711089	17.52%	2.302%
29	15.527	2111	2115	2119	rVB4	6410	9298	0.23%	0.030%
30	16.068	2201	2207	2211	rVB7	4952	8395	0.21%	0.027%
31	16.827	2330	2336	2341	rBB8	2401	4779	0.12%	0.015%
32	17.039	2365	2372	2379	rBV	1046720	1479217	36.45%	4.788%
33	17.139	2382	2389	2401	rBV2	2166451	3000050	73.92%	9.711%
34	17.445	2437	2441	2447	rVB7	4822	7079	0.17%	0.023%
35	17.815	2501	2504	2506	rBV3	4569	4919	0.12%	0.016%
36	17.951	2522	2527	2534	rBV2	64297	105627	2.60%	0.342%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044990.D
Acq On : 07 Apr 2024 03:26
Operator : MA/JU
Sample : P2013-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	18.021	2537	2539	2545	rVB7	2793	5892	0.15%	0.019%
38	18.386	2596	2601	2604	rBV4	13024	16569	0.41%	0.054%
39	19.009	2702	2707	2710	rBV3	23772	32706	0.81%	0.106%
40	19.080	2715	2719	2723	rBV2	20759	30866	0.76%	0.100%
41	19.121	2724	2726	2729	rVB4	4729	5806	0.14%	0.019%
42	19.245	2743	2747	2751	rBV3	31259	45242	1.11%	0.146%
43	19.392	2769	2772	2775	rBV4	11762	14217	0.35%	0.046%
44	19.445	2775	2781	2791	rVV	2667223	3592321	88.51%	11.628%
45	19.515	2791	2793	2796	rVB4	5566	6565	0.16%	0.021%
46	20.451	2950	2952	2955	rVB4	12698	9271	0.23%	0.030%
47	20.974	3038	3041	3048	rBV4	43659	55007	1.36%	0.178%
48	21.245	3082	3087	3093	rBV	1316697	1701891	41.93%	5.509%
49	23.333	3434	3442	3448	rBV	2279337	4058517	100.00%	13.137%
50	23.468	3459	3465	3477	rVB	1032203	1924671	47.42%	6.230%




Sum of corrected areas: 30892909

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044990.D
Acq On : 07 Apr 2024 03:26
Operator : MA/JU
Sample : P2013-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

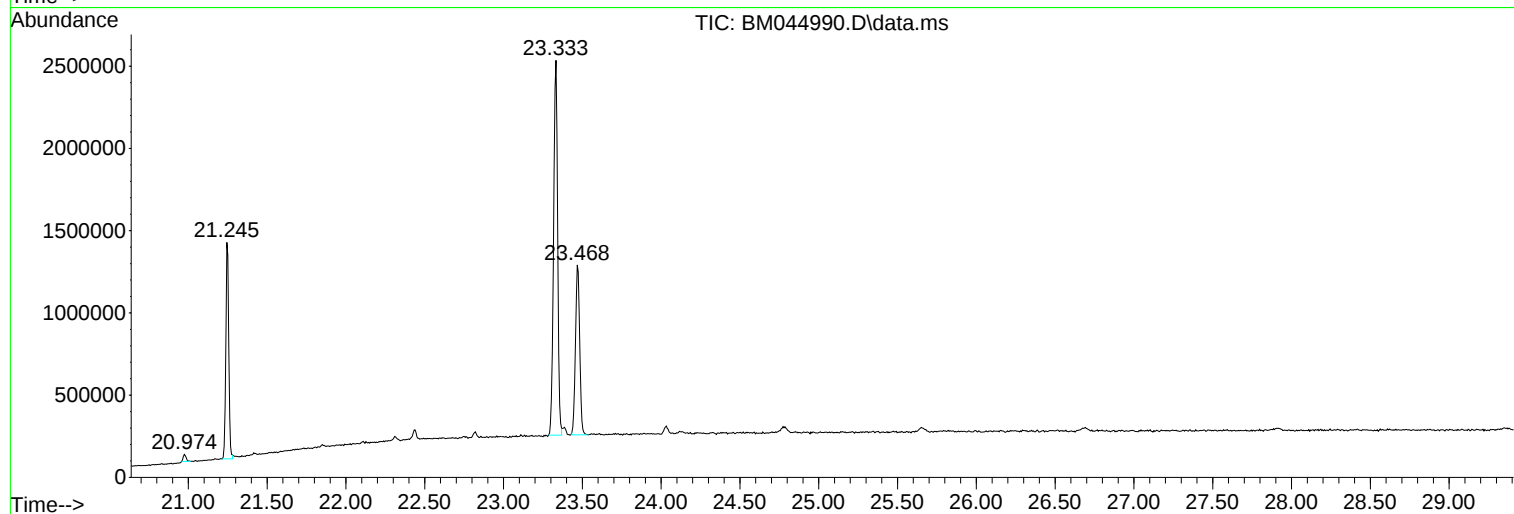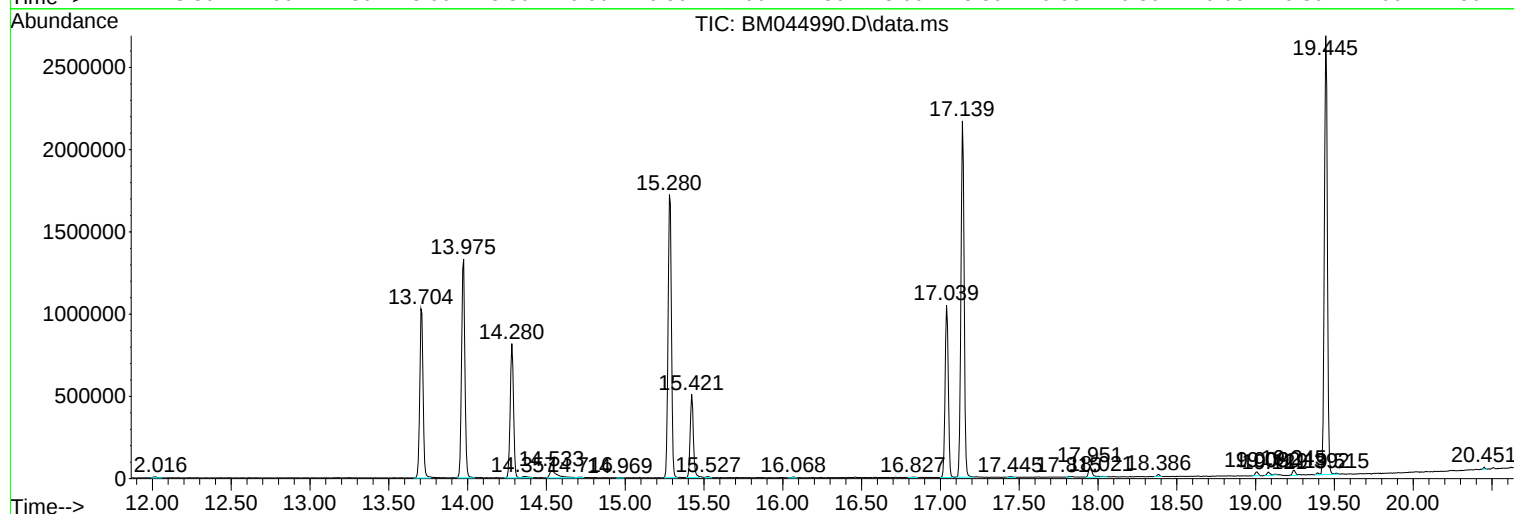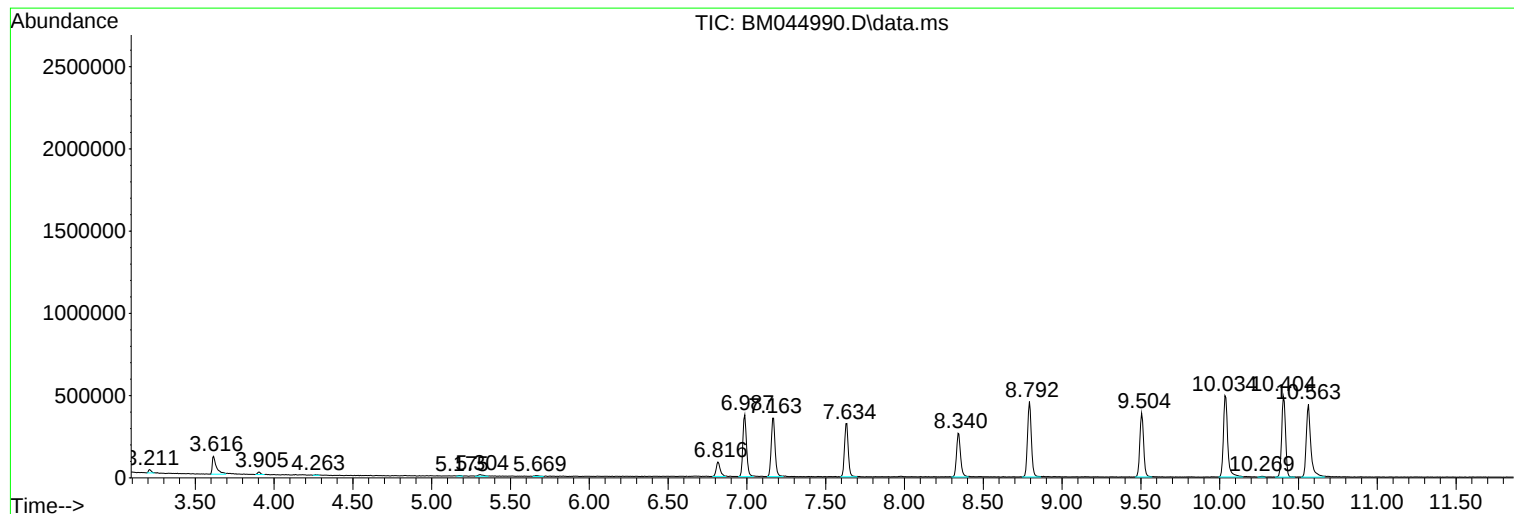

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044990.D
Acq On : 07 Apr 2024 03:26
Operator : MA/JU
Sample : P2013-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044990.D
Acq On : 07 Apr 2024 03:26
Operator : MA/JU
Sample : P2013-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc