

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044993.D
 Acq On : 07 Apr 2024 05:13
 Operator : MA/JU
 Sample : P2013-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	26	rVB	20663	23271	0.66%	0.079%
2	3.534	74	76	82	rVB2	10101	13706	0.39%	0.047%
3	3.616	87	90	102	rBV	102196	179891	5.12%	0.611%
4	3.904	136	139	144	rVB	7599	9885	0.28%	0.034%
5	4.128	173	177	180	rBV6	3637	5399	0.15%	0.018%
6	5.304	374	377	379	rBV3	5923	7578	0.22%	0.026%
7	5.663	434	438	442	rBV6	3684	6550	0.19%	0.022%
8	6.816	629	634	647	rBV	116124	207801	5.91%	0.705%
9	6.987	656	663	674	rBV	438646	685235	19.50%	2.326%
10	7.169	687	694	703	rBV	433397	716860	20.40%	2.433%
11	7.628	765	772	780	rBV	295352	481680	13.71%	1.635%
12	8.345	887	894	909	rBV	314368	558795	15.90%	1.896%
13	8.792	962	970	979	rBV	505532	856705	24.38%	2.908%
14	8.951	992	997	1003	rVB9	3621	5903	0.17%	0.020%
15	9.157	1026	1032	1036	rBV3	8150	14203	0.40%	0.048%
16	9.375	1065	1069	1078	rBV9	6331	12117	0.34%	0.041%
17	9.504	1084	1091	1101	rBV	429206	724002	20.61%	2.457%
18	10.039	1174	1182	1193	rBV	581671	1074490	30.58%	3.647%
19	10.222	1208	1213	1221	rBV5	9434	22857	0.65%	0.078%
20	10.404	1237	1244	1252	rVV	435700	721519	20.54%	2.449%
21	10.563	1264	1271	1296	rBV	282102	608612	17.32%	2.066%
22	11.080	1352	1359	1370	rVB2	8482	22387	0.64%	0.076%
23	11.186	1370	1377	1383	rBV4	7713	22754	0.65%	0.077%
24	11.657	1448	1457	1458	rVB6	1945	4039	0.11%	0.014%
25	12.004	1512	1516	1522	rVB4	8310	13803	0.39%	0.047%
26	12.774	1643	1647	1650	rBV5	2795	4169	0.12%	0.014%
27	13.098	1694	1702	1705	rBV7	3984	7732	0.22%	0.026%
28	13.174	1709	1715	1721	rVB4	9543	16117	0.46%	0.055%
29	13.704	1795	1805	1816	rBV	1096970	1553862	44.23%	5.274%
30	13.798	1819	1821	1828	rVB7	5191	8608	0.25%	0.029%
31	13.974	1841	1851	1870	rBV	1361532	2023118	57.58%	6.866%
32	14.280	1897	1903	1910	rBV	644462	949518	27.03%	3.223%
33	14.363	1911	1917	1926	rVV6	19165	47373	1.35%	0.161%
34	14.468	1932	1935	1938	rBV4	2616	3985	0.11%	0.014%
35	14.533	1941	1946	1964	rVV3	45872	133610	3.80%	0.453%
36	14.686	1969	1972	1974	rBV4	5709	7085	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044993.D
 Acq On : 07 Apr 2024 05:13
 Operator : MA/JU
 Sample : P2013-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.957	2013	2018	2022	rBV7	7102	14653	0.42%	0.050%
38	15.133	2042	2048	2054	rVB9	4832	10046	0.29%	0.034%
39	15.280	2066	2073	2083	rBV	1706274	2468836	70.27%	8.379%
40	15.421	2091	2097	2107	rBV	441900	629465	17.92%	2.136%
41	15.515	2111	2113	2115	rBV3	6994	6553	0.19%	0.022%
42	15.857	2168	2171	2174	rBV4	3416	4833	0.14%	0.016%
43	16.009	2193	2197	2200	rBV6	8384	11131	0.32%	0.038%
44	16.074	2204	2208	2213	rVB8	5500	8181	0.23%	0.028%
45	16.168	2222	2224	2228	rBV4	4619	4145	0.12%	0.014%
46	16.333	2248	2252	2258	rBV9	11143	20160	0.57%	0.068%
47	16.457	2269	2273	2279	rBV8	15223	23699	0.67%	0.080%
48	16.704	2313	2315	2318	rBV4	4287	4943	0.14%	0.017%
49	16.909	2348	2350	2352	rBV3	3932	4577	0.13%	0.016%
50	16.974	2356	2361	2366	rBV2	28400	34796	0.99%	0.118%
51	17.039	2366	2372	2377	rBV	807697	1116195	31.77%	3.788%
52	17.139	2383	2389	2398	rVB	1891706	2612475	74.36%	8.866%
53	17.227	2401	2404	2409	rVB5	13079	14897	0.42%	0.051%
54	17.445	2436	2441	2445	rBV6	16551	27827	0.79%	0.094%
55	17.521	2452	2454	2456	rBV3	5531	6456	0.18%	0.022%
56	17.715	2485	2487	2488	rBV2	7514	6114	0.17%	0.021%
57	17.821	2502	2505	2509	rBV5	17300	27165	0.77%	0.092%
58	17.951	2522	2527	2537	rBV	221023	343749	9.78%	1.167%
59	18.280	2581	2583	2584	rBV2	10015	8516	0.24%	0.029%
60	18.380	2597	2600	2605	rVB2	35451	40920	1.16%	0.139%
61	18.821	2671	2675	2682	rBV2	57880	78174	2.23%	0.265%
62	19.003	2703	2706	2711	rBV3	24772	35574	1.01%	0.121%
63	19.245	2743	2747	2754	rBV	92969	136645	3.89%	0.464%
64	19.445	2775	2781	2789	rBV	2443956	3202914	91.16%	10.870%
65	20.974	3038	3041	3048	rBV	157811	197508	5.62%	0.670%
66	21.244	3083	3087	3093	rBV	1022867	1292113	36.78%	4.385%
67	22.433	3286	3289	3295	rVB	261980	336691	9.58%	1.143%
68	23.333	3435	3442	3448	rBV	1966078	3513349	100.00%	11.924%
69	23.468	3459	3465	3474	rVB	776079	1466636	41.74%	4.978%




Sum of corrected areas: 29465155

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044993.D
Acq On : 07 Apr 2024 05:13
Operator : MA/JU
Sample : P2013-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

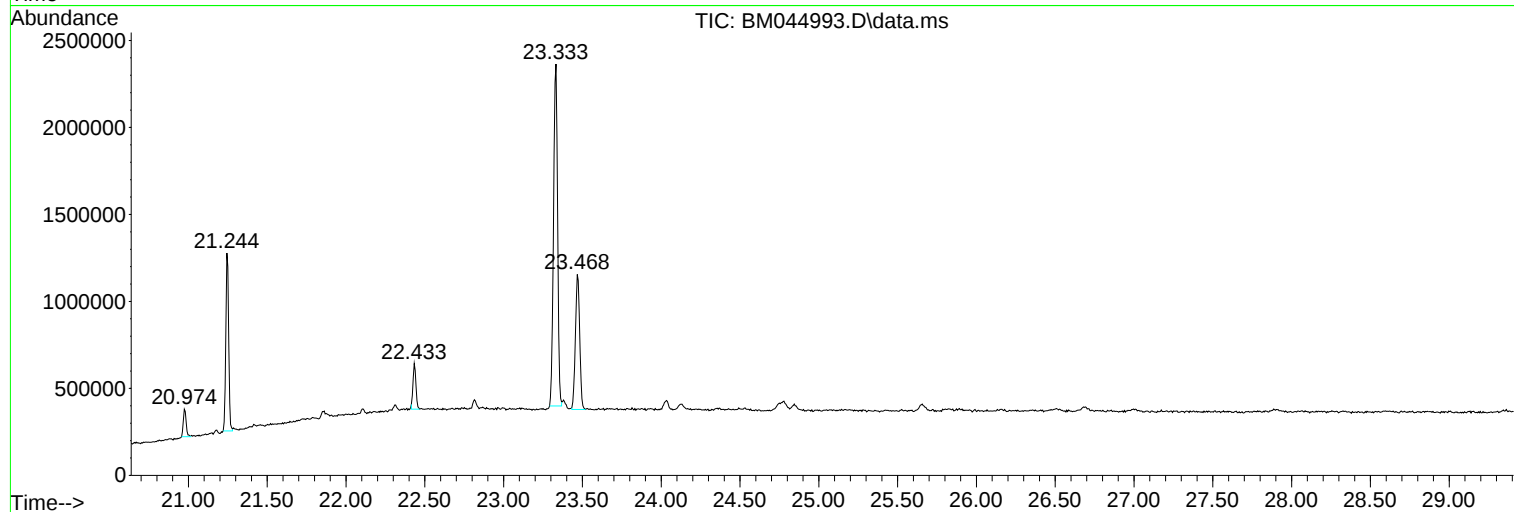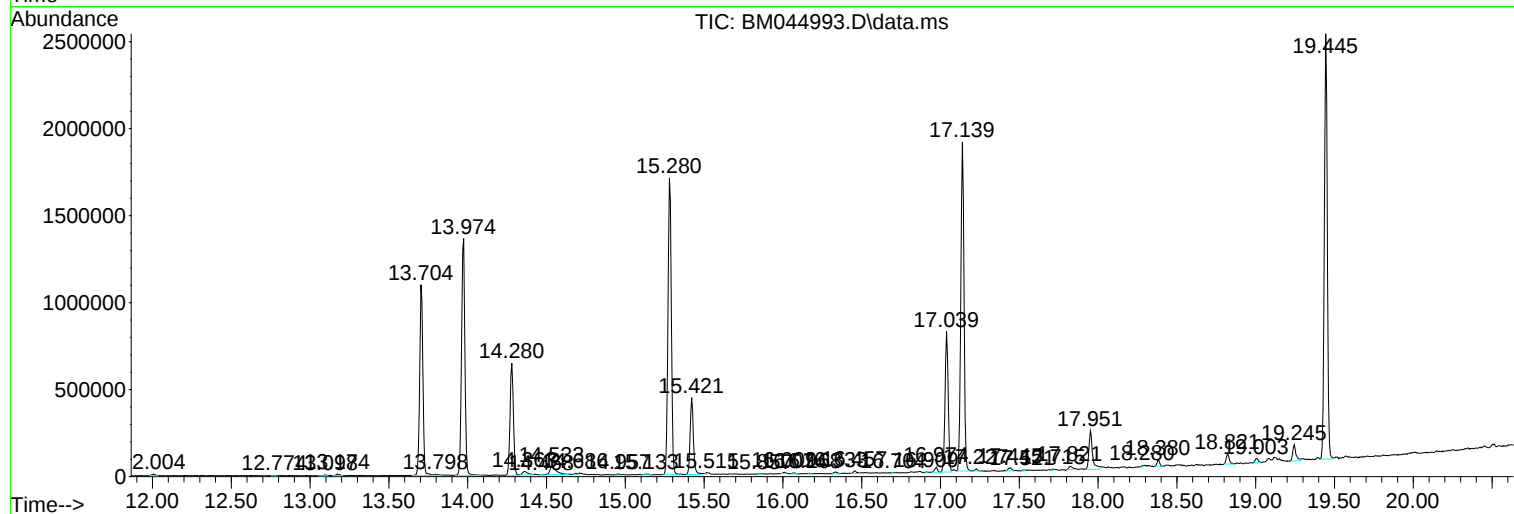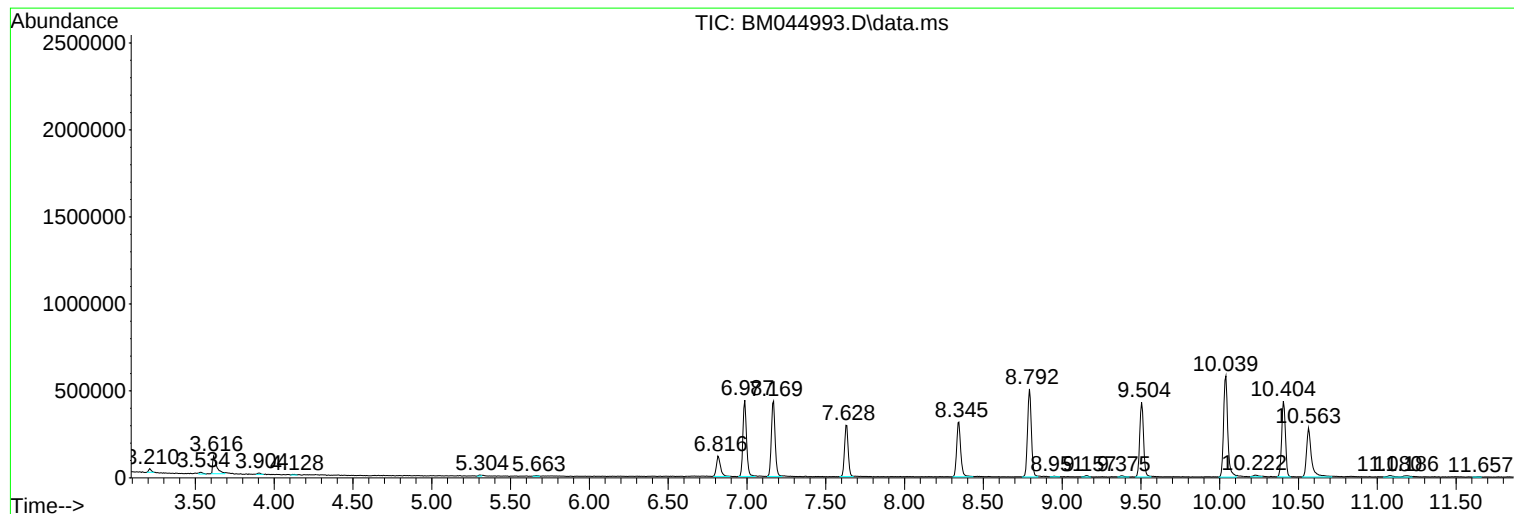

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044993.D
Acq On : 07 Apr 2024 05:13
Operator : MA/JU
Sample : P2013-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044993.D
Acq On : 07 Apr 2024 05:13
Operator : MA/JU
Sample : P2013-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc