

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044994.D
 Acq On : 07 Apr 2024 05:49
 Operator : MA/JU
 Sample : P2013-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	25	rBV	19961	25666	0.79%	0.097%
2	3.616	87	90	103	rBV	88223	165671	5.08%	0.625%
3	3.898	136	138	142	rVB3	4943	5014	0.15%	0.019%
4	5.175	352	355	360	rBV4	3707	5882	0.18%	0.022%
5	5.304	374	377	384	rVB3	8768	14757	0.45%	0.056%
6	5.669	435	439	444	rBV6	5159	8688	0.27%	0.033%
7	6.822	628	635	644	rBV	89880	176115	5.40%	0.664%
8	6.987	657	663	675	rBV	376671	598086	18.33%	2.256%
9	7.169	686	694	704	rBV	376760	624151	19.13%	2.355%
10	7.628	765	772	781	rBV	295482	490628	15.04%	1.851%
11	8.345	886	894	905	rBV	280758	488178	14.96%	1.842%
12	8.792	963	970	987	rBV	449005	764116	23.42%	2.883%
13	8.945	995	996	1005	rVB6	2499	5097	0.16%	0.019%
14	9.157	1028	1032	1038	rVB2	6753	10065	0.31%	0.038%
15	9.504	1084	1091	1104	rBV	376426	637781	19.55%	2.406%
16	10.039	1174	1182	1192	rBV	473522	889767	27.28%	3.357%
17	10.404	1236	1244	1253	rVB	429583	725799	22.25%	2.738%
18	10.563	1262	1271	1286	rBV	363941	746083	22.87%	2.815%
19	12.016	1513	1518	1523	rBV3	6519	12316	0.38%	0.046%
20	13.174	1710	1715	1724	rVB8	7513	13863	0.42%	0.052%
21	13.704	1796	1805	1817	rBV	967821	1373780	42.11%	5.183%
22	13.974	1843	1851	1861	rBV	1170028	1769839	54.25%	6.677%
23	14.280	1893	1903	1911	rBV	672608	971337	29.78%	3.664%
24	14.351	1911	1915	1931	rVV	46131	110612	3.39%	0.417%
25	14.539	1941	1947	1961	rBV2	42408	130909	4.01%	0.494%
26	15.280	2067	2073	2084	rBV	1524670	2209898	67.74%	8.337%
27	15.421	2091	2097	2109	rVV	445404	629550	19.30%	2.375%
28	15.521	2111	2114	2122	rVB7	6104	11159	0.34%	0.042%
29	16.074	2203	2208	2211	rVB6	4939	6913	0.21%	0.026%
30	16.827	2330	2336	2338	rBV6	3199	6416	0.20%	0.024%
31	16.968	2357	2360	2364	rBV5	6209	7816	0.24%	0.029%
32	17.039	2366	2372	2381	rBV	821005	1128979	34.61%	4.259%
33	17.139	2381	2389	2401	rBV	1836470	2552594	78.25%	9.630%
34	17.439	2436	2440	2445	rBV7	7622	10568	0.32%	0.040%
35	17.827	2503	2506	2509	rBV5	3589	4980	0.15%	0.019%
36	17.951	2521	2527	2533	rBV3	41088	64073	1.96%	0.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044994.D
Acq On : 07 Apr 2024 05:49
Operator : MA/JU
Sample : P2013-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	18.280	2579	2583	2585	rBV5	3020	5101	0.16%	0.019%
38	18.386	2597	2601	2603	rBV5	7478	8912	0.27%	0.034%
39	18.821	2671	2675	2678	rBV6	8380	12909	0.40%	0.049%
40	19.003	2702	2706	2713	rVB3	20313	29598	0.91%	0.112%
41	19.080	2714	2719	2724	rBV2	22401	30687	0.94%	0.116%
42	19.245	2743	2747	2751	rBV4	25554	32685	1.00%	0.123%
43	19.397	2770	2773	2775	rBV4	7315	6663	0.20%	0.025%
44	19.445	2775	2781	2788	rBV	2351171	2971232	91.08%	11.209%
45	20.974	3038	3041	3049	rBV8	40182	66341	2.03%	0.250%
46	21.244	3082	3087	3096	rBV	966541	1270948	38.96%	4.795%
47	23.333	3435	3442	3448	rBV	1828931	3262143	100.00%	12.307%
48	23.468	3459	3465	3475	rVB	738745	1412922	43.31%	5.330%




Sum of corrected areas: 26507287

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044994.D
Acq On : 07 Apr 2024 05:49
Operator : MA/JU
Sample : P2013-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

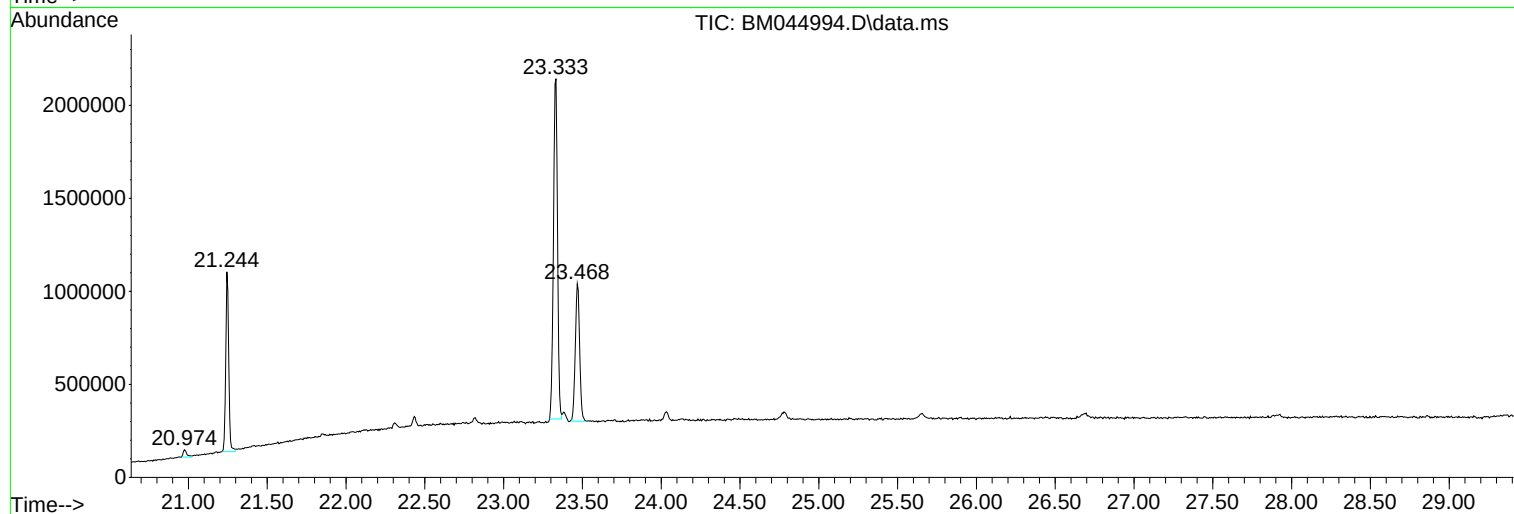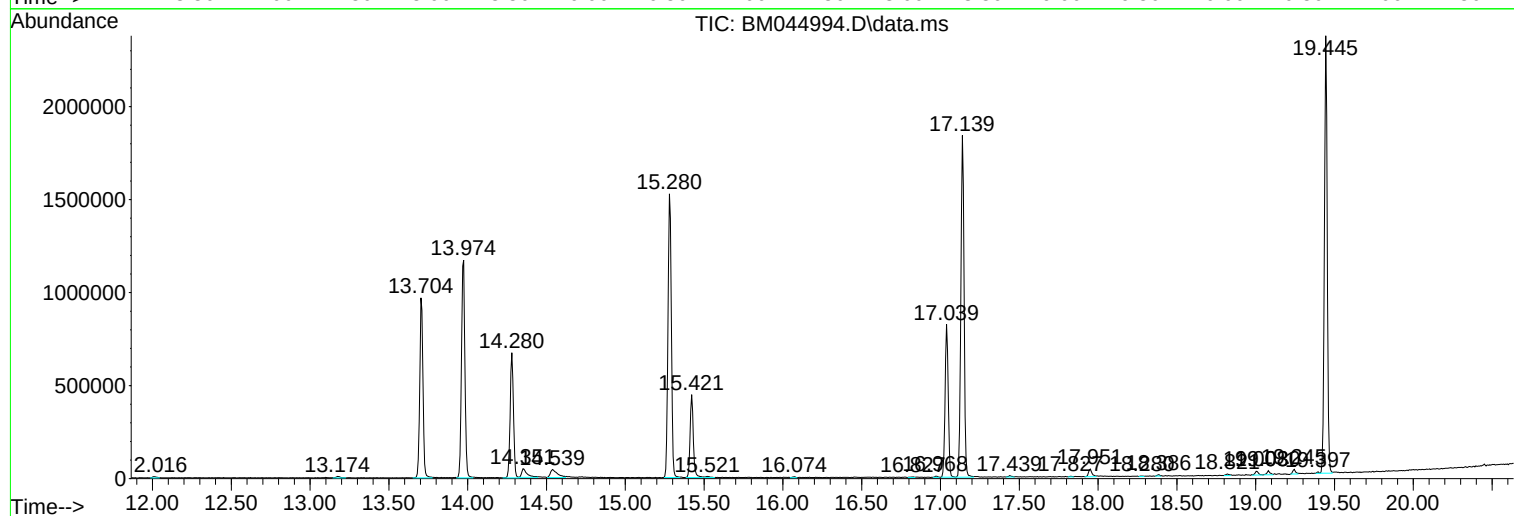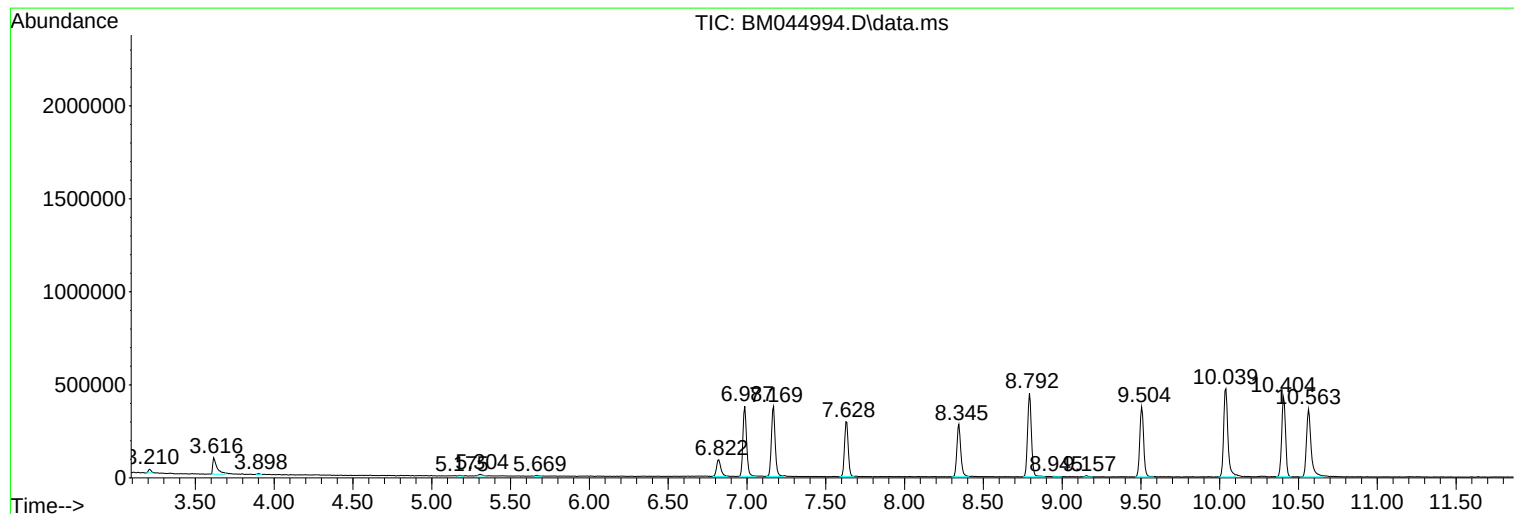

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044994.D
Acq On : 07 Apr 2024 05:49
Operator : MA/JU
Sample : P2013-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzoic acid, 2,4-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.351	2.28 ng/ul	110612	Acenaphthene-d10	14.280

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzoic acid, 2,4-dichloro-	190	C7H4Cl2O2	000050-84-0	97
2			Benzoic acid, 2,6-dichloro-	190	C7H4Cl2O2	000050-30-6	97
3			Benzoic acid, 2,6-dichloro-	190	C7H4Cl2O2	000050-30-6	95
4			Benzoic acid, 3,4-dichloro-	190	C7H4Cl2O2	000051-44-5	95
5			Benzoic acid, 3,4-dichloro-	190	C7H4Cl2O2	000051-44-5	95

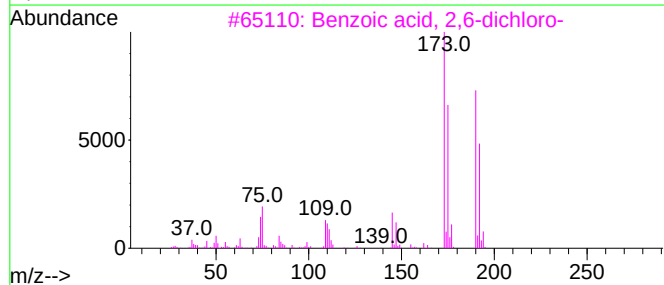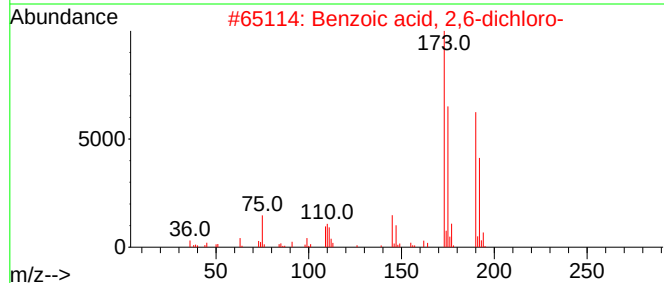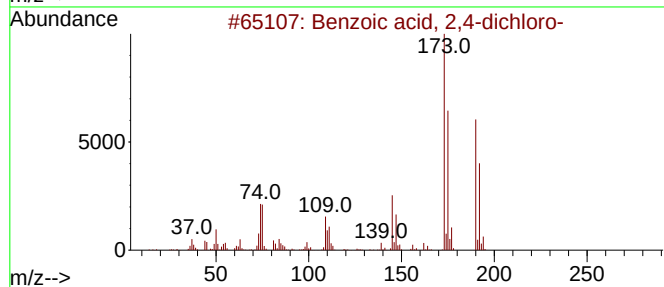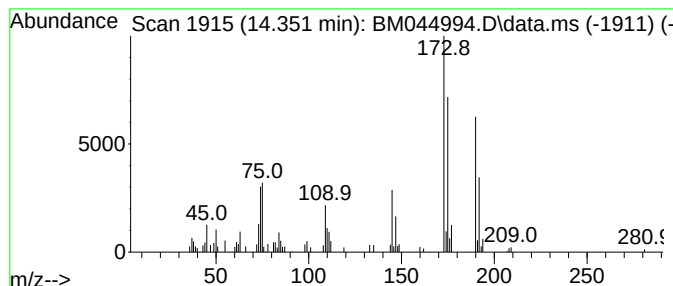

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044994.D
Acq On : 07 Apr 2024 05:49
Operator : MA/JU
Sample : P2013-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzoic acid, 2...	14.351	2.3	ng/u1	110612	3	14.280	971337	20.0