

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM045000.D
 Acq On : 07 Apr 2024 10:00
 Operator : MA/JU
 Sample : PB160034BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	18	20	25	rBV	21912	27350	1.16%	0.131%
2	3.605	85	88	108	rBV	239091	430408	18.22%	2.063%
3	3.905	135	139	142	rBV4	4608	5362	0.23%	0.026%
4	4.322	208	210	214	rVB3	3328	3258	0.14%	0.016%
5	4.922	310	312	315	rBV4	2101	2563	0.11%	0.012%
6	5.028	329	330	334	rVB3	2644	2826	0.12%	0.014%
7	5.069	334	337	338	rBV2	2511	2641	0.11%	0.013%
8	5.275	369	372	375	rVB5	2333	3142	0.13%	0.015%
9	5.322	375	380	383	rBV5	2717	4630	0.20%	0.022%
10	6.181	525	526	531	rVB5	3028	2664	0.11%	0.013%
11	6.481	574	577	581	rBV6	1508	2851	0.12%	0.014%
12	6.816	627	634	644	rBV	289168	515231	21.82%	2.469%
13	6.987	656	663	673	rBV	244564	406191	17.20%	1.946%
14	7.163	687	693	707	rBV	318851	526747	22.30%	2.524%
15	7.628	764	772	785	rBV	220966	357366	15.13%	1.713%
16	8.340	884	893	908	rVV	372758	640243	27.11%	3.068%
17	8.792	963	970	983	rBV	291444	502064	21.26%	2.406%
18	8.881	983	985	990	rVB7	2171	3224	0.14%	0.015%
19	9.504	1084	1091	1099	rBV	254403	433628	18.36%	2.078%
20	9.557	1099	1100	1106	rVB6	3462	3630	0.15%	0.017%
21	9.798	1137	1141	1144	rVB5	1778	2582	0.11%	0.012%
22	10.039	1175	1182	1199	rBV	331617	652810	27.64%	3.128%
23	10.404	1236	1244	1252	rBV	317210	527594	22.34%	2.528%
24	10.563	1262	1271	1288	rBV	375128	790945	33.49%	3.790%
25	12.028	1515	1520	1528	rVB5	3813	8959	0.38%	0.043%
26	12.469	1592	1595	1599	rBV5	1967	3004	0.13%	0.014%
27	13.180	1712	1716	1719	rVB5	3100	4212	0.18%	0.020%
28	13.704	1797	1805	1818	rBV	669913	1001028	42.39%	4.797%
29	13.969	1843	1850	1860	rBV	836919	1234411	52.27%	5.915%
30	14.280	1896	1903	1913	rBV	511122	763697	32.34%	3.660%
31	14.521	1938	1944	1962	rBV	179763	470769	19.93%	2.256%
32	14.892	2005	2007	2013	rVB6	1638	2595	0.11%	0.012%
33	15.280	2065	2073	2084	rBV	1101738	1570868	66.52%	7.528%
34	15.421	2090	2097	2111	rBV	309400	447609	18.95%	2.145%
35	15.521	2111	2114	2118	rVB4	4322	5382	0.23%	0.026%
36	16.068	2203	2207	2212	rVB5	3806	4880	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM045000.D
 Acq On : 07 Apr 2024 10:00
 Operator : MA/JU
 Sample : PB160034BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.445	2268	2271	2274	rBV3	2010	2916	0.12%	0.014%
38	17.039	2366	2372	2381	rBV	663323	944278	39.98%	4.525%
39	17.139	2382	2389	2400	rVV	1245673	1765830	74.77%	8.462%
40	17.215	2400	2402	2405	rVB3	2869	2887	0.12%	0.014%
41	17.439	2435	2440	2443	rVV6	1641	2403	0.10%	0.012%
42	17.704	2483	2485	2489	rVB3	1811	2483	0.11%	0.012%
43	18.009	2534	2537	2539	rBV4	1879	2485	0.11%	0.012%
44	19.009	2703	2707	2710	rBV4	12023	16255	0.69%	0.078%
45	19.080	2715	2719	2725	rVB2	11159	16278	0.69%	0.078%
46	19.345	2760	2764	2767	rBV6	2769	4635	0.20%	0.022%
47	19.392	2770	2772	2775	rBV4	5822	6269	0.27%	0.030%
48	19.445	2775	2781	2791	rVV	1507502	2063112	87.36%	9.887%
49	21.245	3082	3087	3096	rBV	806077	1083240	45.87%	5.191%
50	23.327	3434	3441	3448	rBV2	1275913	2361670	100.00%	11.317%
51	23.468	3458	3465	3475	rVB	620901	1225785	51.90%	5.874%




Sum of corrected areas: 20867890

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045000.D
Acq On : 07 Apr 2024 10:00
Operator : MA/JU
Sample : PB160034BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

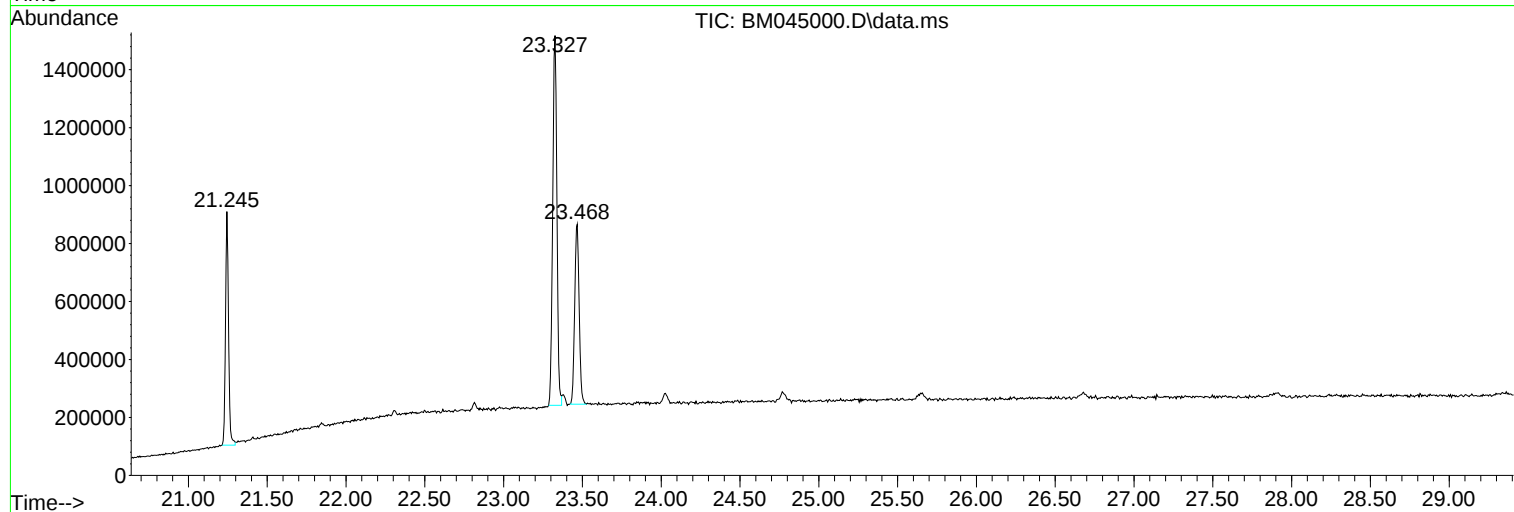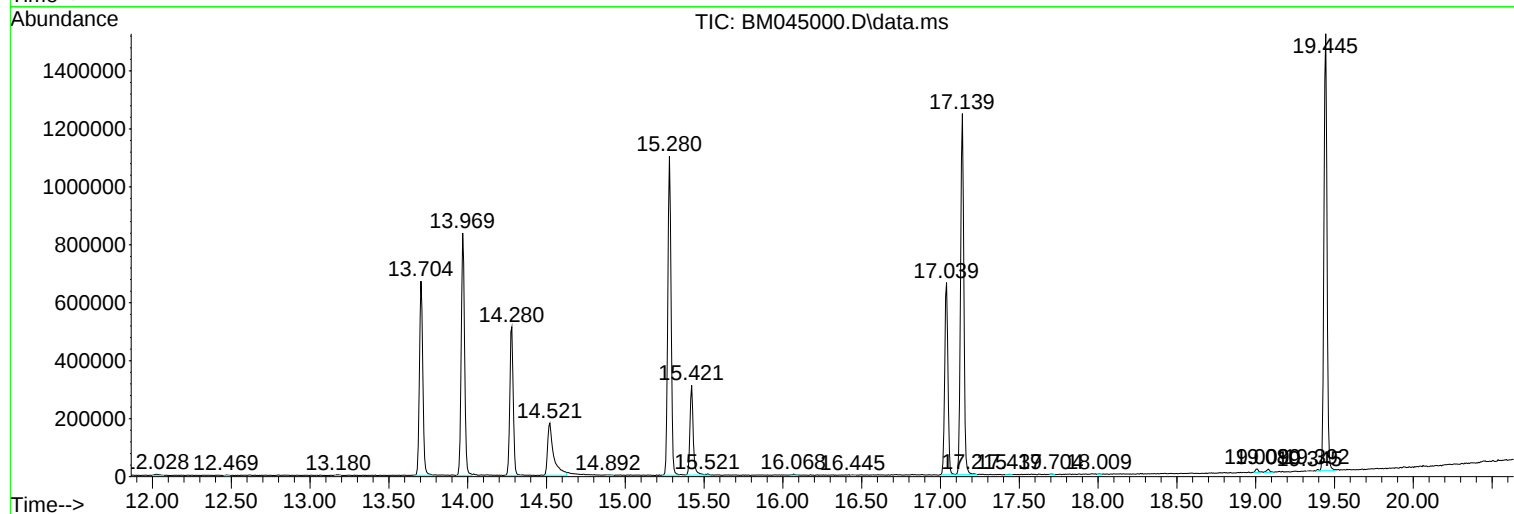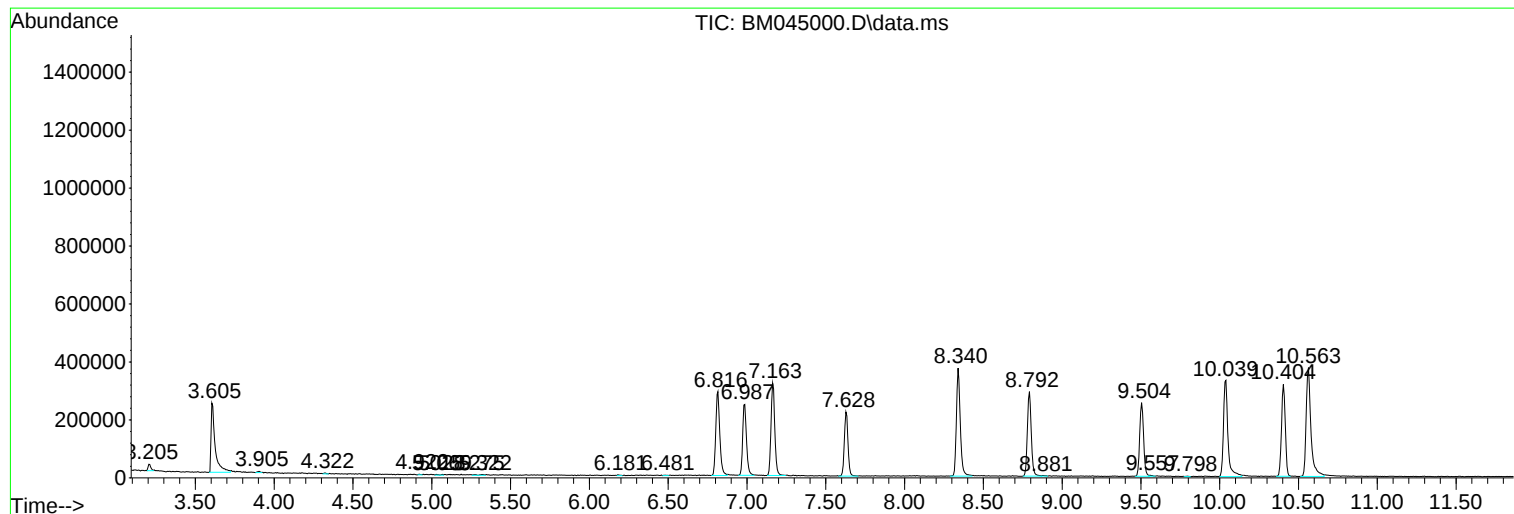

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045000.D
Acq On : 07 Apr 2024 10:00
Operator : MA/JU
Sample : PB160034BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045000.D
Acq On : 07 Apr 2024 10:00
Operator : MA/JU
Sample : PB160034BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc