

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM045001.D
 Acq On : 07 Apr 2024 10:35
 Operator : MA/JU
 Sample : P1997-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	24	rBV	15177	16910	0.56%	0.071%
2	3.616	87	90	104	rBV	80426	155630	5.11%	0.652%
3	6.028	497	500	503	rBV4	2775	3494	0.11%	0.015%
4	6.816	629	634	643	rBV	73114	137985	4.53%	0.578%
5	6.987	656	663	675	rBV	353463	579613	19.04%	2.428%
6	7.163	687	693	704	rBV	344498	574261	18.87%	2.405%
7	7.628	766	772	781	rBV	221635	361464	11.87%	1.514%
8	8.339	884	893	904	rBV	250535	437837	14.38%	1.834%
9	8.792	962	970	983	rBV	435864	733545	24.10%	3.072%
10	9.504	1084	1091	1110	rBV	368586	631276	20.74%	2.644%
11	9.698	1120	1124	1127	rBV5	1778	3182	0.10%	0.013%
12	10.033	1174	1181	1198	rBV	476696	884459	29.06%	3.705%
13	10.404	1235	1244	1254	rVB	337205	556843	18.29%	2.332%
14	10.563	1263	1271	1288	rBV	390758	824367	27.08%	3.453%
15	12.022	1511	1519	1525	rBV4	5554	12239	0.40%	0.051%
16	13.174	1709	1715	1721	rVV8	5874	11240	0.37%	0.047%
17	13.704	1797	1805	1818	rBV	910468	1316349	43.25%	5.514%
18	13.968	1843	1850	1862	rBV	1165737	1733356	56.94%	7.260%
19	14.280	1895	1903	1911	rBV	500305	743231	24.42%	3.113%
20	14.551	1943	1949	1960	rBV5	21464	72674	2.39%	0.304%
21	15.280	2067	2073	2085	rBV	1536276	2151096	70.67%	9.010%
22	15.421	2091	2097	2110	rBV	380356	563446	18.51%	2.360%
23	15.527	2110	2115	2119	rVB5	6992	12514	0.41%	0.052%
24	16.068	2203	2207	2211	rBV4	4176	6751	0.22%	0.028%
25	16.368	2253	2258	2261	rBV5	1844	4046	0.13%	0.017%
26	16.468	2272	2275	2278	rBV5	2979	3891	0.13%	0.016%
27	17.039	2365	2372	2381	rBV	622151	878281	28.85%	3.679%
28	17.139	2382	2389	2402	rVV	1693600	2399191	78.82%	10.049%
29	17.945	2522	2526	2535	rBV3	26054	42802	1.41%	0.179%
30	18.239	2571	2576	2577	rBV5	2289	3201	0.11%	0.013%
31	18.880	2683	2685	2690	rBV6	3121	6007	0.20%	0.025%
32	19.003	2702	2706	2711	rVB4	18840	26584	0.87%	0.111%
33	19.080	2715	2719	2725	rVV	13216	20073	0.66%	0.084%
34	19.239	2742	2746	2753	rBV7	24653	40831	1.34%	0.171%
35	19.445	2774	2781	2789	rBV	2157400	2820358	92.66%	11.813%
36	19.939	2863	2865	2866	rBV2	5068	3749	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045001.D
Acq On : 07 Apr 2024 10:35
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	21.244	3082	3087	3095	rBV2	725465	973343	31.98%	4.077%
38	23.327	3434	3441	3448	rBV2	1679221	3043914	100.00%	12.749%
39	23.468	3458	3465	3473	rBV	557578	1084893	35.64%	4.544%




Sum of corrected areas: 23874926

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045001.D
Acq On : 07 Apr 2024 10:35
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

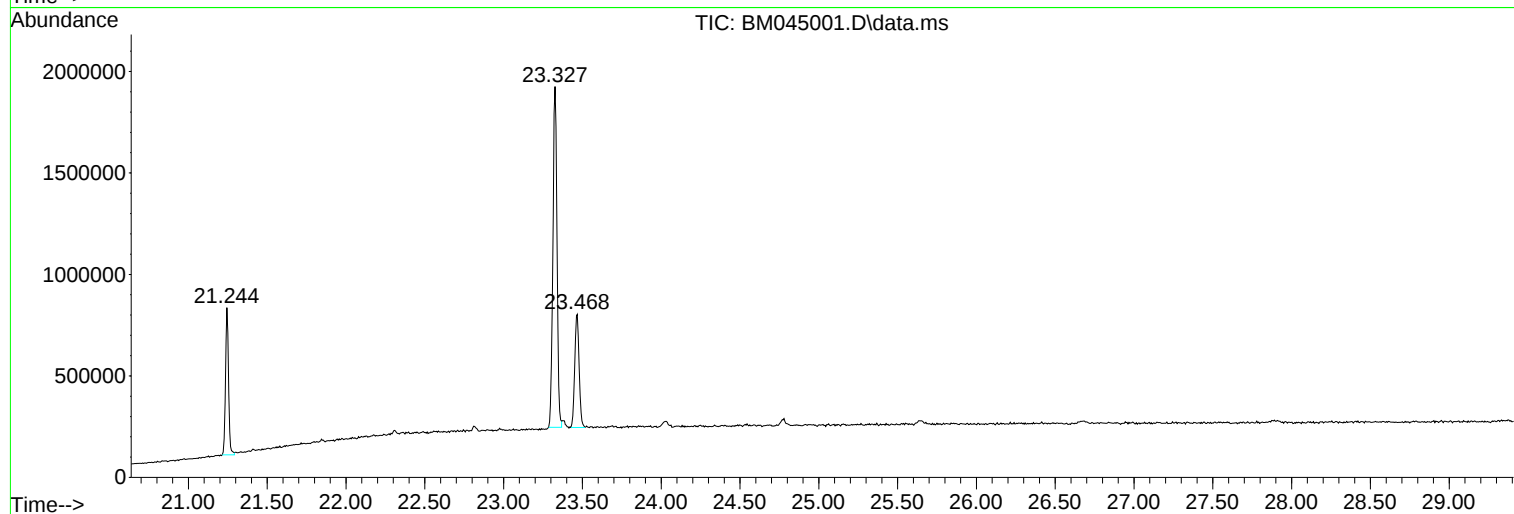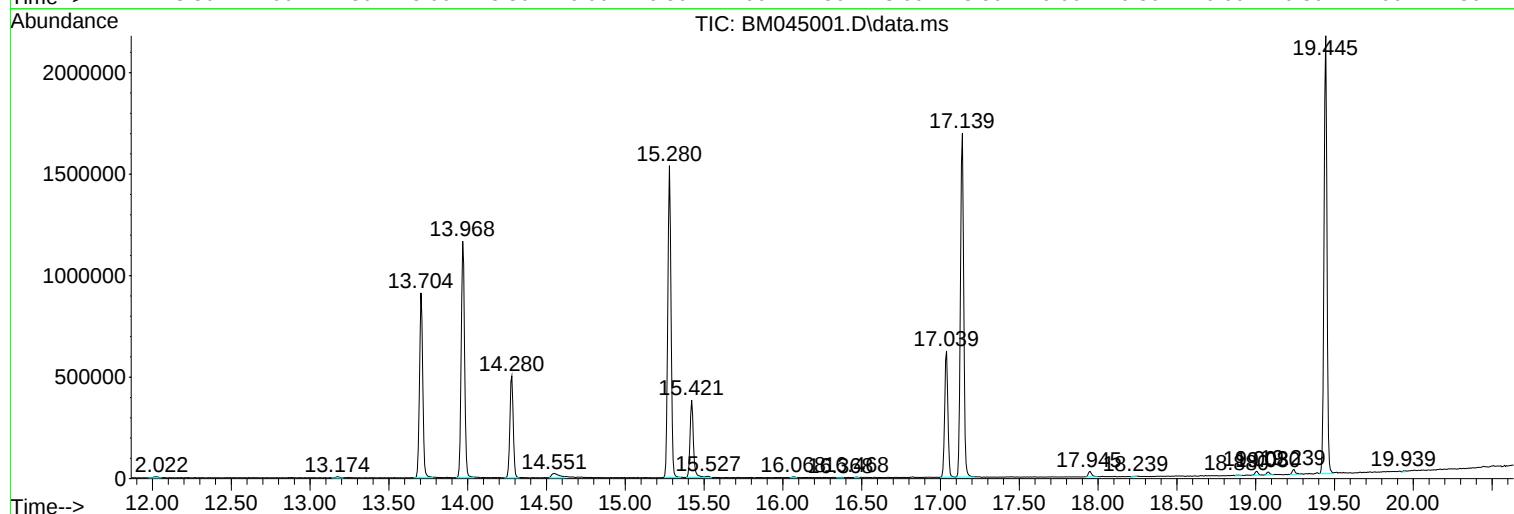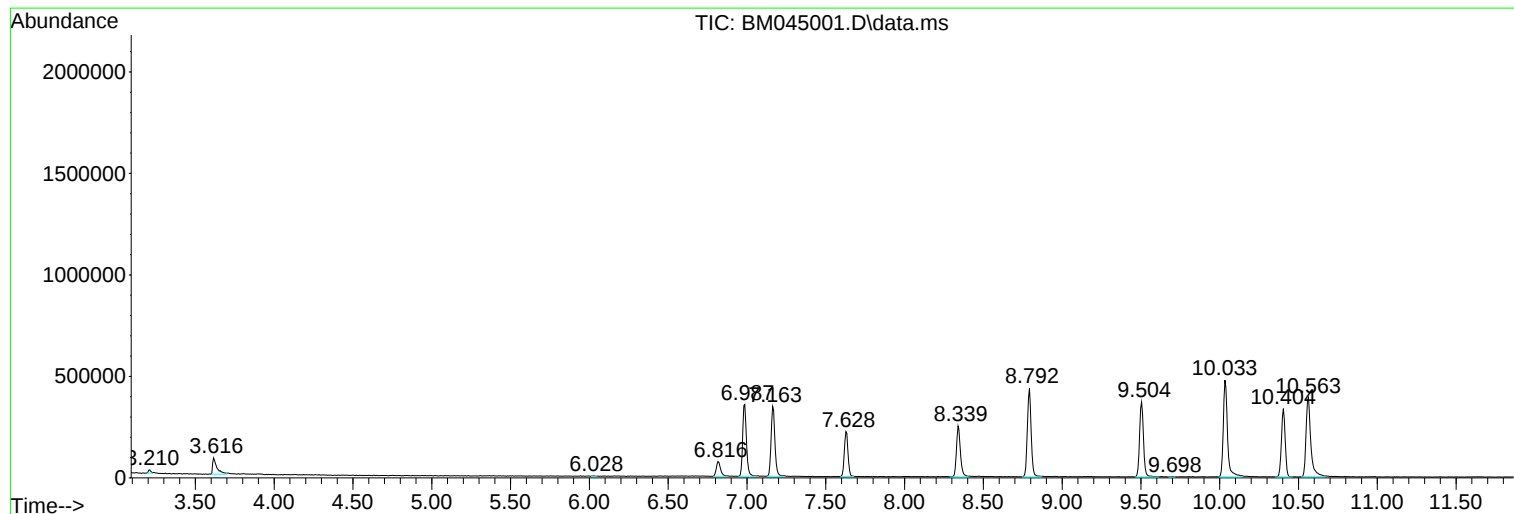

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045001.D
Acq On : 07 Apr 2024 10:35
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM045001.D
Acq On : 07 Apr 2024 10:35
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc