




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040722\
 Data File : BM034540.D
 Acq On : 07 Apr 2022 10:17
 Operator : CG/JU
 Sample : PB143886BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK886

Manual IntegrationsAPPROVED

Quant Time: Apr 08 04:56:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 07 12:11:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

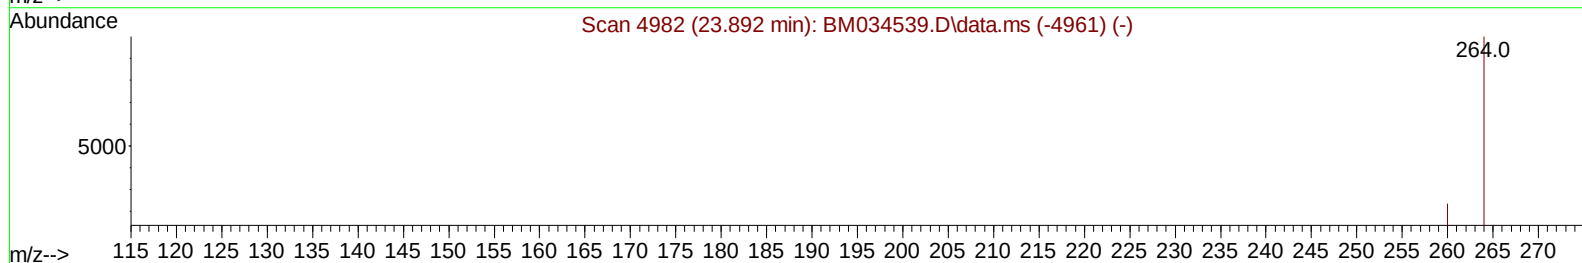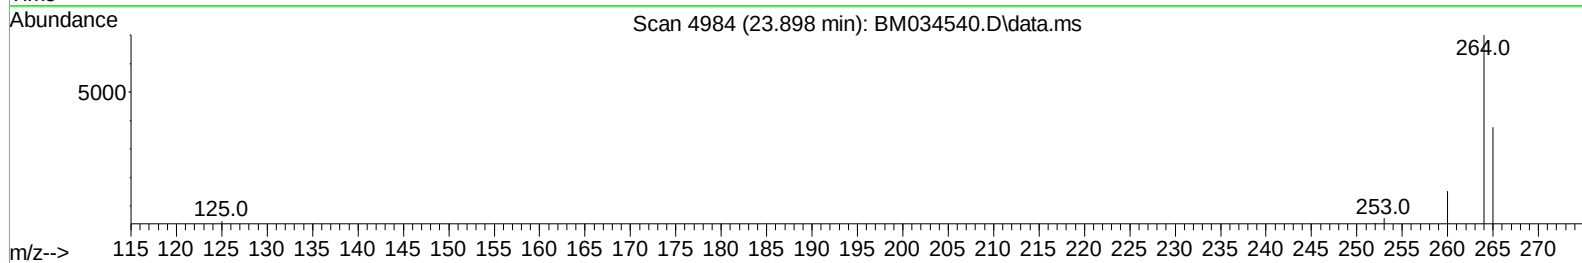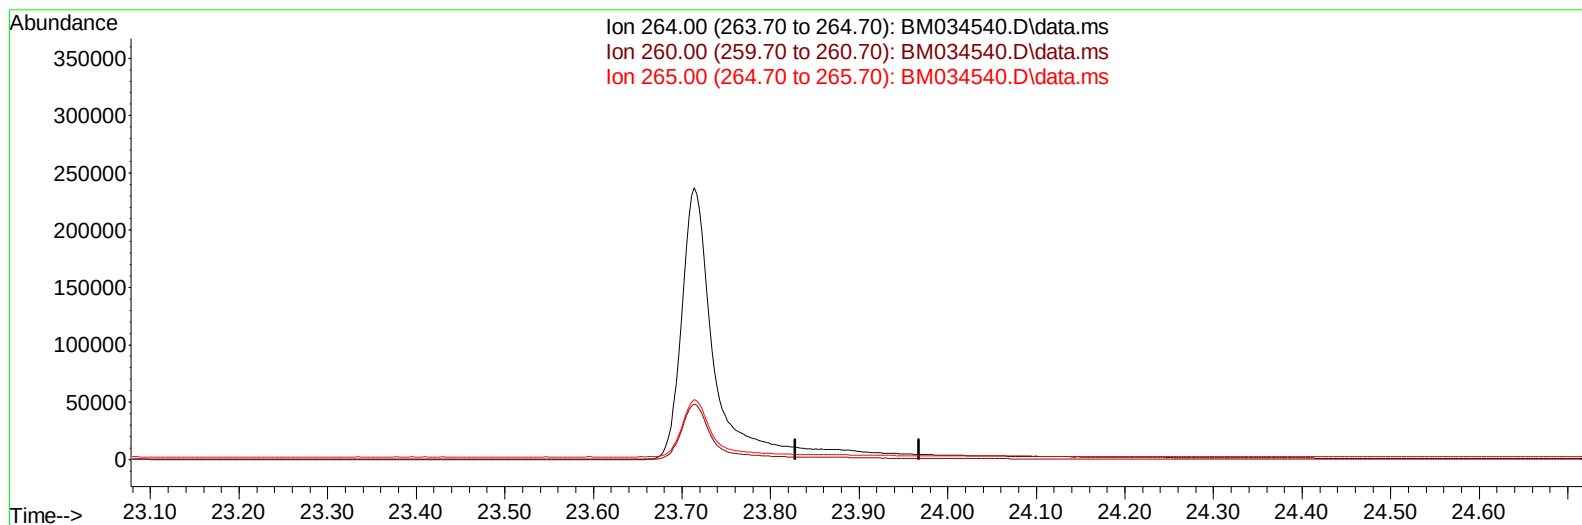

TIC: BM034540.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040722\
 Data File : BM034540.D
 Acq On : 07 Apr 2022 10:17
 Operator : CG/JU
 Sample : PB143886BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK886

Manual IntegrationsAPPROVED

Quant Time: Apr 08 04:56:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 07 12:11:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

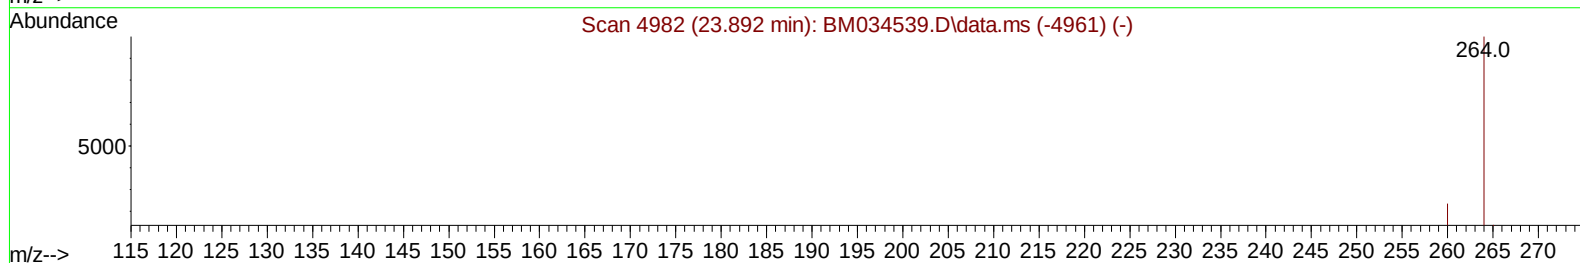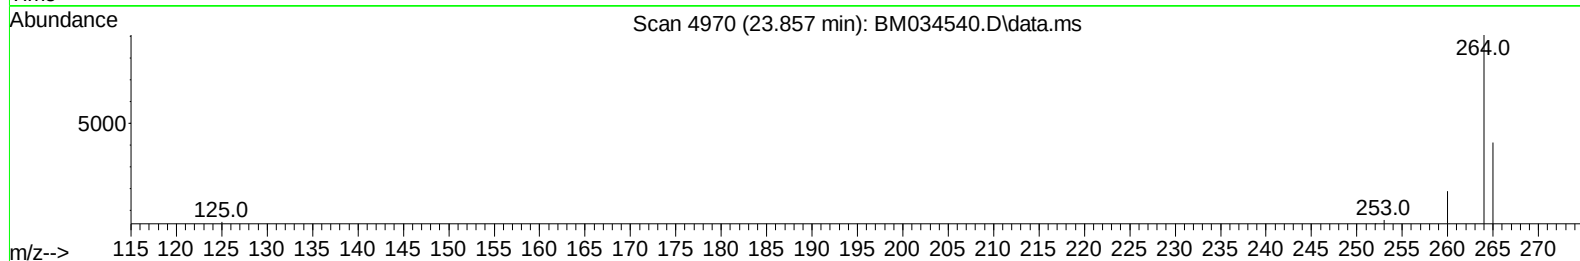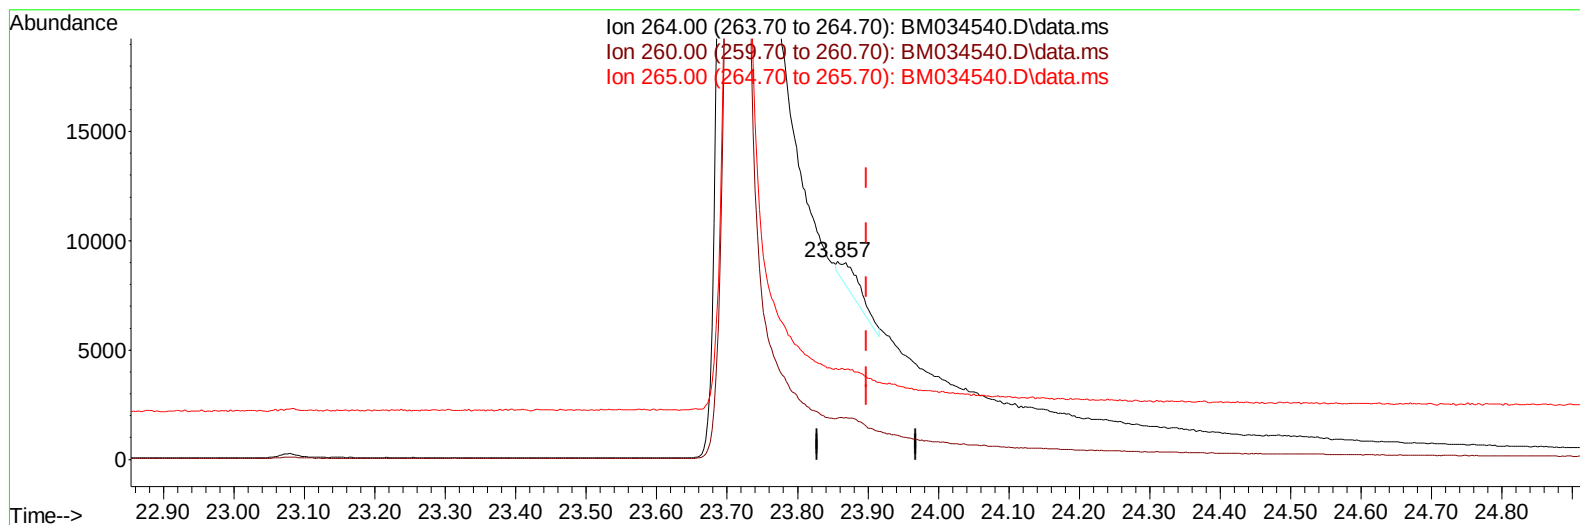

TIC: BM034540.D\data.ms

(23) Perylene-d12 (I)

23.857min (-0.041) 0.40 ng/ul m

response 2505

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	20.92#
265.00	95.30	45.42#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040722\
 Data File : BM034540.D
 Acq On : 07 Apr 2022 10:17
 Operator : CG/JU
 Sample : PB143886BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK886

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

Quant Time: Apr 08 04:56:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 07 12:11:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.912	152		3013	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.719	136		8078	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.551	164		4188	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.295	188		7260	0.400	ng/ul	-0.02
17) Chrysene-d12	21.516	240		4862	0.400	ng/ul	# 0.02
23) Perylene-d12	23.857	264		2505m	0.400	ng/ul	-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.292	96		25713	5.095	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152		3579	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.325	212		6366	0.446	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040722\
Data File : BM034540.D
Acq On : 07 Apr 2022 10:17
Operator : CG/JU
Sample : PB143886BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK886

Manual IntegrationsAPPROVED

Quant Time: Apr 08 04:56:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 07 12:11:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

