

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045028.D
 Acq On : 08 Apr 2024 04:07
 Operator : MA/JU
 Sample : P1970-19
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/09/2024
 Supervised By :mohammad ahmed 04/09/2024

Quant Time: Apr 08 05:24:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 08 05:01:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	82389	20.000	ng/u1	0.00
20) Naphthalene-d8	10.398	136	364075	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.274	164	238833	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.033	188	521485	20.000	ng/u1	-0.01
79) Chrysene-d12	21.239	240	487749	20.000	ng/u1	-0.01
88) Perylene-d12	23.456	264	583715	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	9879	4.478	ng/uL	0.00
4) Pyridine-d5	3.622	84	29119	4.853	ng/u1	0.01
7) Phenol-d5	6.810	99	44264	6.337	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	139788	33.592	ng/u1	0.00
11) 2-Chlorophenol-d4	7.163	132	147924	27.033	ng/u1	0.00
15) 4-Methylphenol-d8	8.339	113	87377	15.982	ng/u1	0.00
21) Nitrobenzene-d5	8.786	128	97394	34.826	ng/u1	0.00
24) 2-Nitrophenol-d4	9.498	143	104513	35.407	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	165830	30.642	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.557	131	192972	22.396	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	589375	35.442	ng/u1	-0.01
49) Acenaphthylene-d8	13.963	160	713999	36.344	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.539	143	14718m	4.241	ng/u1	0.02
60) Fluorene-d10	15.274	176	548849	37.021	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.415	200	73048	23.625	ng/u1	-0.01
73) Anthracene-d10	17.133	188	945478	40.303	ng/u1	0.00
81) Pyrene-d10	19.439	212	1097578	45.701	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.321	264	1143729	40.166	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.240	88	11318	4.912	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045028.D
Acq On : 08 Apr 2024 04:07
Operator : MA/JU
Sample : P1970-19
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AM3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/09/2024
Supervised By :mohammad ahmed 04/09/2024


Quant Time: Apr 08 05:24:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 08 05:01:54 2024
Response via : Initial Calibration

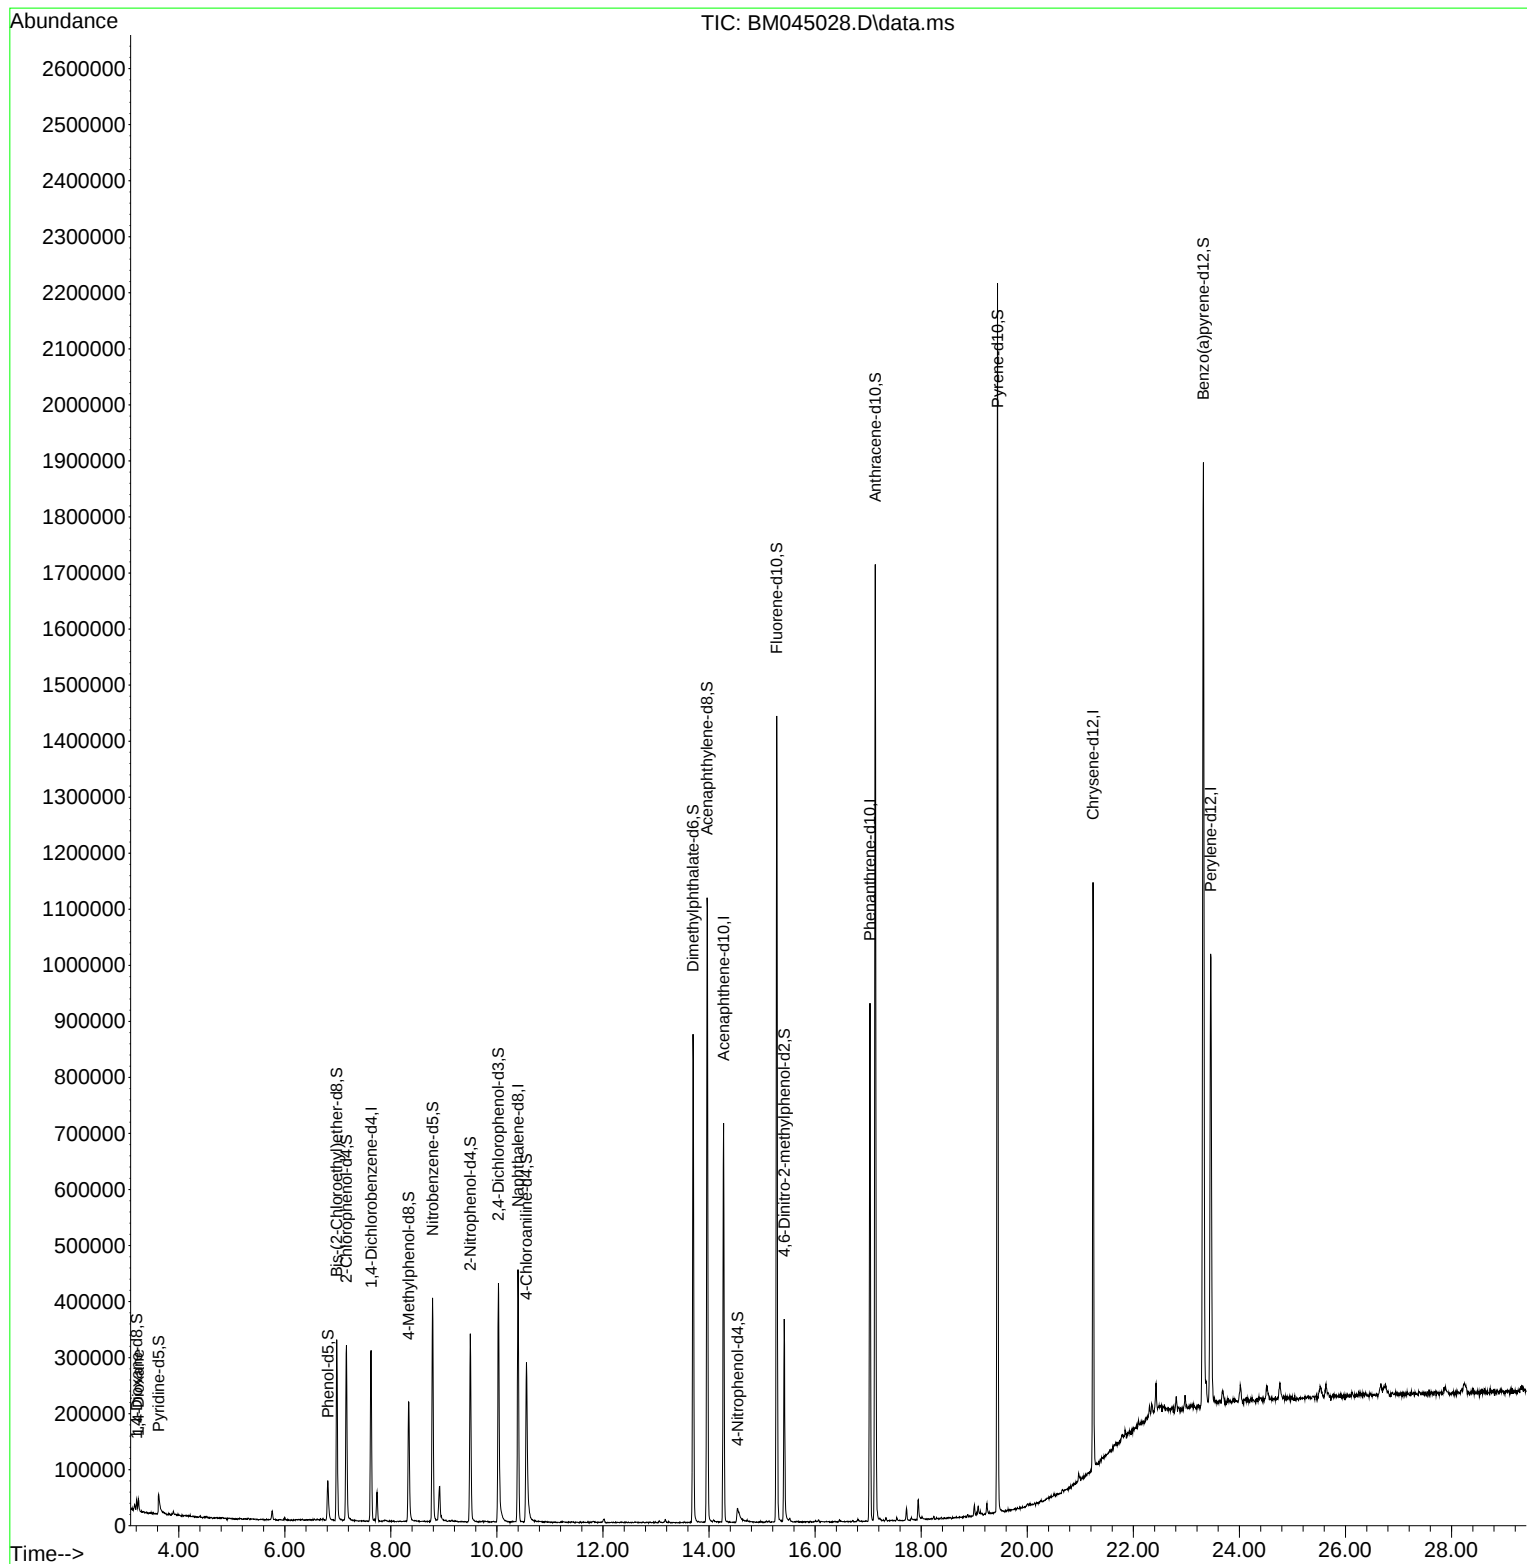

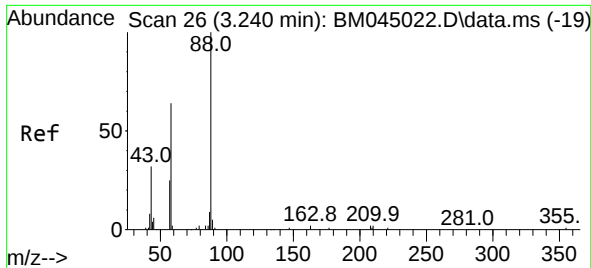

#2
 1,4-Dioxane
 Concen: 4.912 ng/uL
 RT: 3.240 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BM045028.D
 Acq: 08 Apr 2024 04:07

Instrument :
 BNA_M
 ClientSampleId :
 C0AM3

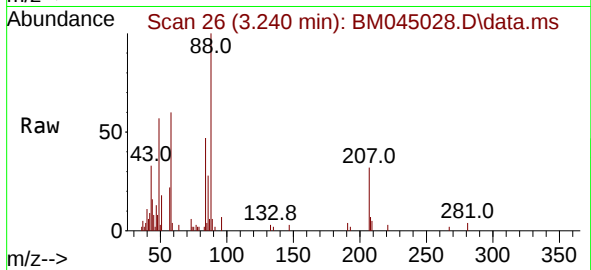

Tgt Ion: 88 Resp: 11318
 Ion Ratio Lower Upper
 88 100
 43 32.7 24.0 36.0
 58 59.8 45.4 68.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/09/2024
 Supervised By :mohammad ahmed 04/09/2024

