

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045006.D
 Acq On : 07 Apr 2024 14:19
 Operator : MA/JU
 Sample : PB160068BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	18	20	26	rVB	22067	28800	1.33%	0.129%
2	3.605	85	88	113	rBV	276516	485244	22.36%	2.176%
3	3.905	135	139	143	rBV6	3945	5761	0.27%	0.026%
4	4.016	156	158	160	rBV3	2967	3089	0.14%	0.014%
5	5.363	384	387	390	rBV5	1560	2501	0.12%	0.011%
6	5.434	397	399	402	rBV3	2221	3187	0.15%	0.014%
7	5.640	432	434	437	rVB4	2167	2286	0.11%	0.010%
8	6.810	627	633	646	rBV	353205	606167	27.93%	2.719%
9	6.981	654	662	674	rBV	281829	462126	21.30%	2.073%
10	7.163	686	693	709	rBV	382842	615245	28.35%	2.759%
11	7.628	764	772	780	rBV	296366	472302	21.77%	2.118%
12	7.710	785	786	790	rBV4	2106	2507	0.12%	0.011%
13	7.893	814	817	819	rBV4	1772	2421	0.11%	0.011%
14	8.340	886	893	910	rBV	437886	749079	34.52%	3.360%
15	8.716	953	957	960	rBV5	1382	2304	0.11%	0.010%
16	8.793	963	970	980	rBV	332465	570604	26.30%	2.559%
17	9.504	1084	1091	1102	rBV	296651	506012	23.32%	2.270%
18	10.034	1174	1181	1197	rBV	411427	764919	35.25%	3.431%
19	10.404	1235	1244	1253	rBV	404972	685600	31.60%	3.075%
20	10.557	1263	1270	1295	rBV	403799	880169	40.56%	3.948%
21	11.551	1434	1439	1441	rBV3	1777	2991	0.14%	0.013%
22	12.028	1516	1520	1526	rVB5	5095	9078	0.42%	0.041%
23	13.080	1692	1699	1701	rBV4	1785	2352	0.11%	0.011%
24	13.175	1711	1715	1720	rBV5	3776	6012	0.28%	0.027%
25	13.704	1799	1805	1817	rBV	702371	1032016	47.56%	4.629%
26	13.969	1842	1850	1863	rBV	921895	1372954	63.27%	6.158%
27	14.275	1896	1902	1911	rVV	602876	897412	41.36%	4.025%
28	14.516	1937	1943	1983	rBV	187854	529459	24.40%	2.375%
29	15.280	2066	2073	2084	rBV	1156555	1682545	77.54%	7.546%
30	15.421	2089	2097	2111	rBV	263820	408347	18.82%	1.831%
31	15.521	2111	2114	2122	rVB6	5674	7676	0.35%	0.034%
32	15.986	2189	2193	2199	rBV5	1860	3244	0.15%	0.015%
33	16.069	2204	2207	2210	rVV5	3649	4360	0.20%	0.020%
34	16.674	2307	2310	2313	rVB5	1502	2270	0.10%	0.010%
35	16.833	2333	2337	2339	rVB6	2321	2888	0.13%	0.013%
36	17.039	2365	2372	2382	rBV	724438	1058593	48.78%	4.748%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045006.D
 Acq On : 07 Apr 2024 14:19
 Operator : MA/JU
 Sample : PB160068BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	17.133	2382	2388	2404	rBV	1232380	1821269	83.93%	8.169%
38	17.468	2439	2445	2447	rVB7	1626	2658	0.12%	0.012%
39	17.910	2517	2520	2525	rBV7	1839	3111	0.14%	0.014%
40	18.115	2551	2555	2557	rBV4	2713	3104	0.14%	0.014%
41	18.174	2563	2565	2568	rBV3	1994	2408	0.11%	0.011%
42	18.410	2602	2605	2607	rBV4	1700	2375	0.11%	0.011%
43	18.862	2680	2682	2683	rBV	2750	2349	0.11%	0.011%
44	18.904	2687	2689	2691	rBV2	1964	2358	0.11%	0.011%
45	19.004	2702	2706	2711	rBV4	11860	17600	0.81%	0.079%
46	19.080	2714	2719	2722	rBV2	12126	18278	0.84%	0.082%
47	19.315	2756	2759	2761	rBV4	4114	5490	0.25%	0.025%
48	19.439	2775	2780	2789	rBV	1437957	2029608	93.53%	9.103%
49	21.245	3082	3087	3097	rBV	816569	1110620	51.18%	4.981%
50	23.321	3434	3440	3455	rVB2	1200011	2169922	100.00%	9.732%
51	23.462	3458	3464	3475	rVB	630175	1232369	56.79%	5.527%




Sum of corrected areas: 22296039

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045006.D
Acq On : 07 Apr 2024 14:19
Operator : MA/JU
Sample : PB160068BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

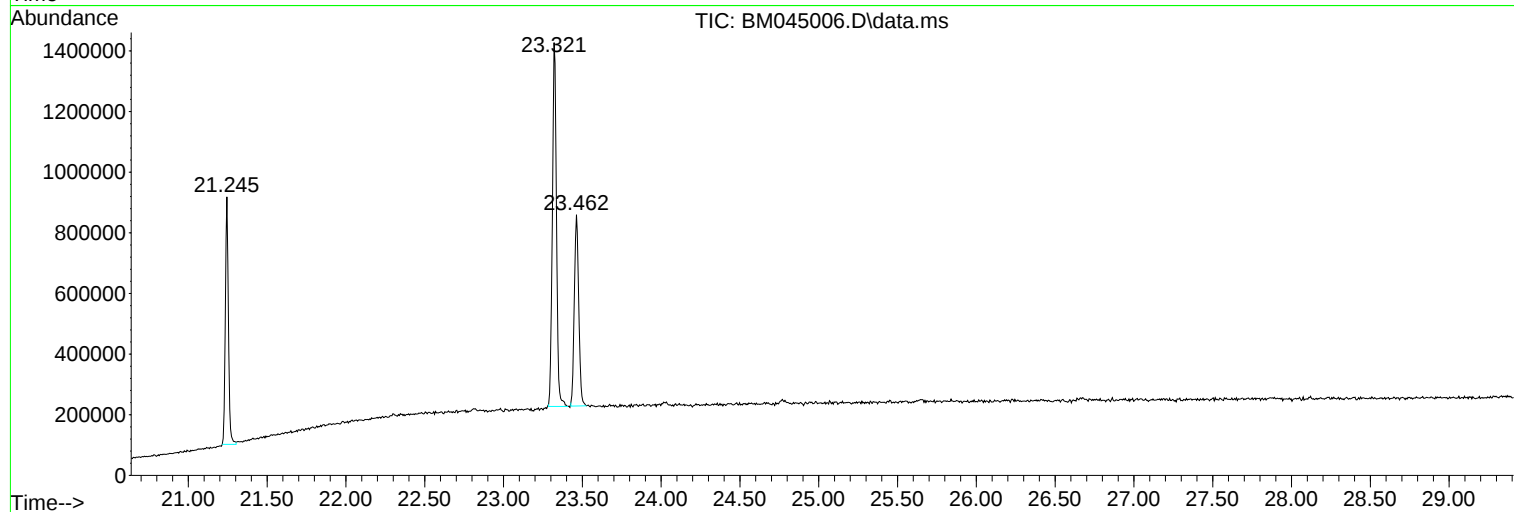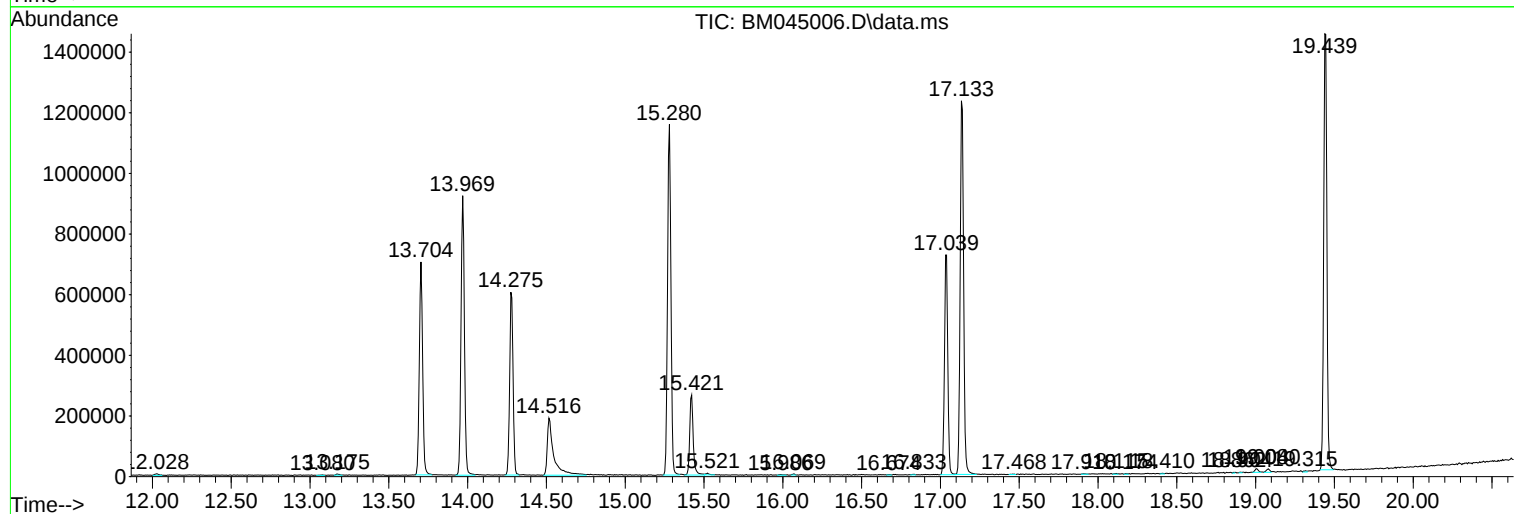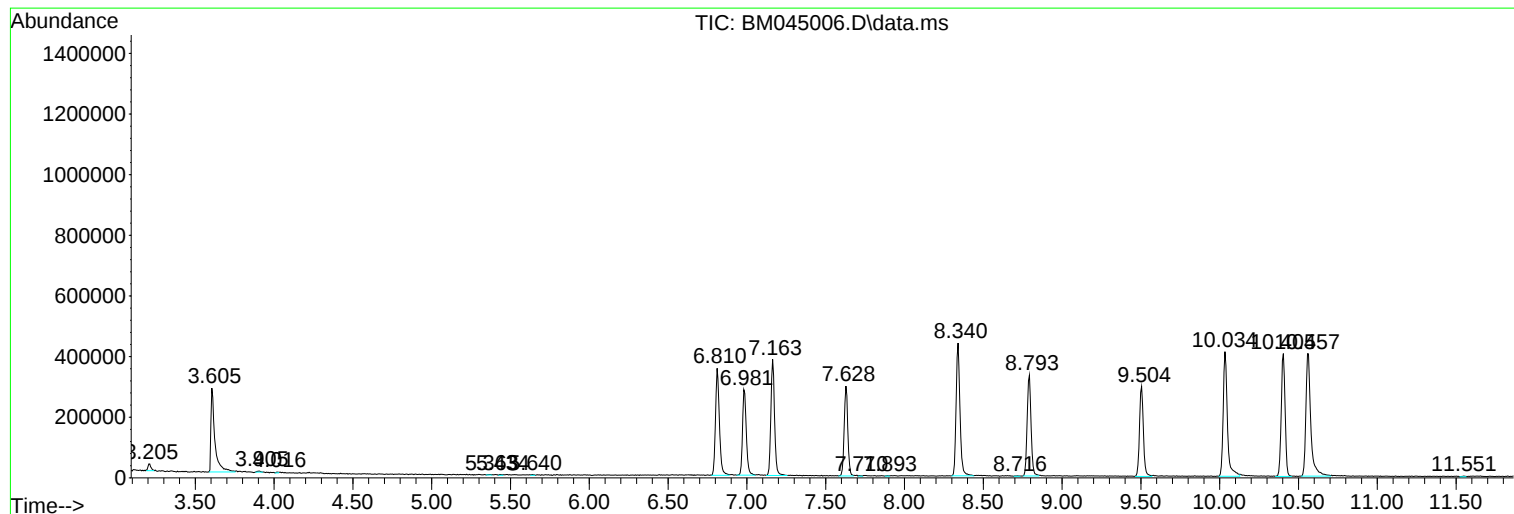

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045006.D
Acq On : 07 Apr 2024 14:19
Operator : MA/JU
Sample : PB160068BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045006.D
Acq On : 07 Apr 2024 14:19
Operator : MA/JU
Sample : PB160068BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------