

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045007.D
 Acq On : 07 Apr 2024 14:55
 Operator : MA/JU
 Sample : PB160062BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rVB	23296	32845	1.58%	0.145%
2	3.605	85	88	109	rBV	265559	460590	22.10%	2.034%
3	3.899	136	138	143	rVB4	5857	8120	0.39%	0.036%
4	4.387	219	221	224	rBV4	2301	3020	0.14%	0.013%
5	4.857	298	301	304	rVB5	1724	2298	0.11%	0.010%
6	5.963	487	489	492	rBV4	1681	2227	0.11%	0.010%
7	6.545	584	588	594	rBV8	1246	2545	0.12%	0.011%
8	6.810	626	633	645	rBV	338104	592504	28.43%	2.617%
9	6.981	656	662	675	rVB	279673	449872	21.59%	1.987%
10	7.163	686	693	704	rBV	374141	602527	28.91%	2.661%
11	7.628	765	772	780	rBV	337217	536091	25.72%	2.367%
12	8.339	886	893	905	rBV	431704	729781	35.02%	3.223%
13	8.792	960	970	980	rBV	328558	562937	27.01%	2.486%
14	9.134	1023	1028	1032	rBV7	1760	4068	0.20%	0.018%
15	9.204	1039	1040	1044	rBV3	2300	2490	0.12%	0.011%
16	9.504	1083	1091	1102	rBV	289336	487893	23.41%	2.155%
17	10.033	1172	1181	1199	rBV	395218	747576	35.87%	3.301%
18	10.404	1237	1244	1255	rVB	460033	768985	36.90%	3.396%
19	10.557	1263	1270	1290	rBV	398433	854276	40.99%	3.773%
20	10.716	1295	1297	1300	rVB4	1813	2278	0.11%	0.010%
21	12.027	1513	1520	1525	rBV5	5915	12578	0.60%	0.056%
22	12.086	1528	1530	1533	rVB3	2201	2096	0.10%	0.009%
23	13.174	1711	1715	1721	rVB8	3500	5471	0.26%	0.024%
24	13.704	1797	1805	1821	rBV	686844	1021505	49.02%	4.511%
25	13.969	1843	1850	1861	rBV	904904	1337835	64.20%	5.908%
26	14.274	1896	1902	1912	rVB	689283	1028391	49.35%	4.542%
27	14.516	1936	1943	1967	rBV	175252	488823	23.46%	2.159%
28	14.698	1972	1974	1980	rVB5	3886	5575	0.27%	0.025%
29	14.874	2000	2004	2006	rBV4	1598	2144	0.10%	0.009%
30	15.221	2059	2063	2065	rBV4	1838	2392	0.11%	0.011%
31	15.280	2066	2073	2086	rVV	1138166	1634433	78.43%	7.218%
32	15.421	2091	2097	2108	rVV	252733	394252	18.92%	1.741%
33	15.521	2111	2114	2121	rVB5	3983	7448	0.36%	0.033%
34	16.063	2202	2206	2210	rBV5	2861	3944	0.19%	0.017%
35	16.827	2331	2336	2338	rBV5	2185	2971	0.14%	0.013%
36	17.033	2364	2371	2381	rBV	846586	1214657	58.29%	5.364%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045007.D
Acq On : 07 Apr 2024 14:55
Operator : MA/JU
Sample : PB160062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.133	2382	2388	2402	rVB	1187684	1761415	84.52%	7.779%
38	17.368	2425	2428	2431	rVB4	2418	2426	0.12%	0.011%
39	17.562	2458	2461	2467	rBV6	1751	2514	0.12%	0.011%
40	17.633	2469	2473	2474	rBV4	1986	2818	0.14%	0.012%
41	18.515	2621	2623	2626	rBV3	2012	2488	0.12%	0.011%
42	18.780	2667	2668	2672	rBV4	1700	2217	0.11%	0.010%
43	19.004	2702	2706	2711	rVB2	12810	17883	0.86%	0.079%
44	19.074	2715	2718	2725	rBV2	10271	15715	0.75%	0.069%
45	19.186	2735	2737	2739	rBV3	2324	2101	0.10%	0.009%
46	19.439	2774	2780	2791	rBV	1439840	1992613	95.62%	8.800%
47	21.245	3081	3087	3097	rBV	940357	1297062	62.24%	5.728%
48	23.321	3434	3440	3447	rBV2	1153082	2083976	100.00%	9.203%
49	23.462	3458	3464	3477	rVB	776565	1443115	69.25%	6.373%


Sum of corrected areas: 22643781

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045007.D
Acq On : 07 Apr 2024 14:55
Operator : MA/JU
Sample : PB160062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

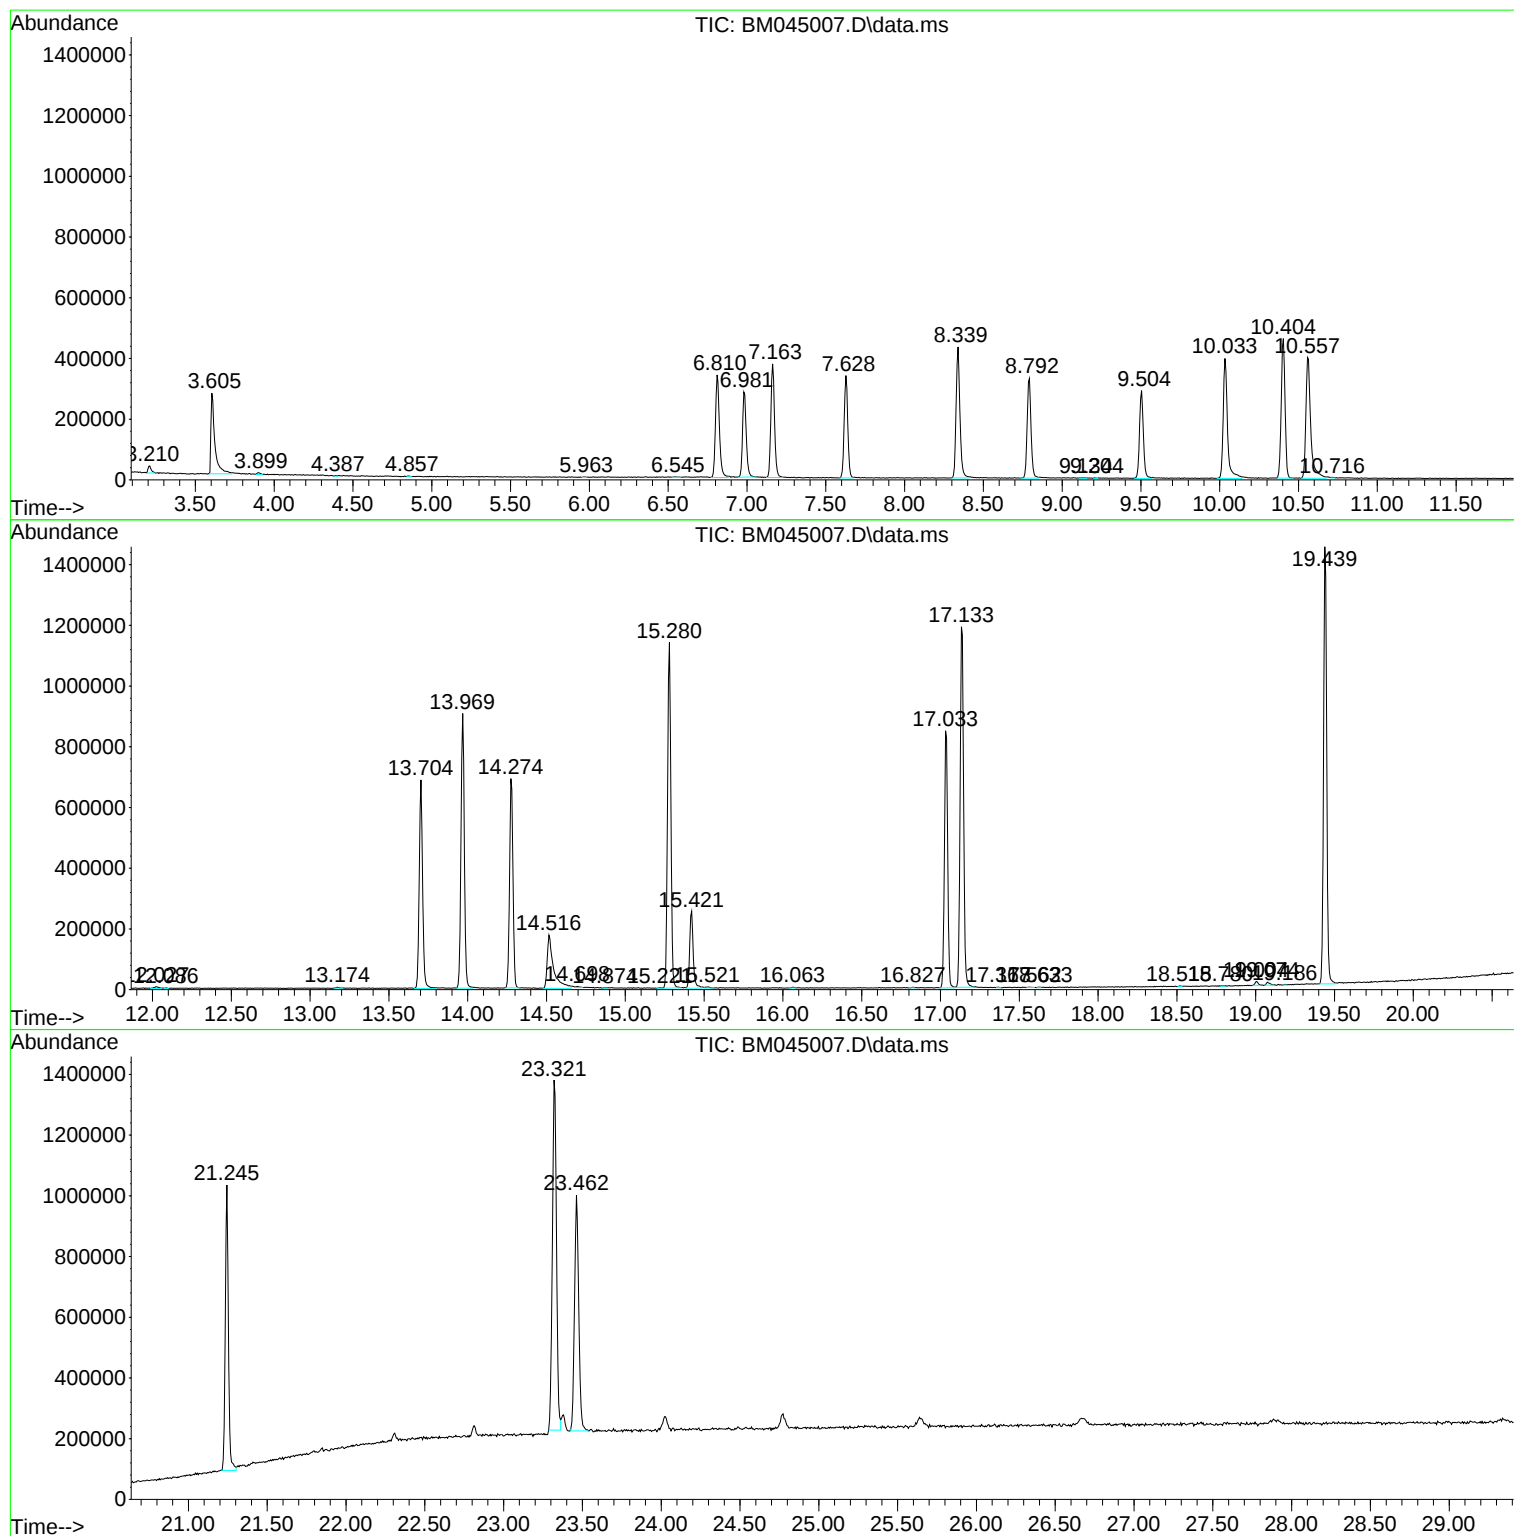

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045007.D
Acq On : 07 Apr 2024 14:55
Operator : MA/JU
Sample : PB160062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045007.D
Acq On : 07 Apr 2024 14:55
Operator : MA/JU
Sample : PB160062BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK062

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc