

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045012.D
 Acq On : 07 Apr 2024 17:55
 Operator : MA/JU
 Sample : P1982-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	27	rVB2	16660	23481	0.86%	0.108%
2	3.616	87	90	106	rBV	56964	111295	4.08%	0.514%
3	3.904	135	139	143	rVB4	7927	10991	0.40%	0.051%
4	4.993	321	324	332	rVB4	8294	13366	0.49%	0.062%
5	5.334	381	382	387	rBV4	1961	2901	0.11%	0.013%
6	5.651	434	436	440	rVB5	2974	2812	0.10%	0.013%
7	6.016	495	498	502	rBV6	1589	2942	0.11%	0.014%
8	6.093	507	511	514	rBV6	2214	3478	0.13%	0.016%
9	6.216	529	532	536	rBV6	2155	2963	0.11%	0.014%
10	6.816	626	634	644	rBV2	76386	156962	5.75%	0.725%
11	6.981	655	662	672	rBV	300793	485328	17.77%	2.241%
12	7.163	686	693	704	rBV	299228	493247	18.06%	2.278%
13	7.628	765	772	782	rBV	263813	429711	15.73%	1.984%
14	7.975	828	831	836	rVB6	3790	4699	0.17%	0.022%
15	8.339	886	893	904	rBV	212248	383803	14.05%	1.772%
16	8.592	933	936	942	rBV6	1736	3497	0.13%	0.016%
17	8.792	962	970	979	rBV	351015	602033	22.04%	2.780%
18	8.951	990	997	1002	rVB8	7317	12252	0.45%	0.057%
19	9.157	1028	1032	1037	rVB6	1913	2841	0.10%	0.013%
20	9.504	1082	1091	1105	rBV	287874	499341	18.28%	2.306%
21	10.033	1174	1181	1195	rBV	379776	714880	26.18%	3.301%
22	10.157	1201	1202	1208	rVB5	2808	3132	0.11%	0.014%
23	10.404	1236	1244	1252	rVB	354990	602279	22.05%	2.781%
24	10.557	1263	1270	1290	rBV	307242	686087	25.12%	3.168%
25	12.016	1512	1518	1523	rBV3	4753	10051	0.37%	0.046%
26	13.174	1712	1715	1720	rVB3	4308	6231	0.23%	0.029%
27	13.704	1798	1805	1818	rBV	782426	1115795	40.86%	5.152%
28	13.969	1843	1850	1860	rBV	975091	1433427	52.49%	6.619%
29	14.274	1896	1902	1909	rBV	527502	779082	28.53%	3.597%
30	14.539	1941	1947	1951	rBV4	20563	43754	1.60%	0.202%
31	15.280	2066	2073	2083	rBV	1291003	1884110	68.99%	8.700%
32	15.421	2091	2097	2110	rBV	317093	476285	17.44%	2.199%
33	15.521	2112	2114	2118	rVB4	5796	6117	0.22%	0.028%
34	16.068	2203	2207	2211	rVB5	4307	7054	0.26%	0.033%
35	16.862	2339	2342	2344	rVV3	2141	2748	0.10%	0.013%
36	17.033	2365	2371	2382	rBV	625581	918603	33.64%	4.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045012.D
Acq On : 07 Apr 2024 17:55
Operator : MA/JU
Sample : P1982-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSQ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.133	2382	2388	2404	rBV	1516387	2229624	81.64%	10.295%
38	17.804	2498	2502	2505	rBV4	2562	3109	0.11%	0.014%
39	17.951	2524	2527	2534	rBV8	10924	17099	0.63%	0.079%
40	19.003	2701	2706	2712	rVB5	15682	24667	0.90%	0.114%
41	19.080	2715	2719	2723	rBV3	13800	18678	0.68%	0.086%
42	19.245	2744	2747	2752	rVB7	9423	13793	0.51%	0.064%
43	19.445	2774	2781	2789	rBV	1851686	2584830	94.65%	11.935%
44	19.715	2825	2827	2829	rVB4	4198	3130	0.11%	0.014%
45	21.245	3082	3087	3094	rBV2	727587	975806	35.73%	4.506%
46	23.321	3434	3440	3448	rBV2	1515116	2730972	100.00%	12.610%
47	23.462	3458	3464	3476	rVB	566344	1117860	40.93%	5.162%




Sum of corrected areas: 21657146

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045012.D
Acq On : 07 Apr 2024 17:55
Operator : MA/JU
Sample : P1982-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

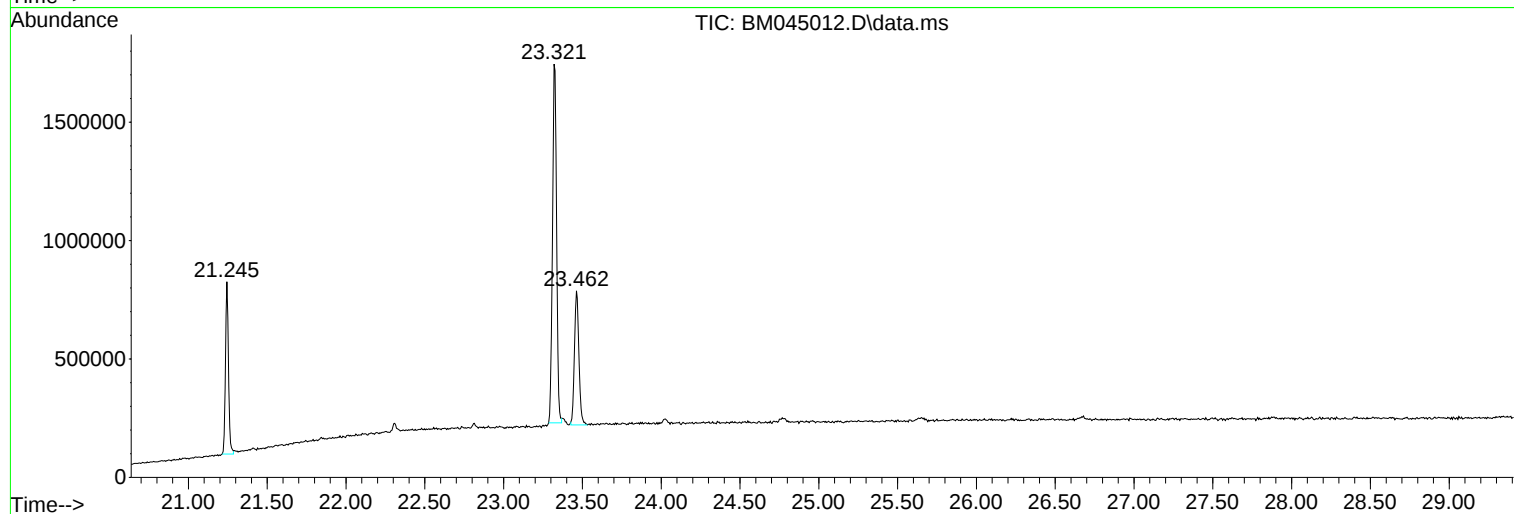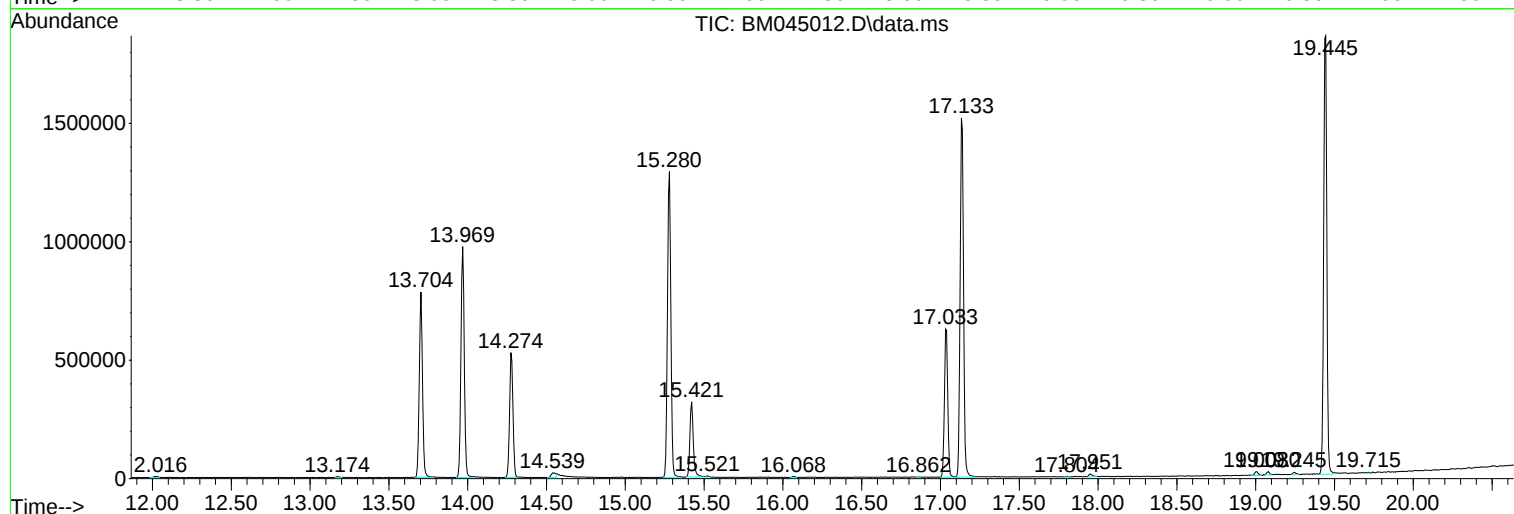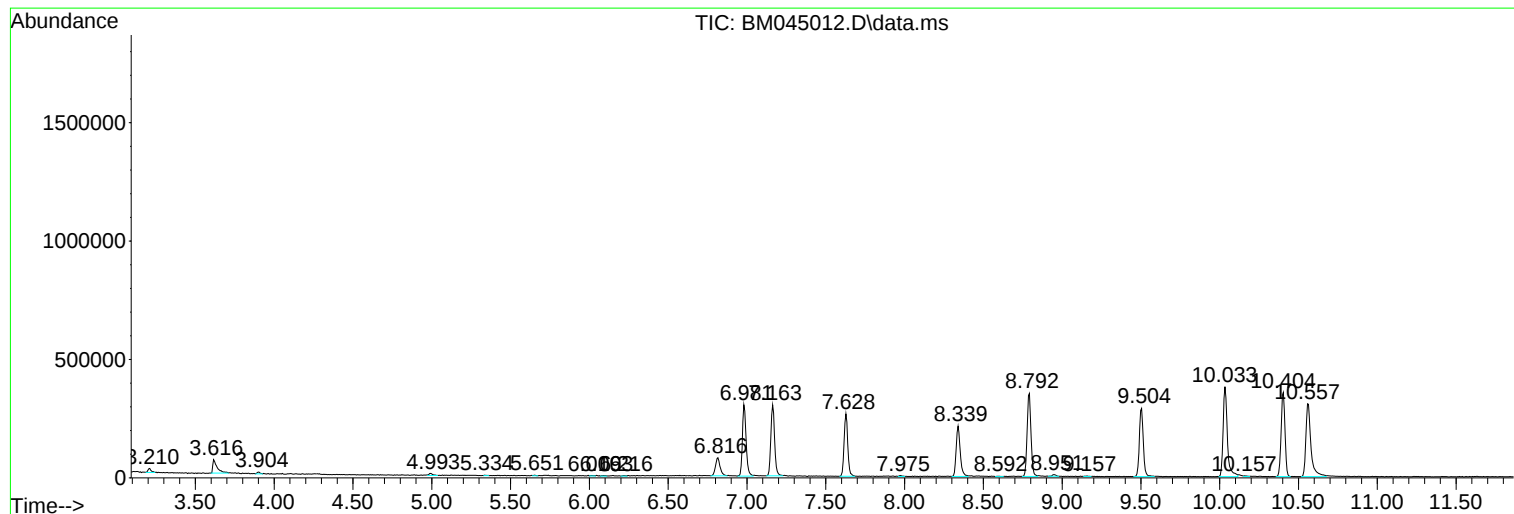

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045012.D
Acq On : 07 Apr 2024 17:55
Operator : MA/JU
Sample : P1982-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045012.D
Acq On : 07 Apr 2024 17:55
Operator : MA/JU
Sample : P1982-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc