

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045014.D
 Acq On : 07 Apr 2024 19:07
 Operator : MA/JU
 Sample : P1970-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	18	rBV	42332	56372	1.99%	0.243%
2	3.205	18	20	22	rVV2	16360	17581	0.62%	0.076%
3	3.240	22	26	36	rVB	83143	113753	4.02%	0.491%
4	3.628	89	92	110	rBV	17688	46090	1.63%	0.199%
5	3.905	135	139	147	rVB6	6852	12304	0.43%	0.053%
6	4.399	219	223	228	rVB5	13367	20501	0.72%	0.088%
7	4.616	258	260	264	rBV4	2842	4217	0.15%	0.018%
8	6.246	534	537	540	rBV5	2750	3872	0.14%	0.017%
9	6.816	628	634	643	rBV	51257	101306	3.58%	0.437%
10	6.981	656	662	675	rBV	273758	453501	16.02%	1.956%
11	7.163	687	693	704	rBV	262401	434910	15.37%	1.876%
12	7.628	765	772	781	rBV	344561	556020	19.65%	2.398%
13	7.745	787	792	795	rVB5	3347	5386	0.19%	0.023%
14	8.340	887	893	903	rBV2	177001	311625	11.01%	1.344%
15	8.792	963	970	982	rBV	325762	566764	20.03%	2.444%
16	9.151	1026	1031	1035	rBV4	3929	6629	0.23%	0.029%
17	9.504	1084	1091	1099	rBV	260550	460241	16.26%	1.985%
18	10.034	1173	1181	1197	rBV	328592	647319	22.87%	2.792%
19	10.404	1236	1244	1252	rBV	473162	808340	28.56%	3.486%
20	10.563	1264	1271	1291	rBV	214778	492110	17.39%	2.122%
21	11.645	1450	1455	1459	rBV6	2700	4426	0.16%	0.019%
22	12.016	1510	1518	1524	rBV4	4617	9869	0.35%	0.043%
23	13.175	1711	1715	1719	rBV4	7591	12434	0.44%	0.054%
24	13.704	1797	1805	1820	rBV	741138	1084173	38.31%	4.675%
25	13.969	1843	1850	1860	rBV	922016	1380582	48.78%	5.954%
26	14.274	1896	1902	1913	rBV	721858	1074154	37.96%	4.632%
27	14.545	1942	1948	1961	rBV4	17445	66822	2.36%	0.288%
28	15.280	2064	2073	2085	rBV	1185852	1795621	63.45%	7.743%
29	15.421	2090	2097	2108	rVV	339709	521223	18.42%	2.248%
30	15.527	2111	2115	2118	rVB5	5176	7117	0.25%	0.031%
31	16.068	2204	2207	2214	rVB5	3745	6225	0.22%	0.027%
32	16.821	2332	2335	2339	rBV4	3505	4478	0.16%	0.019%
33	17.033	2365	2371	2382	rBV	870504	1274790	45.04%	5.497%
34	17.133	2382	2388	2400	rVV	1527290	2272850	80.31%	9.801%
35	17.415	2431	2436	2438	rBV4	2905	4236	0.15%	0.018%
36	17.821	2503	2505	2508	rVV4	2894	2839	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045014.D
Acq On : 07 Apr 2024 19:07
Operator : MA/JU
Sample : P1970-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.945	2521	2526	2532	rBV2	31311	46069	1.63%	0.199%
38	19.004	2702	2706	2711	rVB2	19838	25255	0.89%	0.109%
39	19.080	2714	2719	2723	rBV	16131	24576	0.87%	0.106%
40	19.115	2723	2725	2728	rVB3	4514	4296	0.15%	0.019%
41	19.239	2742	2746	2751	rBV6	16729	22812	0.81%	0.098%
42	19.439	2774	2780	2790	rBV	1986772	2691951	95.12%	11.609%
43	21.245	3082	3087	3095	rBV	1045869	1374355	48.56%	5.927%
44	23.327	3434	3441	3448	rBV2	1559250	2830044	100.00%	12.204%
45	23.462	3458	3464	3475	rVB	798168	1528832	54.02%	6.593%




Sum of corrected areas: 23188870

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045014.D
Acq On : 07 Apr 2024 19:07
Operator : MA/JU
Sample : P1970-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

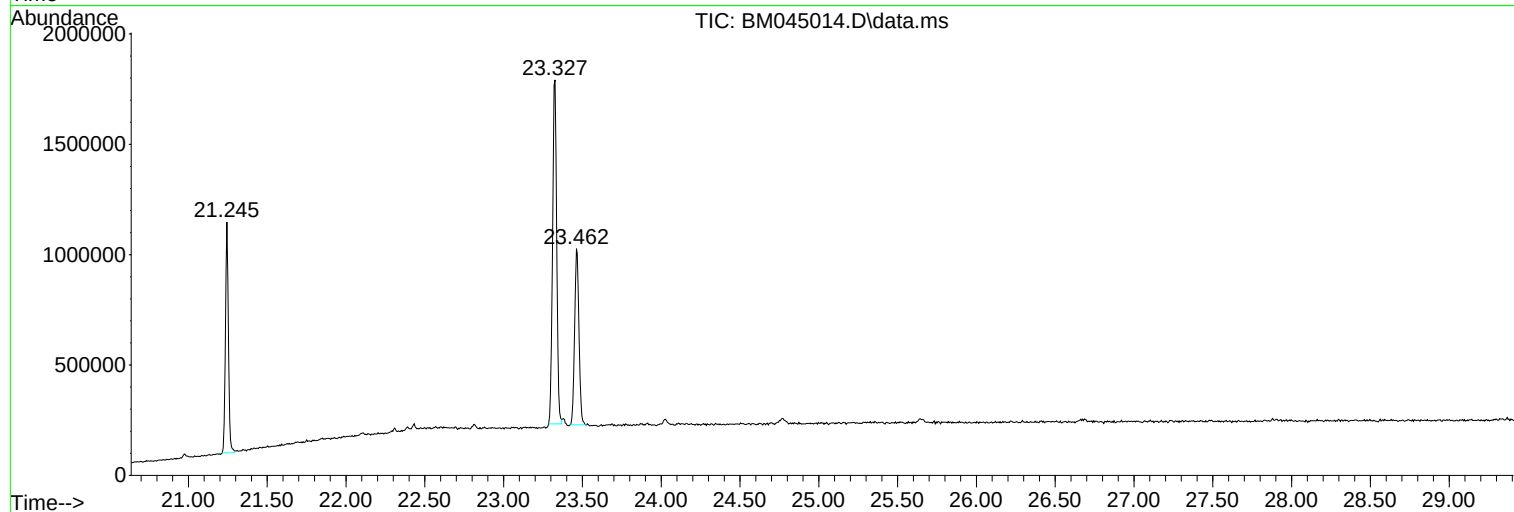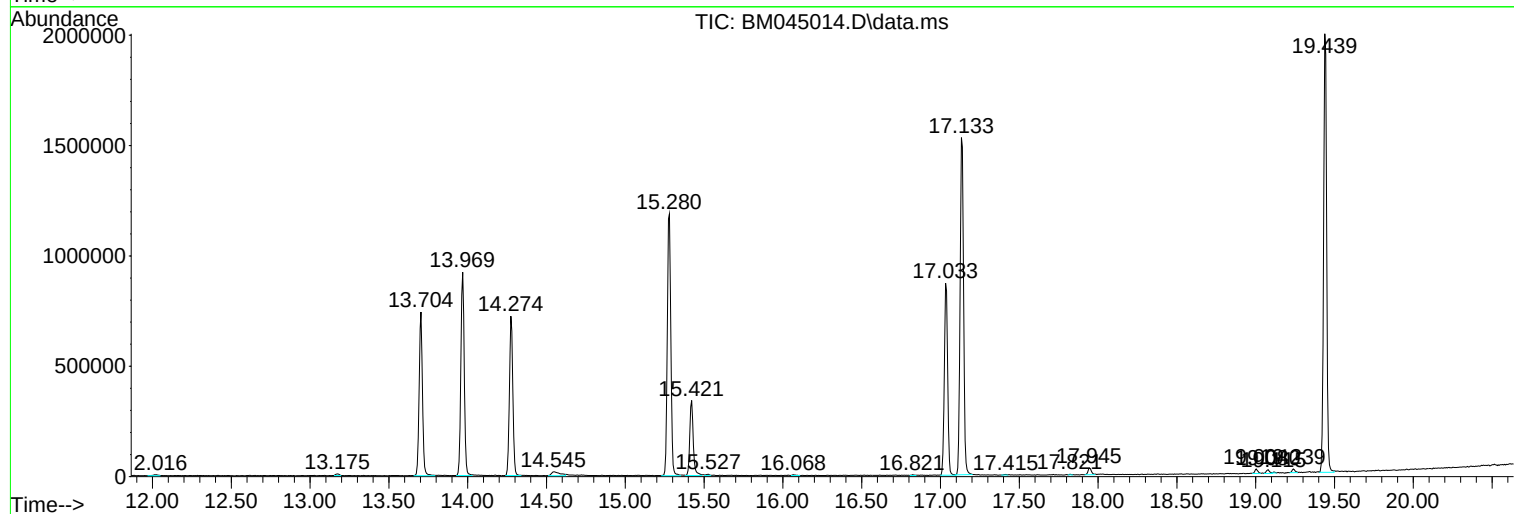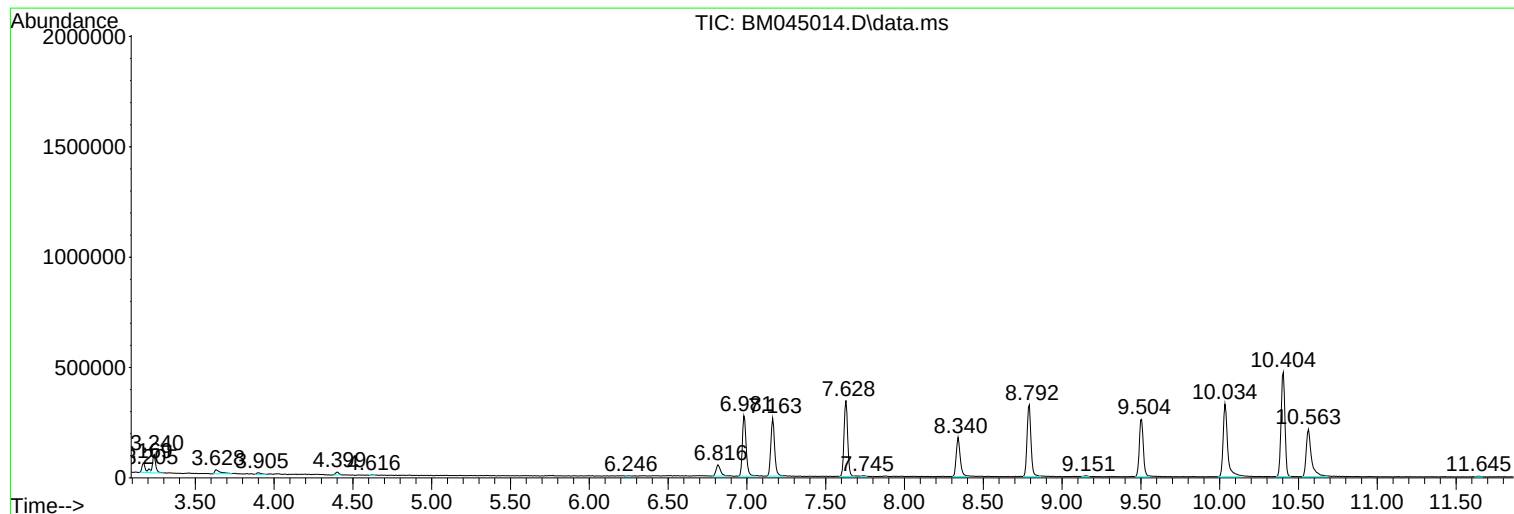

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045014.D
Acq On : 07 Apr 2024 19:07
Operator : MA/JU
Sample : P1970-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045014.D
Acq On : 07 Apr 2024 19:07
Operator : MA/JU
Sample : P1970-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc