

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045015.D
 Acq On : 07 Apr 2024 19:43
 Operator : MA/JU
 Sample : P1970-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	18	rBV	76213	104667	4.10%	0.477%
2	3.205	18	20	22	rVV	19387	22712	0.89%	0.104%
3	3.240	22	26	39	rVB	125062	180957	7.08%	0.825%
4	3.616	87	90	102	rBV	50881	105230	4.12%	0.480%
5	3.905	137	139	142	rVB4	6609	6090	0.24%	0.028%
6	4.399	219	223	228	rVB5	10736	17119	0.67%	0.078%
7	4.687	268	272	275	rBV6	1492	2633	0.10%	0.012%
8	5.769	451	456	459	rVB5	3659	6089	0.24%	0.028%
9	6.816	628	634	645	rVB	54597	106887	4.18%	0.488%
10	6.981	656	662	674	rBV	277490	454095	17.77%	2.071%
11	7.098	680	682	685	rVB4	2697	2800	0.11%	0.013%
12	7.163	685	693	703	rBV	258018	442774	17.33%	2.020%
13	7.628	765	772	781	rVV	295272	475304	18.60%	2.168%
14	7.693	781	783	787	rVV4	3262	4049	0.16%	0.018%
15	7.740	787	791	798	rVB3	11991	18866	0.74%	0.086%
16	7.875	812	814	818	rVB3	3046	3137	0.12%	0.014%
17	8.340	886	893	902	rVV	178174	316195	12.37%	1.442%
18	8.398	902	903	909	rVV5	5169	8150	0.32%	0.037%
19	8.469	912	915	918	rVB4	2477	2660	0.10%	0.012%
20	8.787	962	969	979	rBV	323563	566853	22.18%	2.586%
21	9.151	1028	1031	1034	rVB4	2339	3380	0.13%	0.015%
22	9.504	1083	1091	1100	rBV	259631	448814	17.56%	2.047%
23	9.910	1158	1160	1166	rVB5	3463	4661	0.18%	0.021%
24	9.957	1166	1168	1172	rVB4	1970	2600	0.10%	0.012%
25	10.034	1172	1181	1203	rBV	342359	665974	26.06%	3.038%
26	10.398	1236	1243	1253	rVB	395087	679430	26.59%	3.099%
27	10.563	1264	1271	1290	rBV	281730	615018	24.07%	2.805%
28	10.798	1306	1311	1313	rBV6	1848	2872	0.11%	0.013%
29	11.216	1378	1382	1383	rBV3	3282	3862	0.15%	0.018%
30	11.281	1388	1393	1398	rVB7	5717	12384	0.48%	0.056%
31	11.639	1449	1454	1456	rBV3	2548	2971	0.12%	0.014%
32	11.880	1494	1495	1501	rVB6	2055	2684	0.11%	0.012%
33	12.010	1514	1517	1524	rVB5	5924	11202	0.44%	0.051%
34	12.204	1546	1550	1556	rVB5	3741	5507	0.22%	0.025%
35	12.498	1593	1600	1603	rBV7	4788	9361	0.37%	0.043%
36	13.075	1694	1698	1702	rBV6	2546	4651	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045015.D
 Acq On : 07 Apr 2024 19:43
 Operator : MA/JU
 Sample : P1970-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.175	1708	1715	1720	rBV2	8592	15169	0.59%	0.069%
38	13.704	1794	1805	1817	rBV	730933	1060766	41.51%	4.839%
39	13.786	1817	1819	1824	rVB6	3830	5370	0.21%	0.024%
40	13.969	1843	1850	1860	rBV	916902	1367844	53.53%	6.239%
41	14.274	1895	1902	1912	rVV	625938	906795	35.49%	4.136%
42	14.445	1929	1931	1936	rVB5	2280	3030	0.12%	0.014%
43	14.545	1942	1948	1959	rBV4	17535	58233	2.28%	0.266%
44	14.992	2019	2024	2032	rVB7	1695	3802	0.15%	0.017%
45	15.086	2036	2040	2043	rBV5	1930	2756	0.11%	0.013%
46	15.280	2066	2073	2086	rBV	1164790	1727148	67.59%	7.878%
47	15.421	2091	2097	2110	rBV	288419	451358	17.66%	2.059%
48	15.521	2110	2114	2116	rVB5	4189	5822	0.23%	0.027%
49	16.068	2202	2207	2210	rVB6	4088	5825	0.23%	0.027%
50	16.115	2210	2215	2219	rBV6	1619	3307	0.13%	0.015%
51	16.186	2225	2227	2232	rVB4	2123	3347	0.13%	0.015%
52	16.457	2270	2273	2277	rBV5	5085	7148	0.28%	0.033%
53	17.033	2366	2371	2380	rVV	749693	1056074	41.33%	4.817%
54	17.133	2382	2388	2401	rVV	1409229	2058377	80.55%	9.389%
55	17.227	2401	2404	2410	rVB8	4982	8634	0.34%	0.039%
56	17.398	2430	2433	2436	rBV4	1872	2770	0.11%	0.013%
57	17.439	2436	2440	2444	rVV6	3343	6127	0.24%	0.028%
58	17.821	2502	2505	2508	rBV4	6322	6307	0.25%	0.029%
59	17.945	2521	2526	2535	rBV3	57826	88741	3.47%	0.405%
60	18.015	2535	2538	2542	rVV5	3850	6178	0.24%	0.028%
61	18.315	2586	2589	2593	rVV5	2299	3610	0.14%	0.016%
62	18.380	2596	2600	2603	rVB6	6814	8239	0.32%	0.038%
63	18.745	2660	2662	2667	rBV5	1982	3535	0.14%	0.016%
64	19.004	2701	2706	2711	rVB5	18364	26443	1.03%	0.121%
65	19.074	2711	2718	2723	rBV2	16071	29791	1.17%	0.136%
66	19.115	2723	2725	2730	rVB5	6730	10071	0.39%	0.046%
67	19.239	2742	2746	2753	rBV7	21422	33644	1.32%	0.153%
68	19.439	2774	2780	2787	rBV	1724170	2411896	94.38%	11.001%
69	20.974	3038	3041	3046	rBV4	25168	32417	1.27%	0.148%
70	21.245	3082	3087	3094	rBV	884132	1171904	45.86%	5.345%
71	22.103	3230	3233	3237	rVB3	54956	65036	2.55%	0.297%
72	22.433	3286	3289	3294	rVB	79787	99220	3.88%	0.453%
73	23.327	3434	3441	3448	rBV	1393934	2555419	100.00%	11.656%
74	23.462	3458	3464	3475	rVB	667405	1288580	50.43%	5.878%

Sum of corrected areas: 21923371

Instrument :

BNA_M

ClientSampleId :




C0AK4

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045015.D
Acq On : 07 Apr 2024 19:43
Operator : MA/JU
Sample : P1970-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

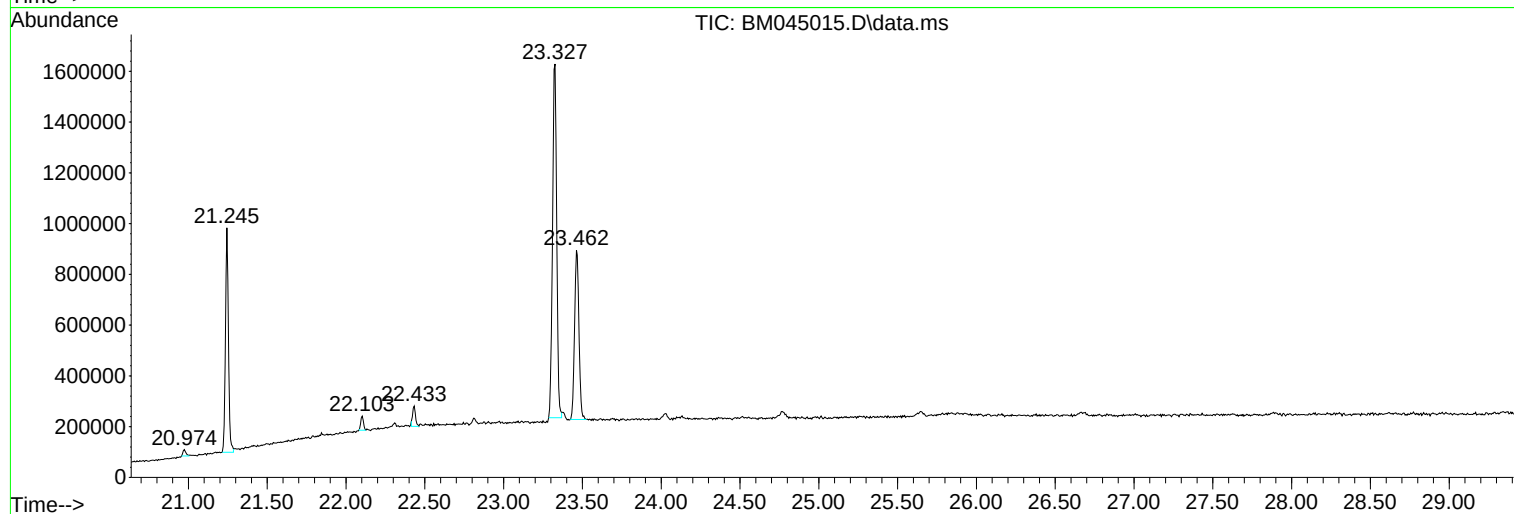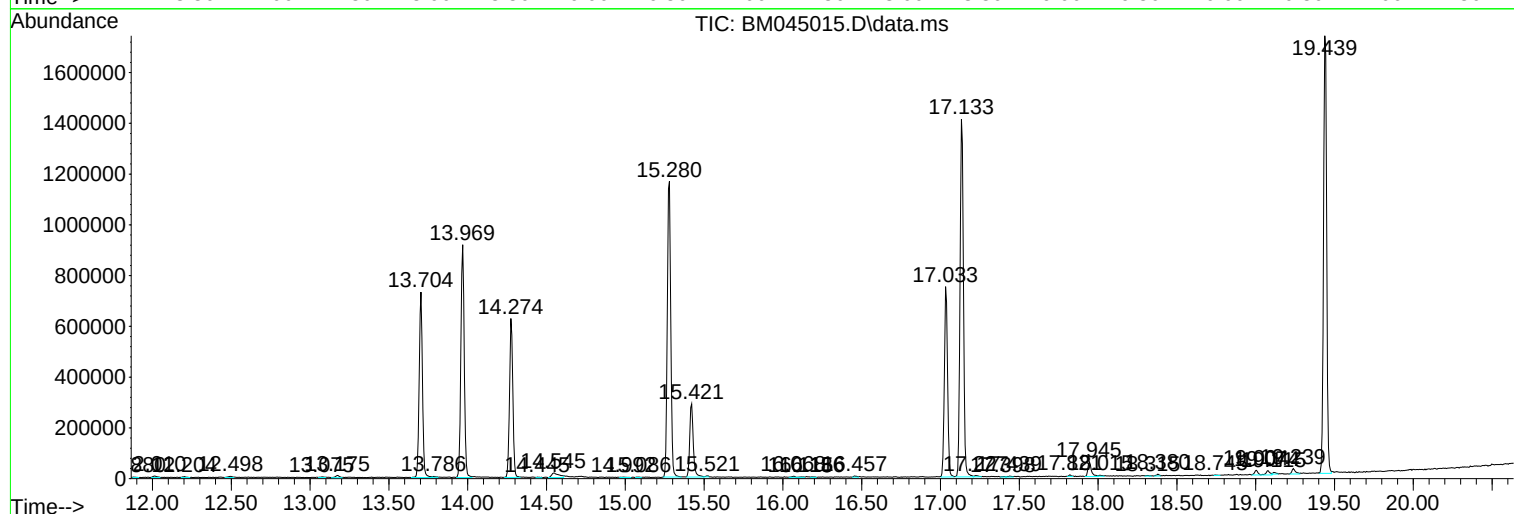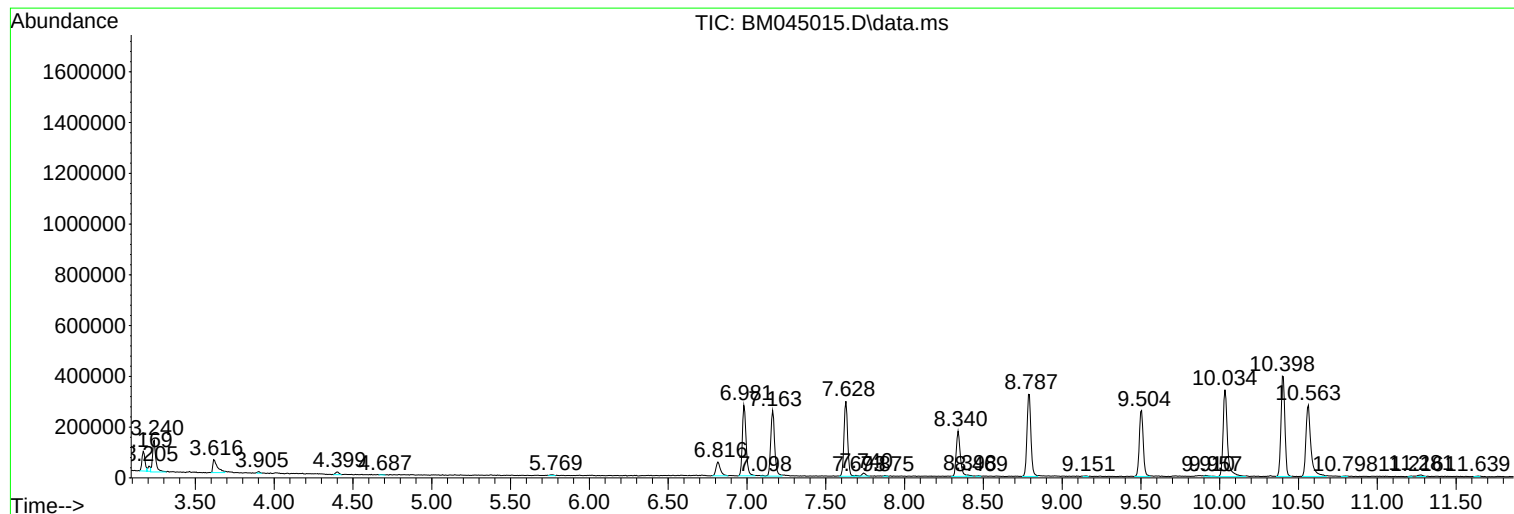

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045015.D
Acq On : 07 Apr 2024 19:43
Operator : MA/JU
Sample : P1970-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045015.D
Acq On : 07 Apr 2024 19:43
Operator : MA/JU
Sample : P1970-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc