

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045023.D
 Acq On : 08 Apr 2024 01:07
 Operator : MA/JU
 Sample : PB160066BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	29	rVB	29352	38342	1.53%	0.149%
2	3.605	84	88	107	rBV	336188	579110	23.15%	2.250%
3	3.899	135	138	143	rVB3	5312	7400	0.30%	0.029%
4	5.346	382	384	387	rBV3	2496	3715	0.15%	0.014%
5	5.646	432	435	436	rBV3	2724	2645	0.11%	0.010%
6	5.822	462	465	468	rBV4	1673	2536	0.10%	0.010%
7	6.810	627	633	644	rBV	416116	709325	28.36%	2.756%
8	6.981	656	662	674	rVB	344802	541057	21.63%	2.103%
9	7.163	685	693	706	rBV	444290	733704	29.33%	2.851%
10	7.275	709	712	715	rVB5	2011	2713	0.11%	0.011%
11	7.628	765	772	783	rBV	320772	527904	21.10%	2.051%
12	8.334	885	892	907	rBV	514126	887712	35.49%	3.450%
13	8.787	962	969	982	rBV	409683	685631	27.41%	2.664%
14	9.498	1084	1090	1099	rBV	346224	590065	23.59%	2.293%
15	9.628	1107	1112	1113	rVB3	2002	2558	0.10%	0.010%
16	10.034	1173	1181	1203	rBV	468398	917941	36.69%	3.567%
17	10.398	1236	1243	1252	rVB	461437	759734	30.37%	2.952%
18	10.557	1261	1270	1285	rBV	426676	891111	35.62%	3.463%
19	12.022	1515	1519	1527	rVV4	5384	9126	0.36%	0.035%
20	13.180	1710	1716	1719	rBV5	4885	7617	0.30%	0.030%
21	13.645	1792	1795	1798	rBV5	2057	3016	0.12%	0.012%
22	13.704	1798	1805	1817	rBV	813119	1223970	48.93%	4.756%
23	13.969	1842	1850	1862	rBV	1045882	1605735	64.19%	6.240%
24	14.274	1895	1902	1911	rBV	688354	1012105	40.46%	3.933%
25	14.510	1936	1942	1966	rBV	221597	588979	23.54%	2.289%
26	15.274	2065	2072	2084	rBV	1327935	1970765	78.78%	7.658%
27	15.416	2090	2096	2109	rBV	308603	478749	19.14%	1.860%
28	15.521	2109	2114	2118	rVB7	4914	8409	0.34%	0.033%
29	15.645	2132	2135	2138	rBV5	1665	2518	0.10%	0.010%
30	16.068	2202	2207	2210	rVB6	2966	4979	0.20%	0.019%
31	17.033	2365	2371	2381	rBV	872255	1198620	47.91%	4.658%
32	17.133	2381	2388	2402	rVV2	1460466	2109588	84.33%	8.198%
33	17.474	2443	2446	2451	rBV5	1694	3098	0.12%	0.012%
34	19.004	2701	2706	2712	rBV4	15793	26404	1.06%	0.103%
35	19.074	2714	2718	2724	rVV3	14022	21750	0.87%	0.085%
36	19.121	2724	2726	2731	rVB6	2475	3904	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045023.D
Acq On : 08 Apr 2024 01:07
Operator : MA/JU
Sample : PB160066BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK066

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	19.439	2774	2780	2794	rBV	1780273	2415176	96.55%	9.385%
38	21.239	3081	3086	3099	rBV	878824	1275927	51.00%	4.958%
39	23.321	3433	3440	3447	rBV	1356991	2501573	100.00%	9.721%
40	23.462	3457	3464	3472	rBV	685372	1378336	55.10%	5.356%




Sum of corrected areas: 25733547

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045023.D
Acq On : 08 Apr 2024 01:07
Operator : MA/JU
Sample : PB160066BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

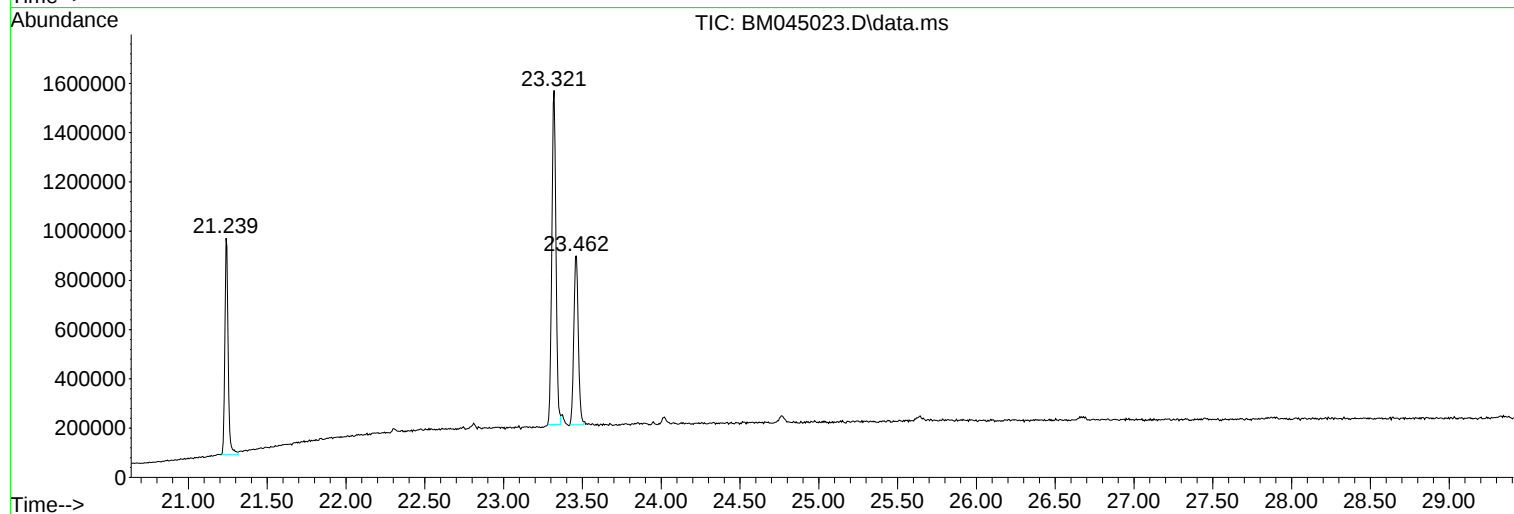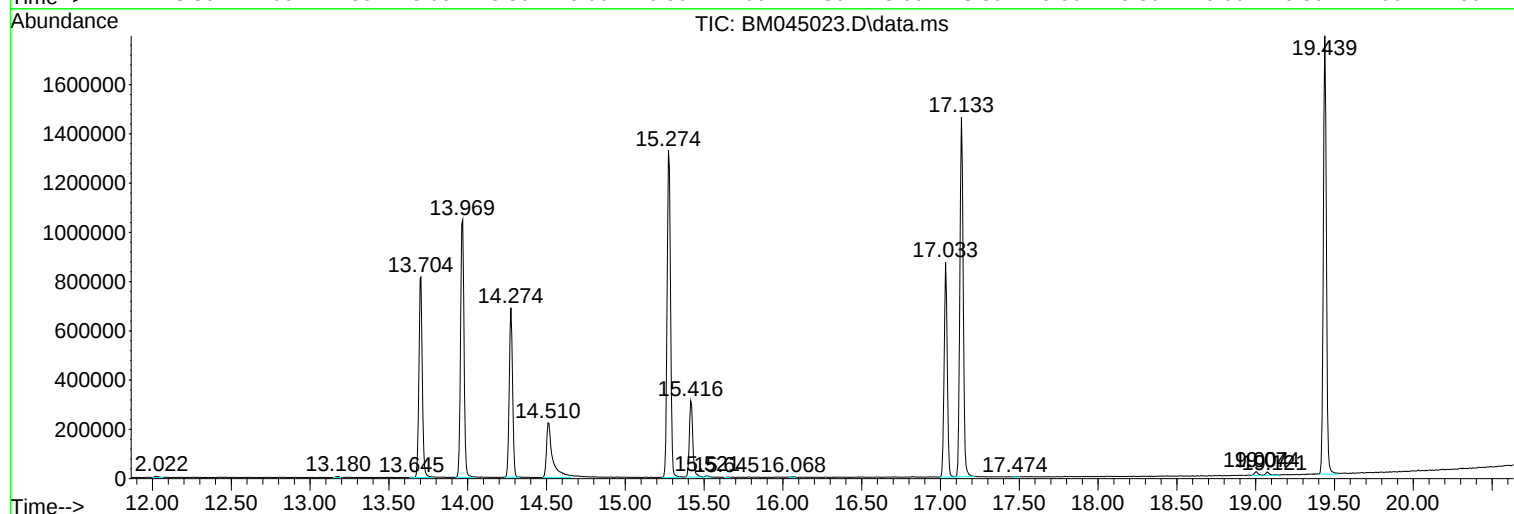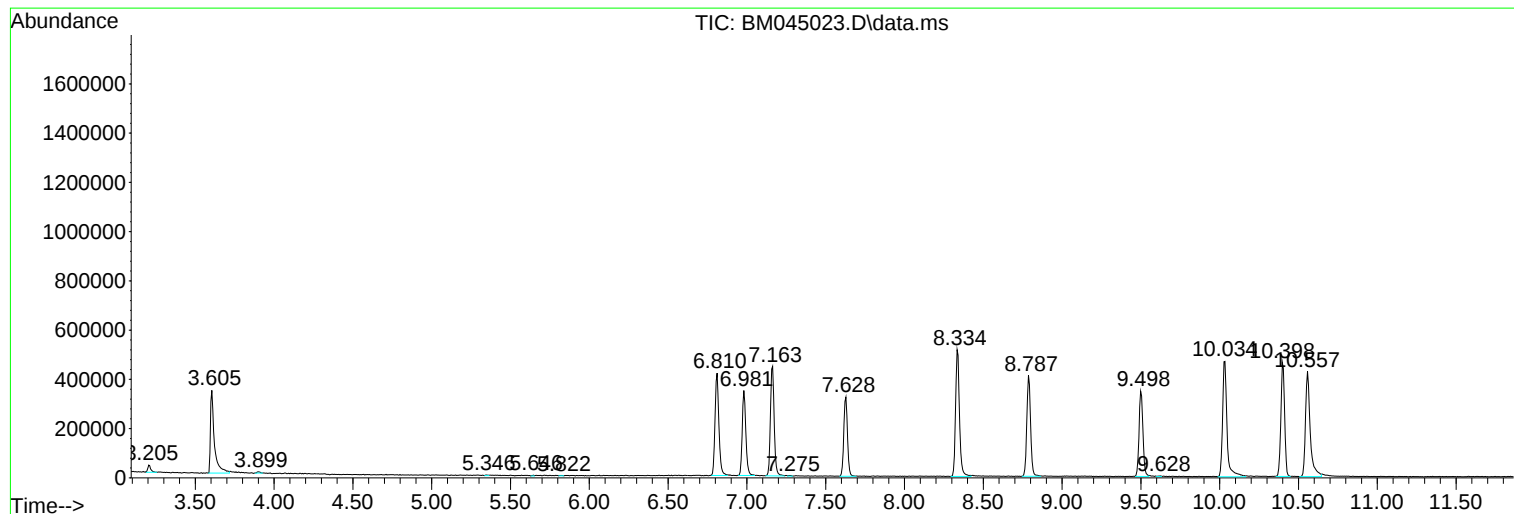

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045023.D
Acq On : 08 Apr 2024 01:07
Operator : MA/JU
Sample : PB160066BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045023.D
Acq On : 08 Apr 2024 01:07
Operator : MA/JU
Sample : PB160066BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc