

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045024.D
 Acq On : 08 Apr 2024 01:43
 Operator : MA/JU
 Sample : PB160064BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	29	rVB	29544	43178	2.19%	0.172%
2	3.605	85	88	105	rBV	363344	616124	31.18%	2.452%
3	3.899	134	138	144	rBV6	5250	8579	0.43%	0.034%
4	4.469	233	235	238	rVB4	2672	2497	0.13%	0.010%
5	4.822	291	295	296	rVB4	2508	2241	0.11%	0.009%
6	5.058	333	335	340	rVB6	2308	3321	0.17%	0.013%
7	5.787	457	459	463	rVB4	1738	1979	0.10%	0.008%
8	6.210	526	531	532	rBV5	1647	2307	0.12%	0.009%
9	6.810	626	633	648	rBV	446969	771120	39.03%	3.068%
10	6.981	656	662	672	rVV	383539	600596	30.40%	2.390%
11	7.052	672	674	677	rVB4	2488	2163	0.11%	0.009%
12	7.163	686	693	706	rBV	474422	785410	39.75%	3.125%
13	7.310	715	718	723	rVB6	1677	2280	0.12%	0.009%
14	7.628	765	772	780	rBV	383961	624674	31.62%	2.486%
15	7.863	809	812	817	rBV6	1132	2189	0.11%	0.009%
16	8.063	842	846	849	rBV5	2086	3305	0.17%	0.013%
17	8.334	885	892	903	rBV	575200	968997	49.04%	3.856%
18	8.540	926	927	930	rVB3	2718	2024	0.10%	0.008%
19	8.581	930	934	935	rBV3	2761	3274	0.17%	0.013%
20	8.681	948	951	954	rVB3	1929	2525	0.13%	0.010%
21	8.728	954	959	961	rBV4	1595	2398	0.12%	0.010%
22	8.787	962	969	983	rVV	450616	765720	38.75%	3.047%
23	8.881	983	985	989	rVV4	2811	4325	0.22%	0.017%
24	8.916	989	991	995	rVB3	1791	2251	0.11%	0.009%
25	9.028	1006	1010	1013	rBV3	1668	2927	0.15%	0.012%
26	9.498	1083	1090	1102	rBV	391372	654251	33.11%	2.603%
27	10.028	1173	1180	1201	rBV	545448	1005824	50.91%	4.002%
28	10.398	1236	1243	1251	rBV	561477	925408	46.84%	3.682%
29	10.557	1263	1270	1286	rBV	490209	990805	50.15%	3.943%
30	10.845	1318	1319	1323	rVB4	2021	2193	0.11%	0.009%
31	11.457	1422	1423	1427	rBV2	1724	2179	0.11%	0.009%
32	12.022	1516	1519	1520	rBV2	5673	4473	0.23%	0.018%
33	12.392	1579	1582	1585	rVB3	1559	2064	0.10%	0.008%
34	12.816	1649	1654	1657	rVB5	1547	2568	0.13%	0.010%
35	13.016	1684	1688	1690	rBV3	1830	2279	0.12%	0.009%
36	13.175	1708	1715	1719	rBV7	4308	7763	0.39%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045024.D
 Acq On : 08 Apr 2024 01:43
 Operator : MA/JU
 Sample : PB160064BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.698	1797	1804	1820	rBV	886653	1330827	67.36%	5.296%
38	13.851	1828	1830	1834	rBV4	1667	2431	0.12%	0.010%
39	13.969	1843	1850	1863	rBV	1148134	1710508	86.57%	6.806%
40	14.275	1894	1902	1909	rBV	816524	1184878	59.97%	4.715%
41	14.375	1917	1919	1922	rVB3	1981	2109	0.11%	0.008%
42	14.516	1936	1943	1965	rBV	169951	490161	24.81%	1.950%
43	15.275	2064	2072	2080	rBV	1324947	1975817	100.00%	7.862%
44	15.357	2085	2086	2091	rVV5	3091	4351	0.22%	0.017%
45	15.416	2091	2096	2109	rVV	266299	415074	21.01%	1.652%
46	15.522	2111	2114	2119	rVB5	5738	7877	0.40%	0.031%
47	15.722	2147	2148	2153	rVB3	1442	2068	0.10%	0.008%
48	16.063	2203	2206	2210	rVB3	3284	4794	0.24%	0.019%
49	16.710	2310	2316	2319	rBV3	1260	2844	0.14%	0.011%
50	16.816	2332	2334	2341	rVB5	2725	4282	0.22%	0.017%
51	17.033	2365	2371	2382	rBV	865701	1196305	60.55%	4.760%
52	17.133	2382	2388	2404	rVV2	1308179	1889493	95.63%	7.519%
53	17.751	2489	2493	2495	rBV5	2374	2520	0.13%	0.010%
54	17.845	2506	2509	2511	rBV4	1782	2166	0.11%	0.009%
55	18.039	2539	2542	2544	rBV3	2320	3075	0.16%	0.012%
56	18.339	2591	2593	2595	rBV3	2240	2543	0.13%	0.010%
57	18.533	2622	2626	2628	rBV5	2505	3446	0.17%	0.014%
58	18.763	2663	2665	2666	rBV2	2102	2036	0.10%	0.008%
59	18.792	2668	2670	2672	rBV2	2956	3142	0.16%	0.013%
60	18.851	2679	2680	2683	rBV3	2917	2092	0.11%	0.008%
61	19.004	2703	2706	2712	rVB5	13069	17958	0.91%	0.071%
62	19.080	2712	2719	2724	rBV2	10181	18260	0.92%	0.073%
63	19.316	2757	2759	2761	rBV3	2462	2502	0.13%	0.010%
64	19.439	2774	2780	2789	rBV	1435191	1943085	98.34%	7.732%
65	21.245	3082	3087	3095	rBV	716001	1039628	52.62%	4.137%
66	23.321	3433	3440	3446	rBV2	1026711	1870469	94.67%	7.443%
67	23.456	3457	3463	3475	rVB	596924	1168081	59.12%	4.648%




Sum of corrected areas: 25131033

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045024.D
Acq On : 08 Apr 2024 01:43
Operator : MA/JU
Sample : PB160064BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

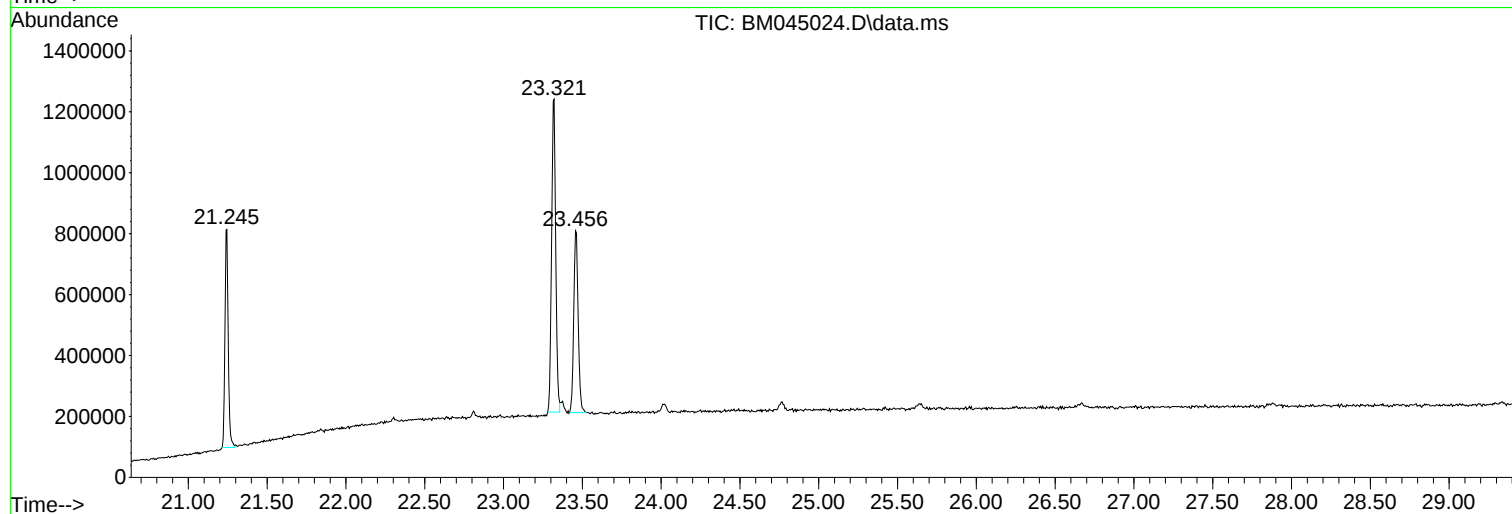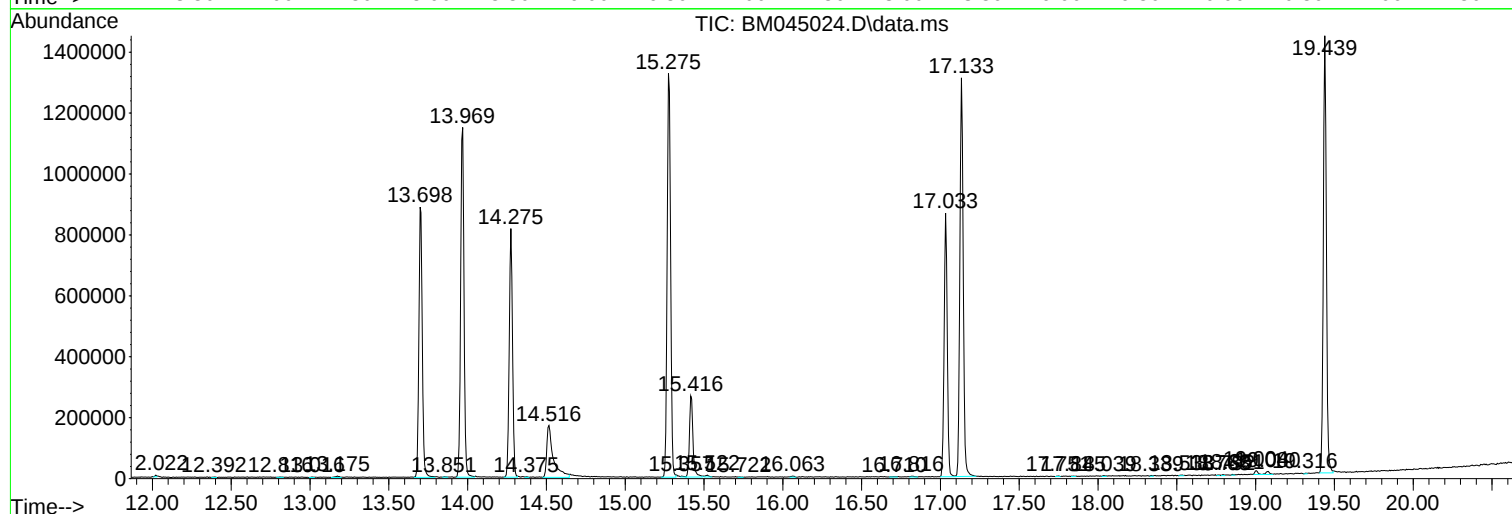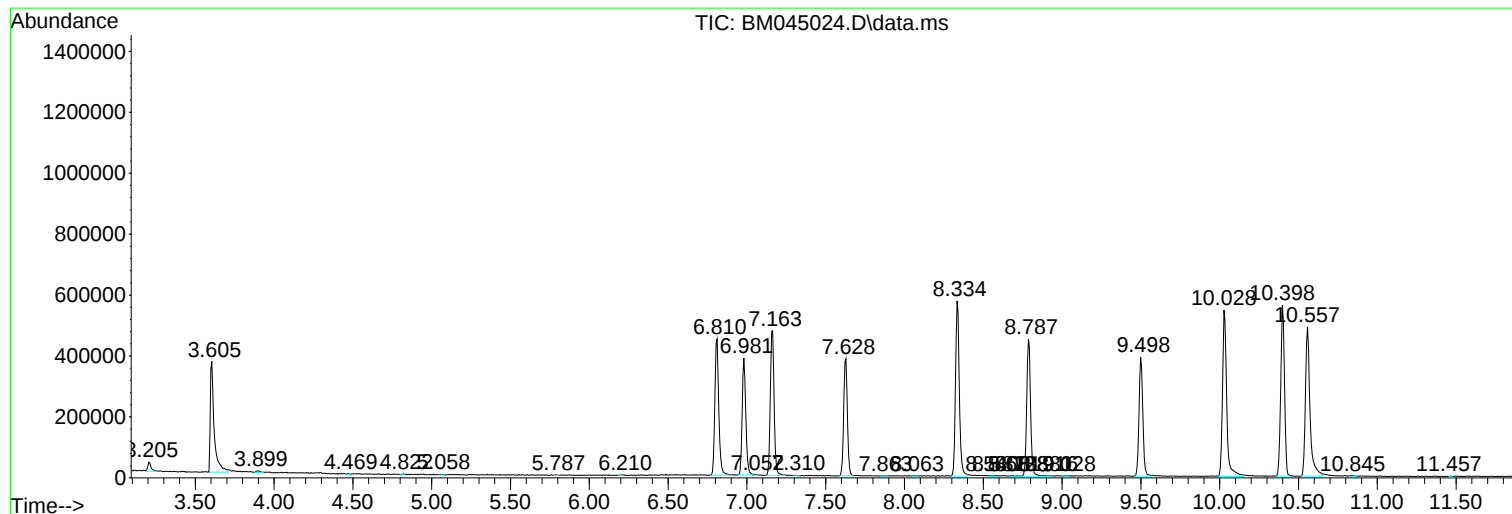

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045024.D
Acq On : 08 Apr 2024 01:43
Operator : MA/JU
Sample : PB160064BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045024.D
Acq On : 08 Apr 2024 01:43
Operator : MA/JU
Sample : PB160064BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------