

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045036.D
 Acq On : 08 Apr 2024 10:18
 Operator : MA/JU
 Sample : PB160051BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	31	rVB	27521	36667	1.49%	0.142%
2	3.463	62	64	67	rBV3	2912	2747	0.11%	0.011%
3	3.604	84	88	112	rBV	300601	562725	22.85%	2.173%
4	3.899	135	138	142	rVB5	4249	5840	0.24%	0.023%
5	3.981	150	152	154	rBV3	3182	2689	0.11%	0.010%
6	4.040	160	162	164	rBV3	2893	2942	0.12%	0.011%
7	4.663	267	268	272	rBV4	2843	2855	0.12%	0.011%
8	5.634	430	433	436	rBV5	2095	2854	0.12%	0.011%
9	5.922	480	482	487	rBV6	1799	2585	0.10%	0.010%
10	6.345	551	554	561	rBV7	1395	2810	0.11%	0.011%
11	6.804	625	632	648	rBV	401430	692142	28.10%	2.672%
12	6.981	656	662	673	rVB	319289	513547	20.85%	1.983%
13	7.157	684	692	706	rBV	427660	696468	28.28%	2.689%
14	7.622	763	771	784	rBV	340006	551131	22.38%	2.128%
15	8.334	885	892	905	rBV	513815	856085	34.76%	3.305%
16	8.786	962	969	979	rBV	390325	659902	26.79%	2.548%
17	9.498	1083	1090	1101	rBV	341128	574739	23.34%	2.219%
18	10.028	1173	1180	1201	rBV	479237	891065	36.18%	3.440%
19	10.398	1235	1243	1251	rBV	480379	803339	32.62%	3.102%
20	10.557	1262	1270	1292	rBV	415516	879784	35.72%	3.397%
21	11.333	1397	1402	1405	rBV6	1895	2888	0.12%	0.011%
22	12.022	1512	1519	1526	rVB6	5622	12287	0.50%	0.047%
23	12.510	1593	1602	1603	rBV6	1860	4770	0.19%	0.018%
24	12.804	1647	1652	1653	rVB3	1785	2497	0.10%	0.010%
25	13.174	1710	1715	1720	rBV6	4297	6818	0.28%	0.026%
26	13.704	1798	1805	1819	rVB	820835	1193891	48.48%	4.610%
27	13.968	1842	1850	1860	rBV	1067411	1577723	64.06%	6.092%
28	14.274	1895	1902	1909	rBV	749763	1100074	44.67%	4.247%
29	14.515	1936	1943	1966	rBV	209870	569904	23.14%	2.200%
30	14.874	1999	2004	2006	rVB4	2048	3851	0.16%	0.015%
31	14.915	2006	2011	2012	rBV5	3060	3856	0.16%	0.015%
32	15.233	2061	2065	2066	rBV2	5416	7180	0.29%	0.028%
33	15.274	2066	2072	2085	rVB	1305235	1932106	78.45%	7.460%
34	15.415	2091	2096	2110	rBV	311735	476229	19.34%	1.839%
35	15.515	2110	2113	2118	rVB7	6002	9605	0.39%	0.037%
36	15.604	2124	2128	2131	rBV4	1691	2953	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045036.D
 Acq On : 08 Apr 2024 10:18
 Operator : MA/JU
 Sample : PB160051BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.074	2202	2208	2210	rBV6	3025	4762	0.19%	0.018%
38	16.492	2274	2279	2283	rBV5	4128	5827	0.24%	0.022%
39	16.815	2330	2334	2339	rBV5	2438	4429	0.18%	0.017%
40	17.033	2365	2371	2381	rBV	931899	1323985	53.76%	5.112%
41	17.133	2382	2388	2400	rVV2	1400939	2091982	84.94%	8.077%
42	17.568	2459	2462	2465	rVB4	2956	3997	0.16%	0.015%
43	17.962	2525	2529	2530	rBV4	3846	3229	0.13%	0.012%
44	18.309	2585	2588	2591	rBV4	2135	2875	0.12%	0.011%
45	18.392	2597	2602	2603	rBV5	1749	2746	0.11%	0.011%
46	18.527	2622	2625	2630	rVB6	4029	5040	0.20%	0.019%
47	19.003	2702	2706	2712	rBV4	16095	22011	0.89%	0.085%
48	19.080	2715	2719	2723	rVV2	10172	14772	0.60%	0.057%
49	19.239	2745	2746	2748	rBV2	3367	2753	0.11%	0.011%
50	19.392	2768	2772	2774	rBV4	15720	19630	0.80%	0.076%
51	19.439	2774	2780	2789	rVV	1770721	2402949	97.57%	9.278%
52	20.444	2948	2951	2955	rBV4	12962	16200	0.66%	0.063%
53	21.244	3082	3087	3097	rBV	1011645	1399878	56.84%	5.405%
54	23.321	3434	3440	3447	rBV2	1354608	2462878	100.00%	9.509%
55	23.462	3458	3464	3473	rVB	756061	1460357	59.29%	5.638%




Sum of corrected areas: 25899848

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045036.D
Acq On : 08 Apr 2024 10:18
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

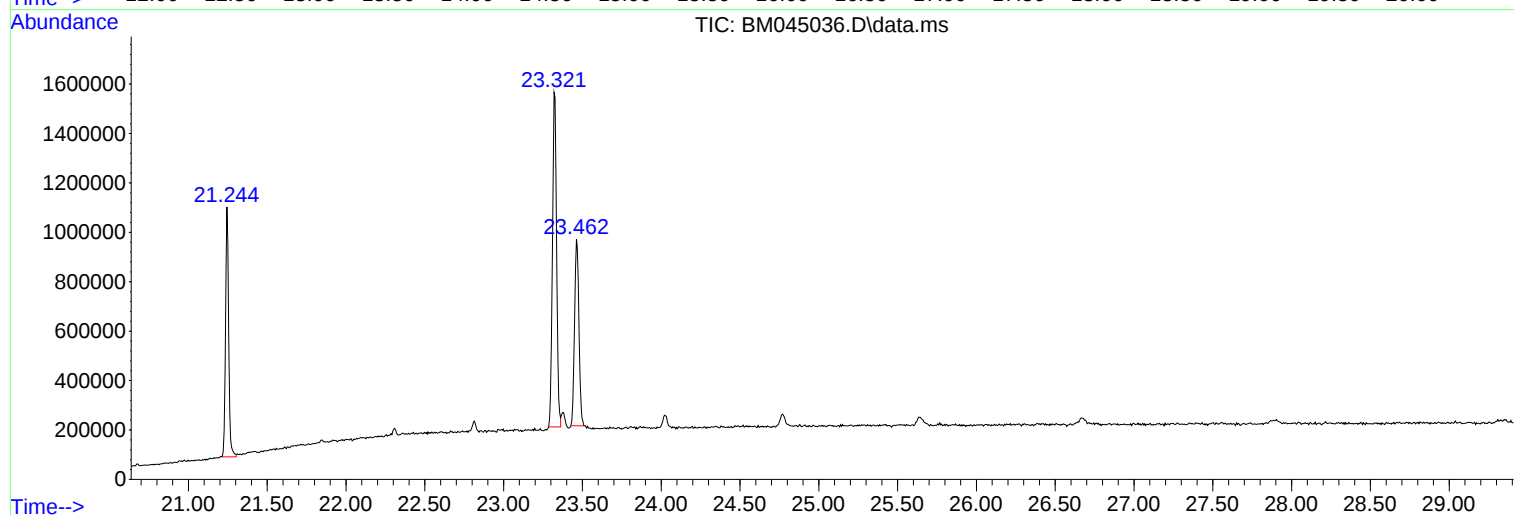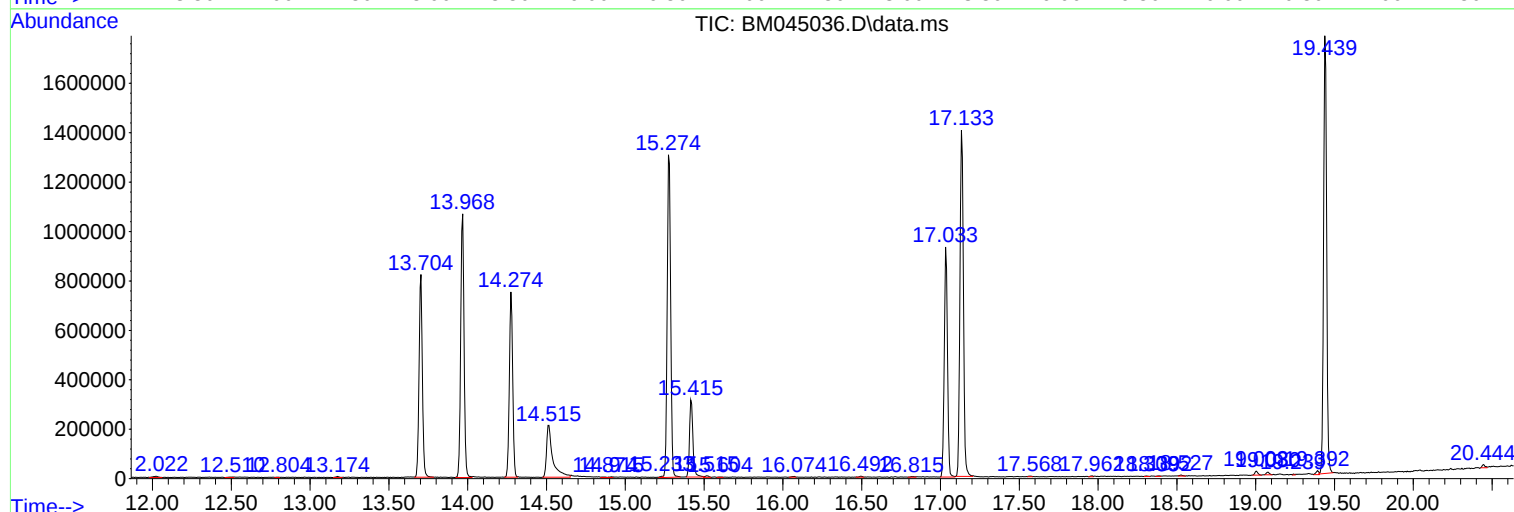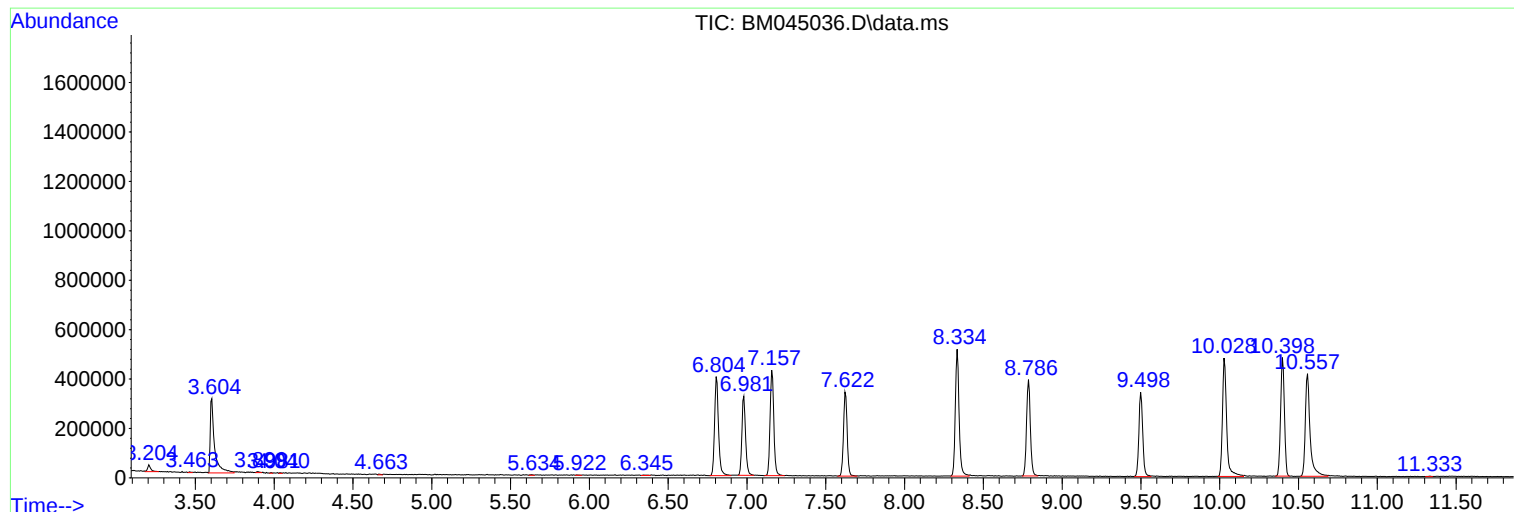

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045036.D
Acq On : 08 Apr 2024 10:18
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045036.D
Acq On : 08 Apr 2024 10:18
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------