

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045038.D
 Acq On : 08 Apr 2024 12:23
 Operator : MA/JU
 Sample : P2012-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	11	14	17	rBV5	3920	5552	0.22%	0.029%
2	3.204	17	20	23	rVV	11724	13018	0.51%	0.068%
3	3.240	23	26	31	rVB3	8588	12828	0.50%	0.067%
4	3.622	87	91	98	rBV	37544	75226	2.93%	0.391%
5	3.899	136	138	143	rVB5	3488	3342	0.13%	0.017%
6	4.146	178	180	182	rBV3	3898	2976	0.12%	0.015%
7	6.004	494	496	501	rVB5	2395	2625	0.10%	0.014%
8	6.816	628	634	645	rBV2	48152	99755	3.88%	0.518%
9	6.981	654	662	672	rBV	234308	391121	15.21%	2.033%
10	7.157	685	692	703	rBV	224002	392132	15.25%	2.038%
11	7.622	765	771	781	rVB	189356	315387	12.26%	1.639%
12	7.763	791	795	799	rVB4	2115	2908	0.11%	0.015%
13	8.334	886	892	905	rBV	159691	285734	11.11%	1.485%
14	8.469	910	915	918	rVB6	2155	3754	0.15%	0.020%
15	8.728	955	959	962	rBV4	4385	5964	0.23%	0.031%
16	8.786	962	969	978	rBV	285821	483854	18.81%	2.515%
17	9.498	1083	1090	1103	rBV	241195	410139	15.95%	2.132%
18	10.028	1173	1180	1199	rBV	298746	606168	23.57%	3.150%
19	10.398	1236	1243	1250	rBV	286684	480617	18.69%	2.498%
20	10.557	1261	1270	1287	rBV	248000	543094	21.12%	2.823%
21	11.092	1358	1361	1363	rBV4	2823	2593	0.10%	0.013%
22	11.228	1379	1384	1388	rBV7	2879	5780	0.22%	0.030%
23	11.292	1390	1395	1396	rBV5	2248	3291	0.13%	0.017%
24	11.551	1436	1439	1443	rBV6	1715	2658	0.10%	0.014%
25	11.669	1453	1459	1464	rVB6	3538	6968	0.27%	0.036%
26	11.963	1503	1509	1513	rBV4	8787	19036	0.74%	0.099%
27	12.004	1513	1516	1522	rVB5	4443	8244	0.32%	0.043%
28	12.263	1555	1560	1564	rBV5	4139	7039	0.27%	0.037%
29	12.351	1573	1575	1580	rVB4	2263	2742	0.11%	0.014%
30	12.898	1665	1668	1672	rVB5	1834	2972	0.12%	0.015%
31	13.098	1698	1702	1705	rVB5	1850	2729	0.11%	0.014%
32	13.163	1710	1713	1719	rVB6	5618	8478	0.33%	0.044%
33	13.504	1768	1771	1776	rBV7	2304	4247	0.17%	0.022%
34	13.698	1798	1804	1819	rBV	708333	1027425	39.95%	5.340%
35	13.963	1842	1849	1860	rBV	849433	1272100	49.46%	6.611%
36	14.039	1860	1862	1865	rVV2	2519	2946	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045038.D
 Acq On : 08 Apr 2024 12:23
 Operator : MA/JU
 Sample : P2012-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.098	1869	1872	1878	rVB5	2377	4898	0.19%	0.025%
38	14.274	1896	1902	1913	rBV	448767	671138	26.10%	3.488%
39	14.551	1943	1949	1960	rBV6	15162	54727	2.13%	0.284%
40	15.274	2065	2072	2081	rBV	1157574	1683188	65.45%	8.748%
41	15.415	2090	2096	2106	rBV	297541	452749	17.60%	2.353%
42	15.510	2111	2112	2117	rVB5	4988	7244	0.28%	0.038%
43	15.663	2134	2138	2144	rBV6	2009	4803	0.19%	0.025%
44	16.062	2203	2206	2211	rVB4	3413	5135	0.20%	0.027%
45	17.033	2364	2371	2379	rBV	571113	811873	31.57%	4.219%
46	17.133	2381	2388	2400	rBV	1329064	1951242	75.87%	10.141%
47	17.286	2408	2414	2415	rBV5	2032	3113	0.12%	0.016%
48	17.339	2420	2423	2426	rBV5	3041	2932	0.11%	0.015%
49	17.633	2470	2473	2477	rBV6	2840	3197	0.12%	0.017%
50	17.815	2500	2504	2508	rBV6	2499	4803	0.19%	0.025%
51	17.939	2521	2525	2536	rBV3	26693	45892	1.78%	0.239%
52	18.374	2597	2599	2602	rBV4	2964	2591	0.10%	0.013%
53	18.703	2651	2655	2660	rBV7	4600	10243	0.40%	0.053%
54	19.003	2701	2706	2710	rBV3	20821	29337	1.14%	0.152%
55	19.074	2715	2718	2722	rBV2	12166	18916	0.74%	0.098%
56	19.239	2742	2746	2748	rBV5	10567	15500	0.60%	0.081%
57	19.439	2774	2780	2790	rBV	1751854	2360328	91.78%	12.267%
58	21.239	3081	3086	3094	rBV	689920	946679	36.81%	4.920%
59	23.315	3433	3439	3446	rBV	1424792	2571774	100.00%	13.366%
60	23.456	3457	3463	3476	rVB	541588	1063305	41.35%	5.526%




Sum of corrected areas: 19241049

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045038.D
Acq On : 08 Apr 2024 12:23
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

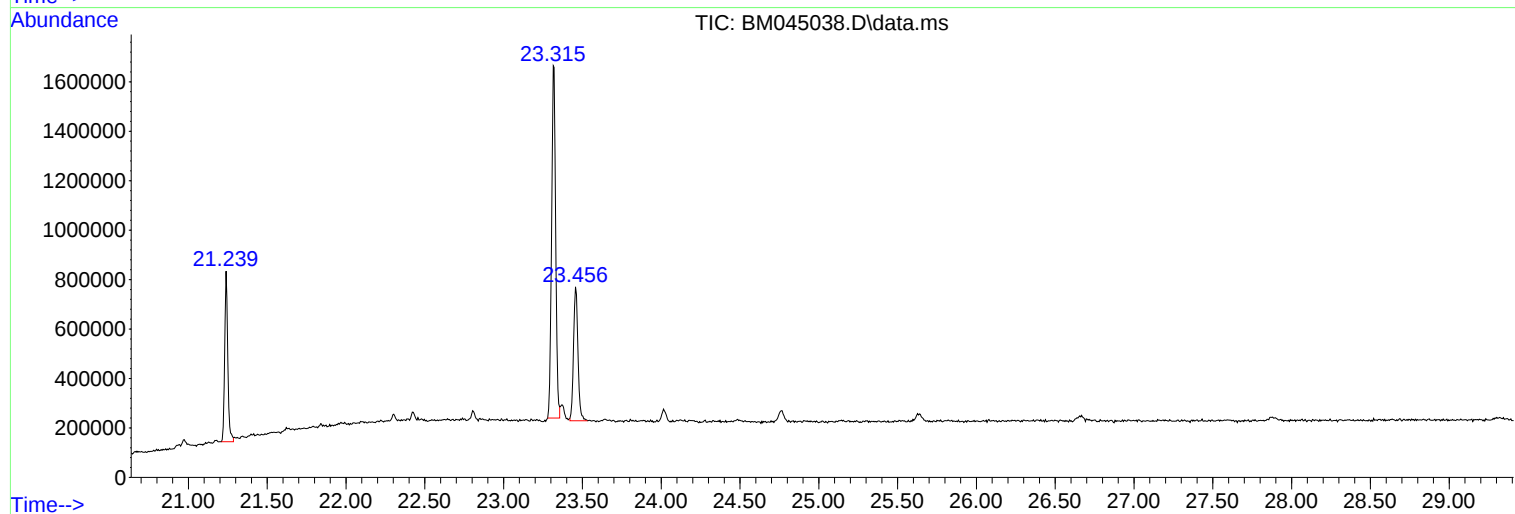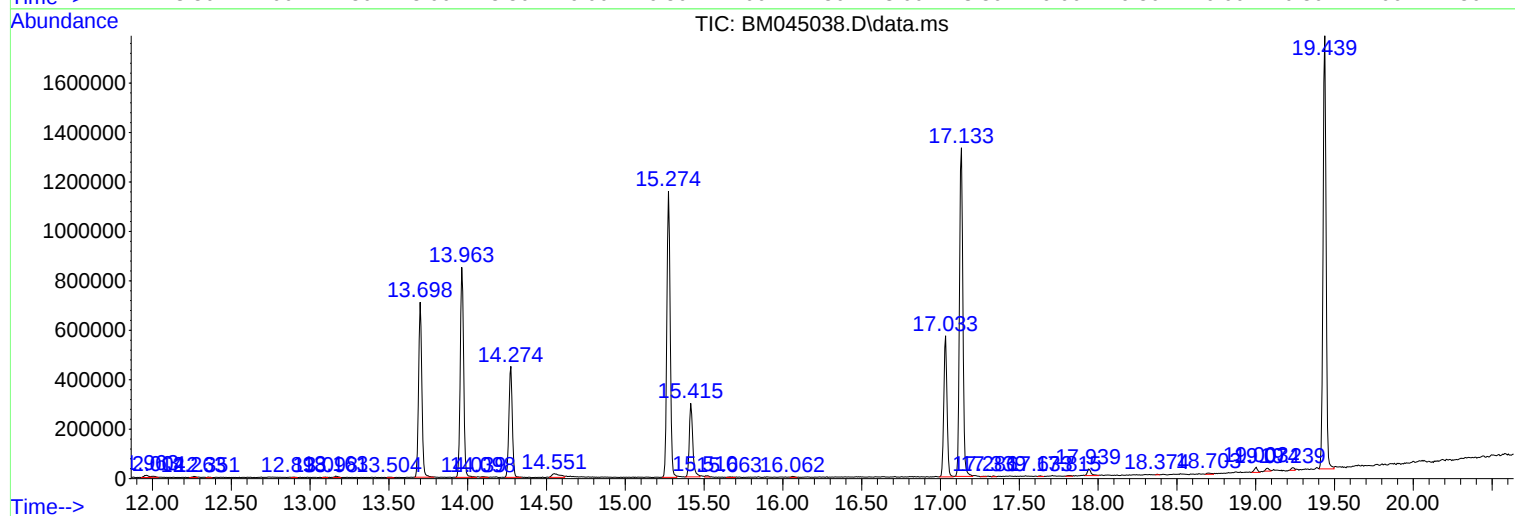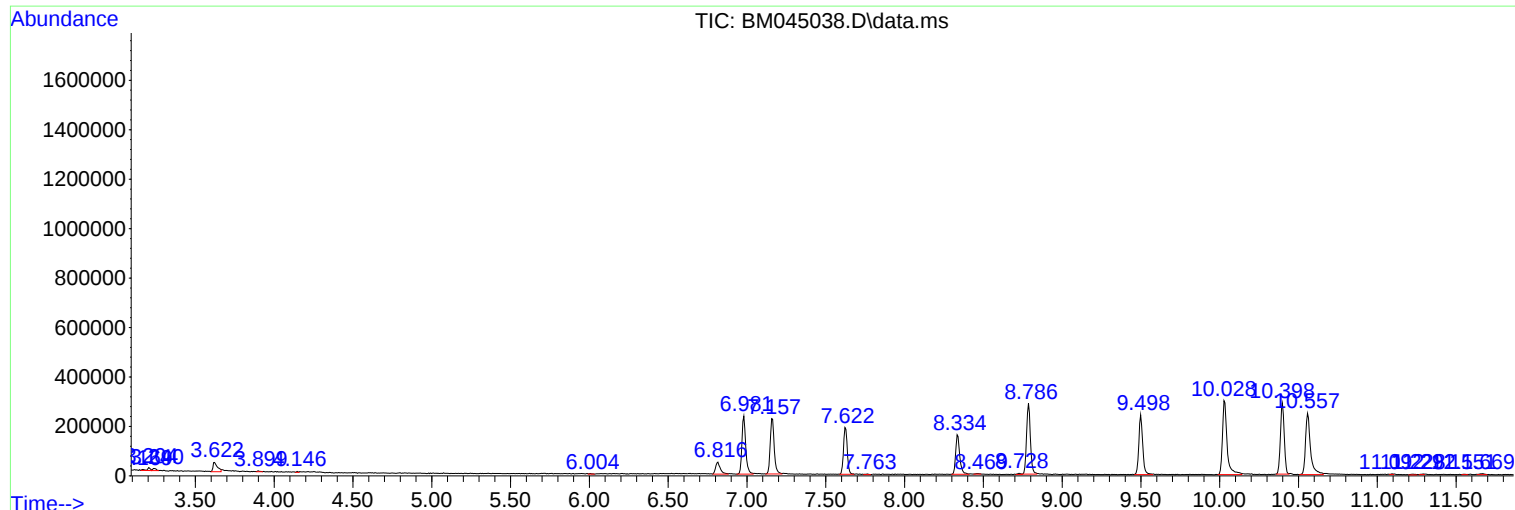

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045038.D
Acq On : 08 Apr 2024 12:23
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045038.D
Acq On : 08 Apr 2024 12:23
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc