

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
 Data File : BM045041.D
 Acq On : 08 Apr 2024 14:42
 Operator : MA/JU
 Sample : P1997-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	26	rVB2	13343	19469	0.69%	0.088%
2	3.616	86	90	101	rBV	61741	137028	4.88%	0.622%
3	5.687	441	442	447	rBV5	1831	2884	0.10%	0.013%
4	6.810	627	633	642	rBV2	56563	114983	4.10%	0.522%
5	6.981	656	662	671	rBV	319486	520577	18.54%	2.365%
6	7.157	686	692	704	rBV	297811	508278	18.11%	2.309%
7	7.622	765	771	782	rBV	246682	396621	14.13%	1.802%
8	8.334	884	892	903	rBV2	209651	373848	13.32%	1.698%
9	8.787	961	969	979	rBV	374788	642027	22.87%	2.916%
10	9.498	1082	1090	1101	rBV	297757	522934	18.63%	2.375%
11	9.828	1141	1146	1150	rVB6	1761	3450	0.12%	0.016%
12	10.028	1171	1180	1199	rBV	385670	741080	26.40%	3.366%
13	10.398	1236	1243	1253	rVB	339930	581931	20.73%	2.643%
14	10.557	1260	1270	1289	rBV	317932	703339	25.05%	3.195%
15	11.622	1448	1451	1457	rVB6	2111	3643	0.13%	0.017%
16	12.016	1513	1518	1528	rBV6	4986	11374	0.41%	0.052%
17	13.174	1709	1715	1716	rBV6	3799	4771	0.17%	0.022%
18	13.633	1788	1793	1796	rVV6	2288	4562	0.16%	0.021%
19	13.698	1798	1804	1821	rVB	777752	1161105	41.36%	5.274%
20	13.969	1843	1850	1861	rBV	954971	1492872	53.18%	6.781%
21	14.274	1894	1902	1910	rVV	541681	785275	27.97%	3.567%
22	14.551	1942	1949	1950	rBV5	12909	20915	0.75%	0.095%
23	15.274	2066	2072	2085	rBV	1274299	1861464	66.31%	8.456%
24	15.416	2091	2096	2110	rBV	324797	516165	18.39%	2.345%
25	15.521	2110	2114	2118	rVB5	4950	5802	0.21%	0.026%
26	16.074	2203	2208	2211	rVB4	3474	6155	0.22%	0.028%
27	16.486	2271	2278	2279	rBV4	2170	3830	0.14%	0.017%
28	16.710	2314	2316	2322	rBV3	2151	2991	0.11%	0.014%
29	16.833	2333	2337	2341	rVB6	2309	3842	0.14%	0.017%
30	17.033	2365	2371	2381	rBV	679549	943324	33.60%	4.285%
31	17.133	2381	2388	2402	rVV	1469266	2123030	75.62%	9.644%
32	17.568	2457	2462	2468	rVB5	3022	5507	0.20%	0.025%
33	17.945	2521	2526	2533	rBV4	23081	38129	1.36%	0.173%
34	18.233	2572	2575	2579	rBV7	2304	3836	0.14%	0.017%
35	18.380	2598	2600	2603	rVB4	2983	3606	0.13%	0.016%
36	18.415	2603	2606	2608	rBV3	3118	3294	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045041.D
Acq On : 08 Apr 2024 14:42
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	18.504	2616	2621	2622	rBV4	2760	4805	0.17%	0.022%
38	18.609	2636	2639	2642	rBV5	2954	3215	0.11%	0.015%
39	19.004	2702	2706	2712	rVV2	18022	25311	0.90%	0.115%
40	19.074	2714	2718	2723	rBV2	13383	20705	0.74%	0.094%
41	19.198	2737	2739	2741	rBV3	2919	2944	0.10%	0.013%
42	19.239	2742	2746	2750	rVV5	24167	32818	1.17%	0.149%
43	19.439	2774	2780	2789	rBV	1864153	2536706	90.36%	11.523%
44	21.245	3082	3087	3098	rBV	805332	1119325	39.87%	5.085%
45	23.327	3434	3441	3448	rBV	1583657	2807341	100.00%	12.752%
46	23.462	3458	3464	3475	rVB	603998	1187009	42.28%	5.392%




Sum of corrected areas: 22014120

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045041.D
Acq On : 08 Apr 2024 14:42
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

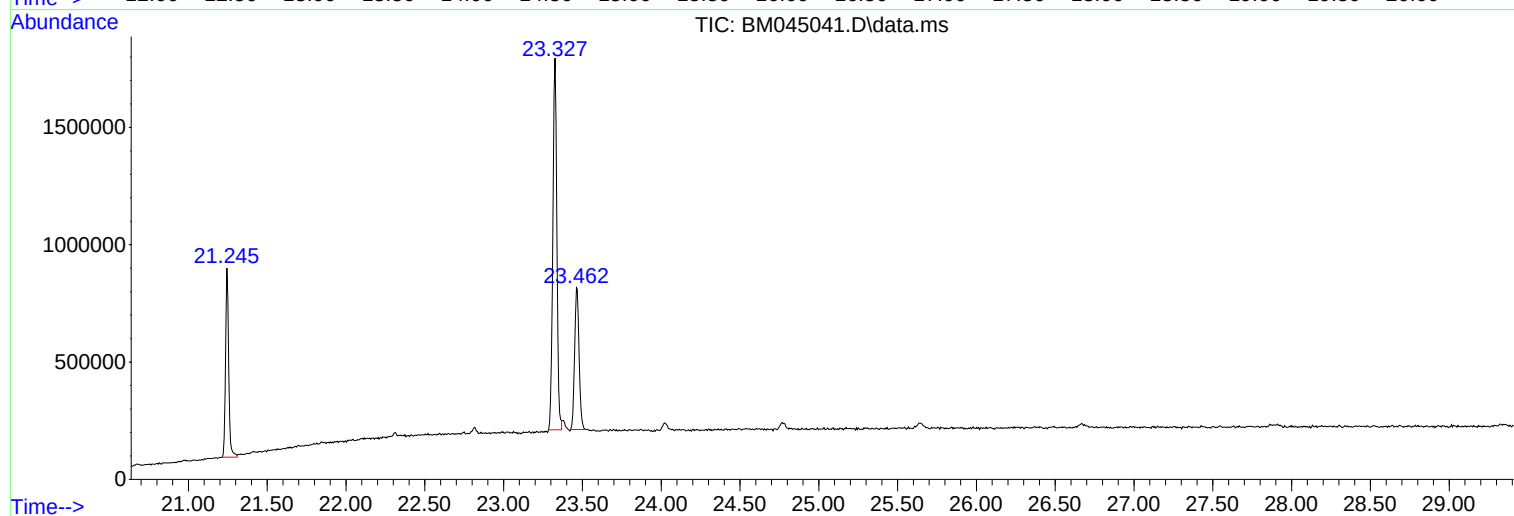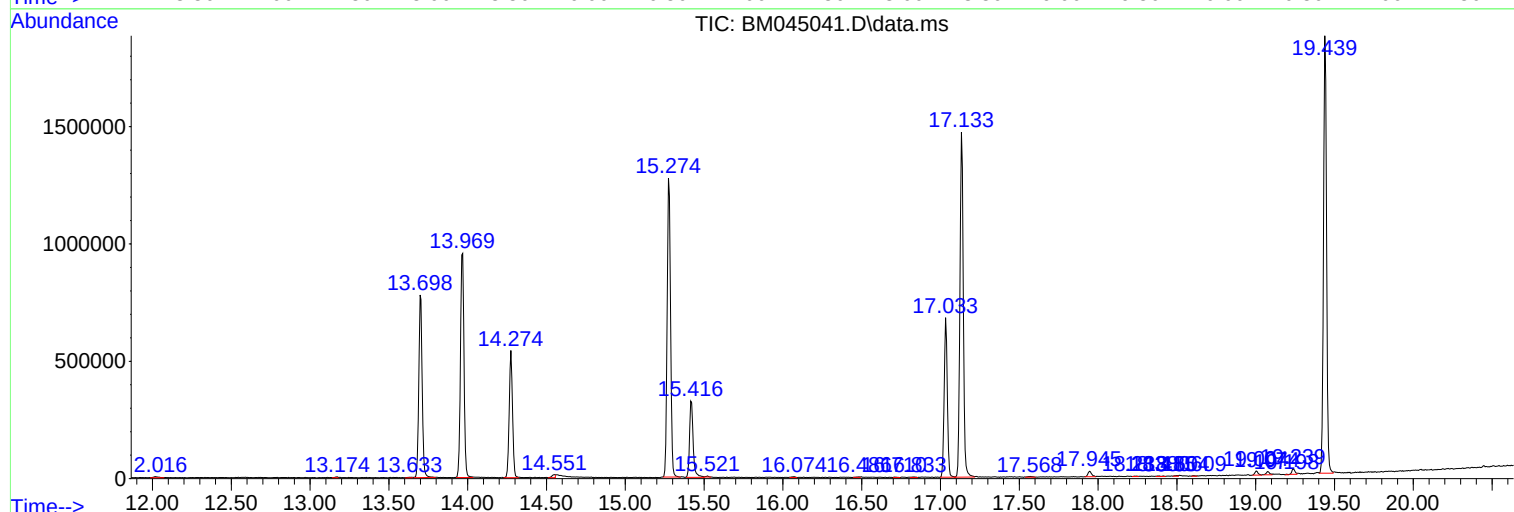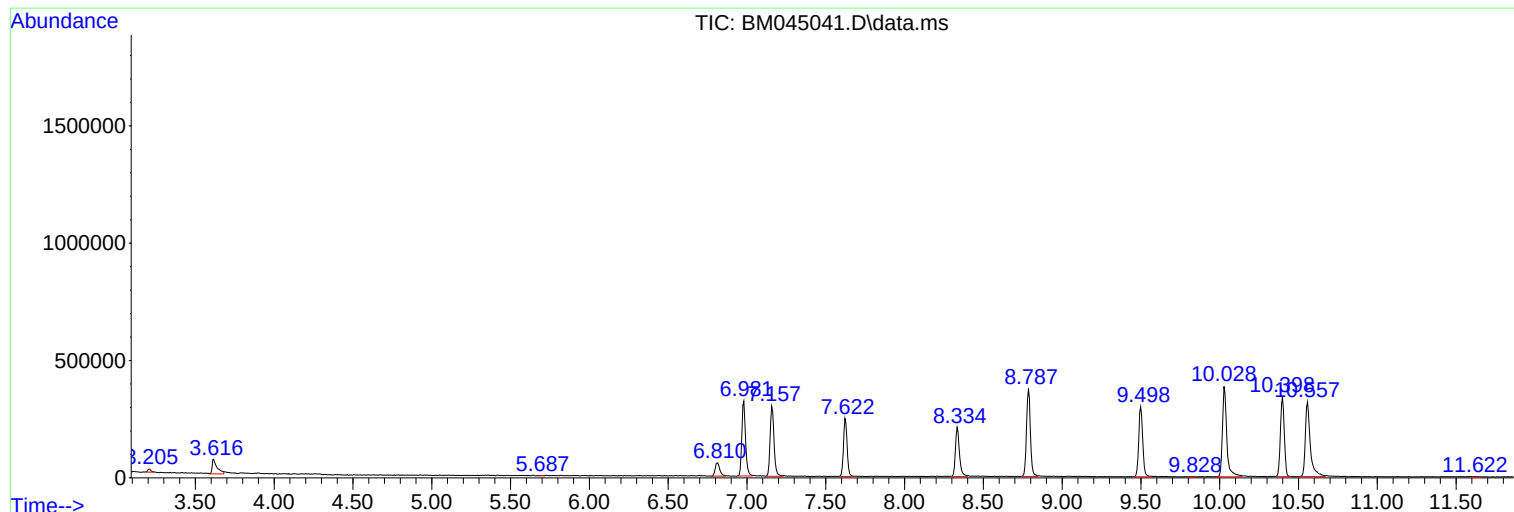

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045041.D
Acq On : 08 Apr 2024 14:42
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040724\
Data File : BM045041.D
Acq On : 08 Apr 2024 14:42
Operator : MA/JU
Sample : P1997-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc