


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019802.D
Acq On : 08 Apr 2019 19:36
Operator : JU/SJ
Sample : K2269-01DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 09 08:25:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 07:14:39 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0BR2DL

Manual Integrations
APPROVED

Sohil
4/10/2019 6:16:32 PM

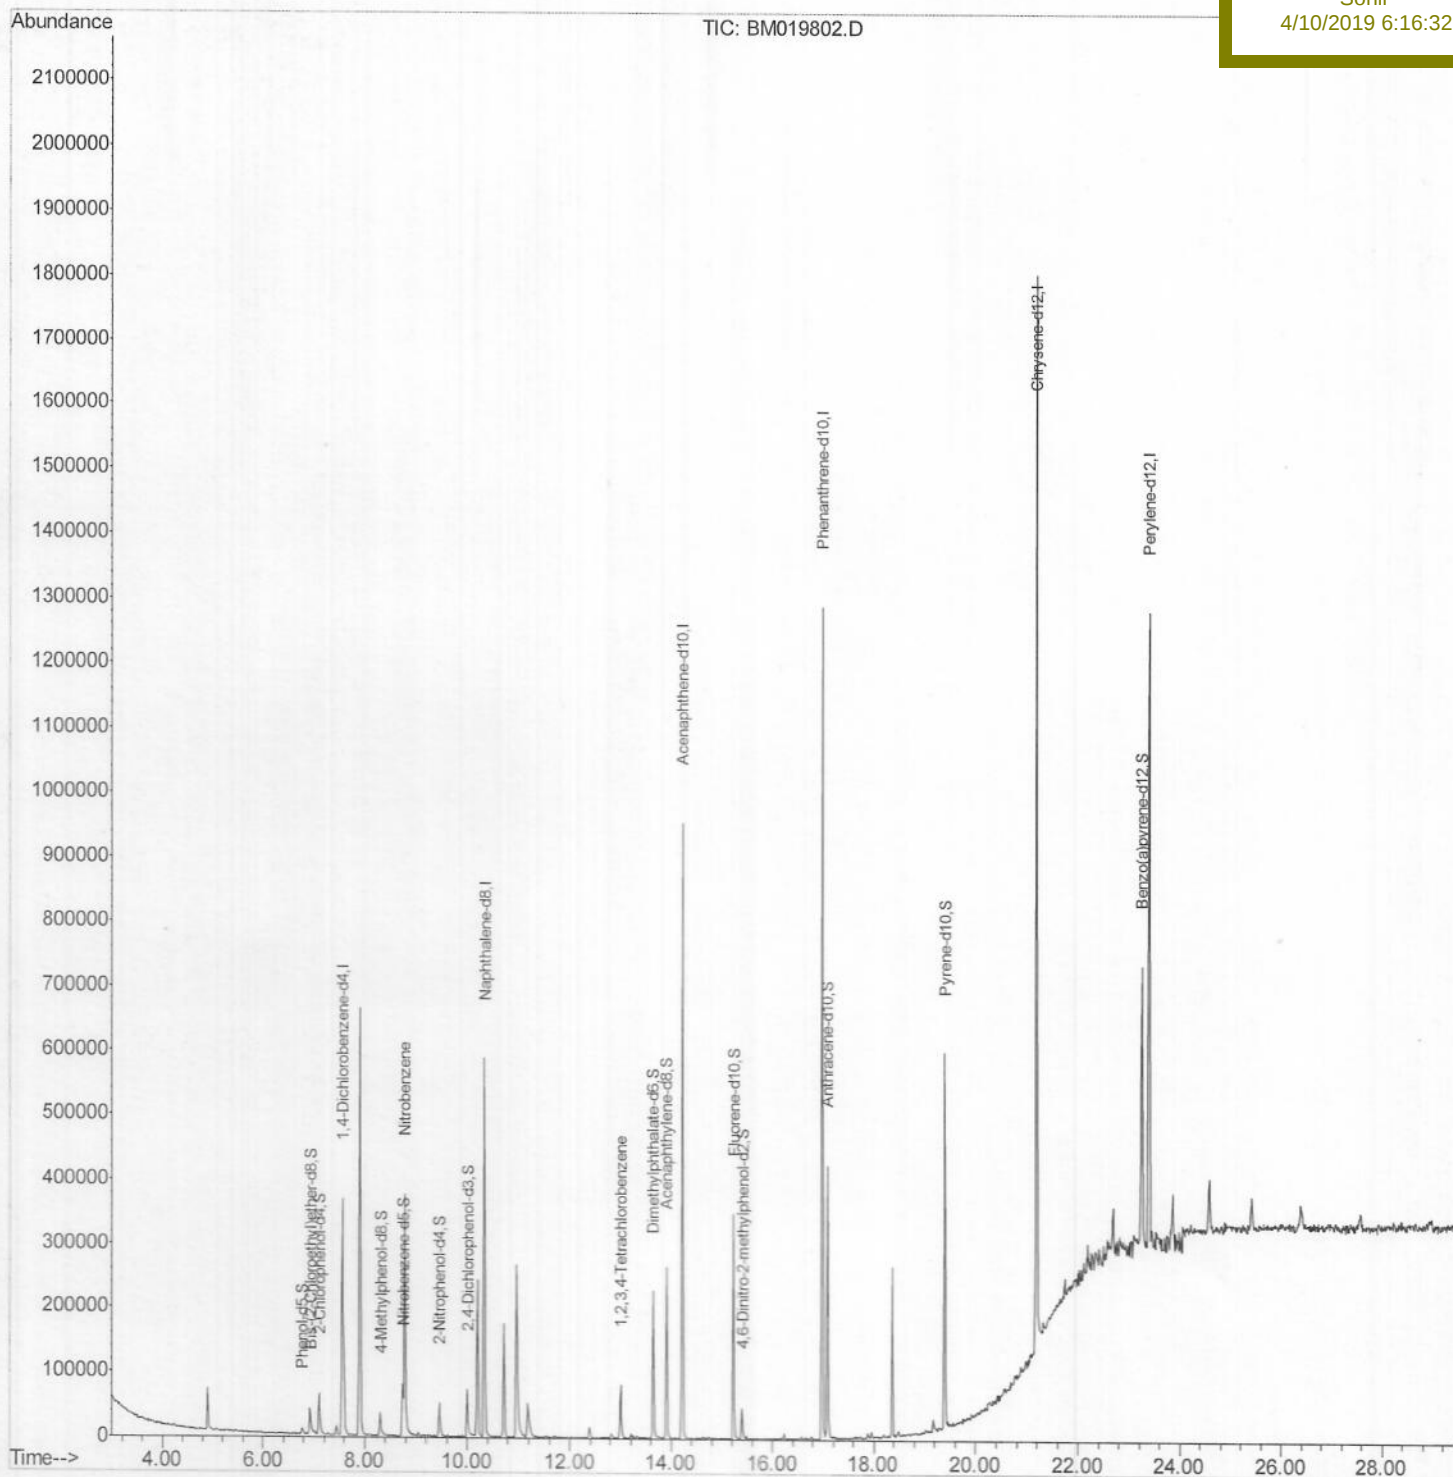

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019802.D
Acq On : 08 Apr 2019 19:36
Operator : JU/SJ
Sample : K2269-01DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 09 07:17:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 07:14:39 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0BR2DL

Manual Integrations
APPROVED

Sohil
4/10/2019 6:16:32 PM

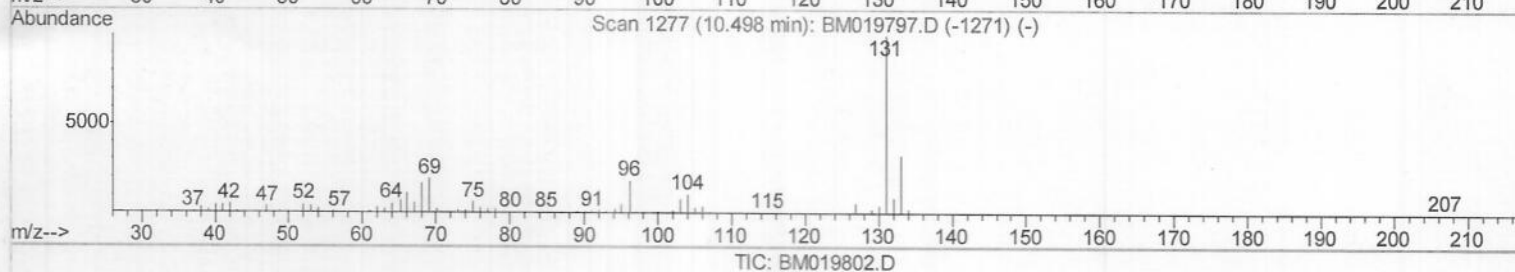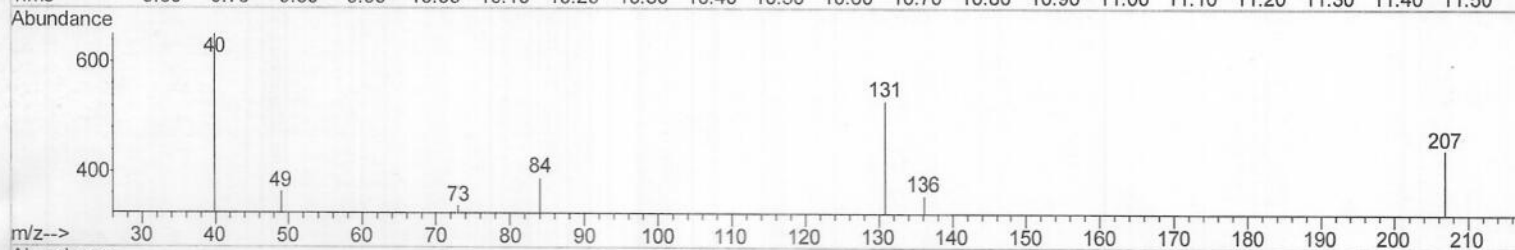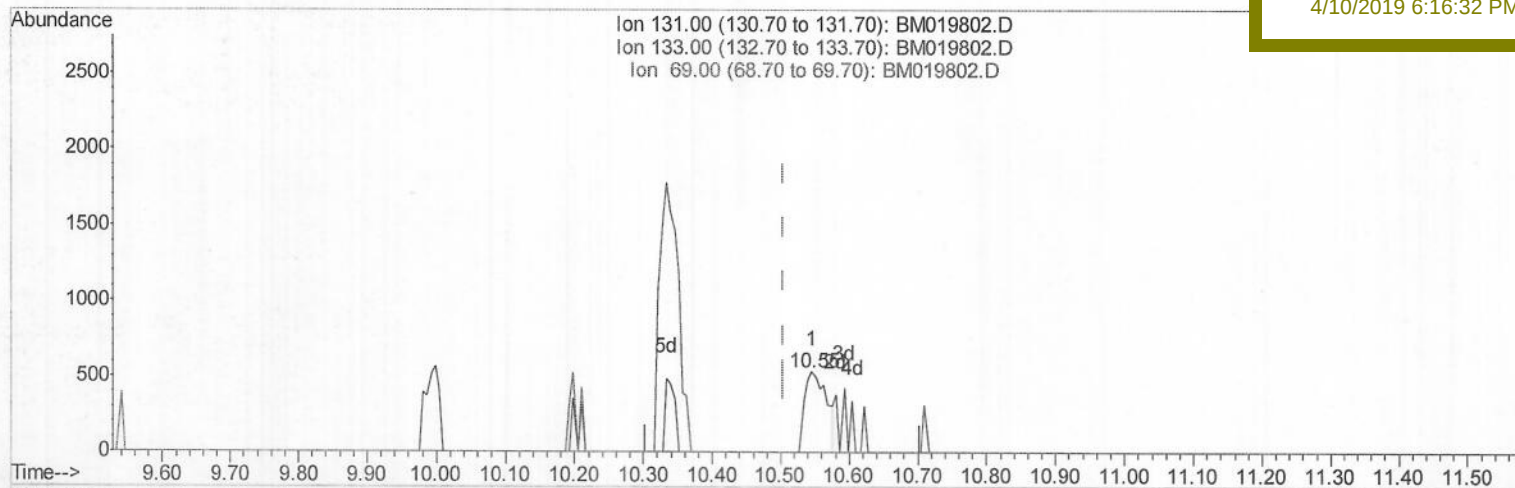

(29) 4-Chloroaniline-d4 (S)

10.545min (+0.041) 0.13ng/ul

response 1176

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	0.00#
69.00	18.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\

Data File : BM019802.D

Acq On : 08 Apr 2019 19:36

Operator : JU/SJ

Sample : K2269-01DL 5X

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 09 07:17:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Apr 09 07:14:39 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0BR2DL

Manual Integrations

APPROVED

Sohil

4/10/2019 6:16:32 PM

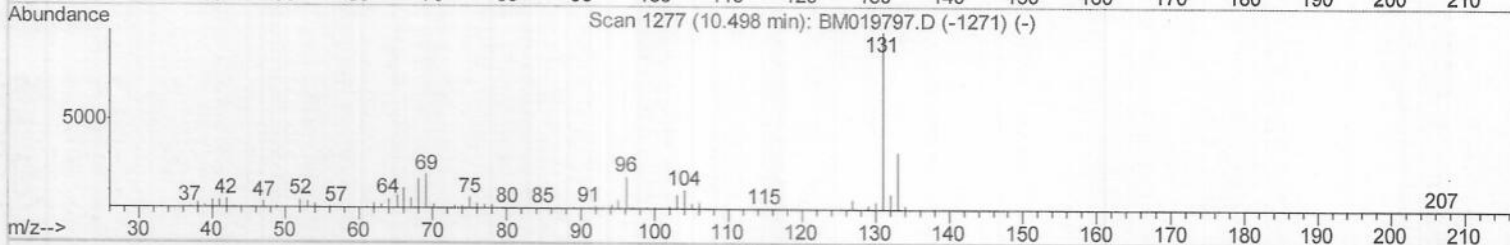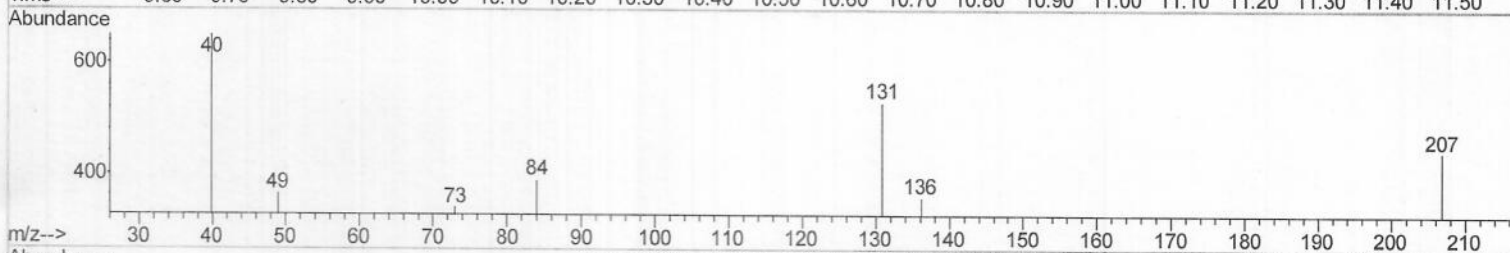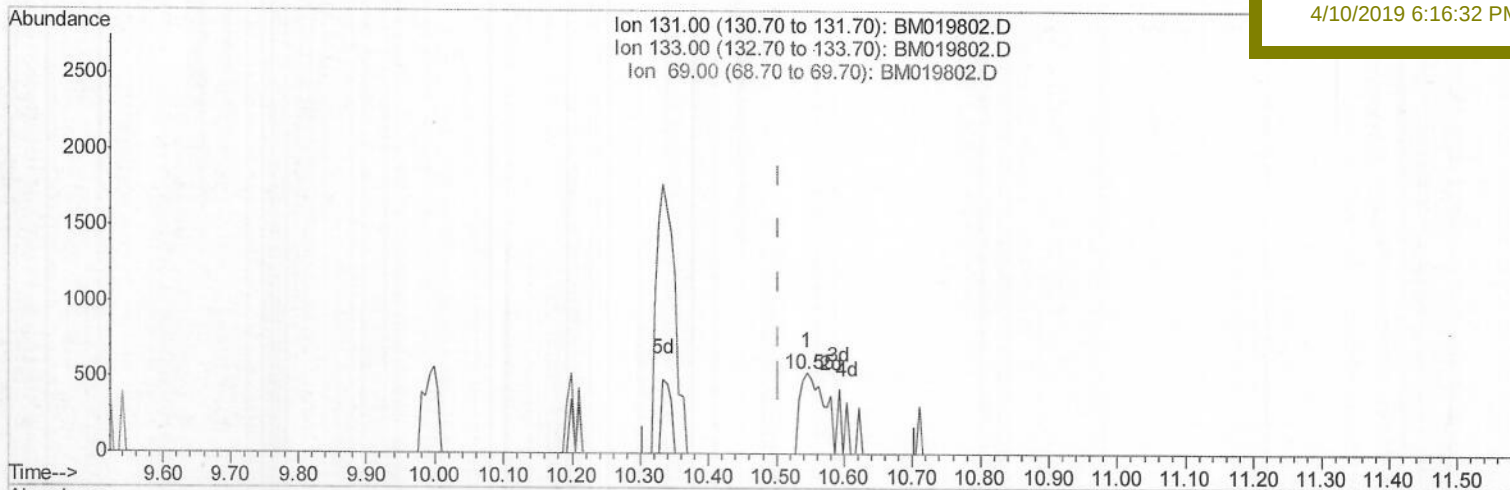

TIC: BM019802.D

(29) 4-Chloroaniline-d4 (S)

10.545min (+0.041) 0.15ng/ul m

response 1310

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	0.00#
69.00	18.60	0.00#
0.00	0.00	0.00

SJ
04/09/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019802.D
 Acq On : 08 Apr 2019 19:36
 Operator : JU/SJ
 Sample : K2269-01DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 09 08:25:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 07:14:39 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0BR2DL

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:32 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	103231	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	488591	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	305476	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	712185	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	763636	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	693844	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	413	0.16	ng/uL	0.02
5) Phenol-d5	6.77	99	9999	1.09	ng/ul	0.02
7) Bis-(2-Chloroethyl) ether-d	6.92	67	27583	4.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	32905	4.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	19999	2.90	ng/ul	0.02
19) Nitrobenzene-d5	8.73	128	19215	5.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	21636	5.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	39806	5.44	ng/ul	0.01
29) 4-Chloroaniline-d4	10.55	131	1310m	0.15	ng/ul	0.04
44) Dimethylphthalate-d6	13.65	166	171917	6.97	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	194633	6.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	957	0.25	ng/ul	0.14
58) Fluorene-d10	15.22	176	148190	6.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	15610	3.31	ng/ul	0.01
71) Anthracene-d10	17.08	188	246477	7.21	ng/ul	0.00
79) Pyrene-d10	19.39	212	293609	8.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	260273	7.08	ng/ul	0.00

Target Compounds					Qvalue
20) Nitrobenzene	8.77	77	289479	27.902 ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.01	216	25343	2.454 ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

57
 04/09/19