

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019793.D
 Acq On : 08 Apr 2019 14:05
 Operator : JU/SJ
 Sample : K2254-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC38

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:25 PM

Quant Time: Apr 09 07:03:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 06:31:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	123474	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	590441	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	351830	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	818946	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	815195	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	734236	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	18178	5.76	ng/uL	0.00
5) Phenol-d5	6.75	99	166158	15.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	113205	15.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	138930	16.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	128263	15.54	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	66051	15.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	71381	15.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	134431	15.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	175310	16.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	503949	17.75	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	577511	16.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	36193m	8.13	ng/ul	0.04
58) Fluorene-d10	15.22	176	440775	18.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	38185	7.05	ng/ul	0.00
71) Anthracene-d10	17.08	188	683943	17.40	ng/ul	0.00
79) Pyrene-d10	19.39	212	755563	20.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	617264	15.86	ng/ul	0.00

Target Compounds					Qvalue	
45) Dimethylphthalate	13.69	163	123656	4.341	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019793.D
Acq On : 08 Apr 2019 14:05
Operator : JU/SJ
Sample : K2254-15
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BFC38

Manual Integrations
APPROVED

Sohil
4/10/2019 6:16:25 PM

Quant Time: Apr 09 07:03:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 06:31:52 2019
Response via : Initial Calibration

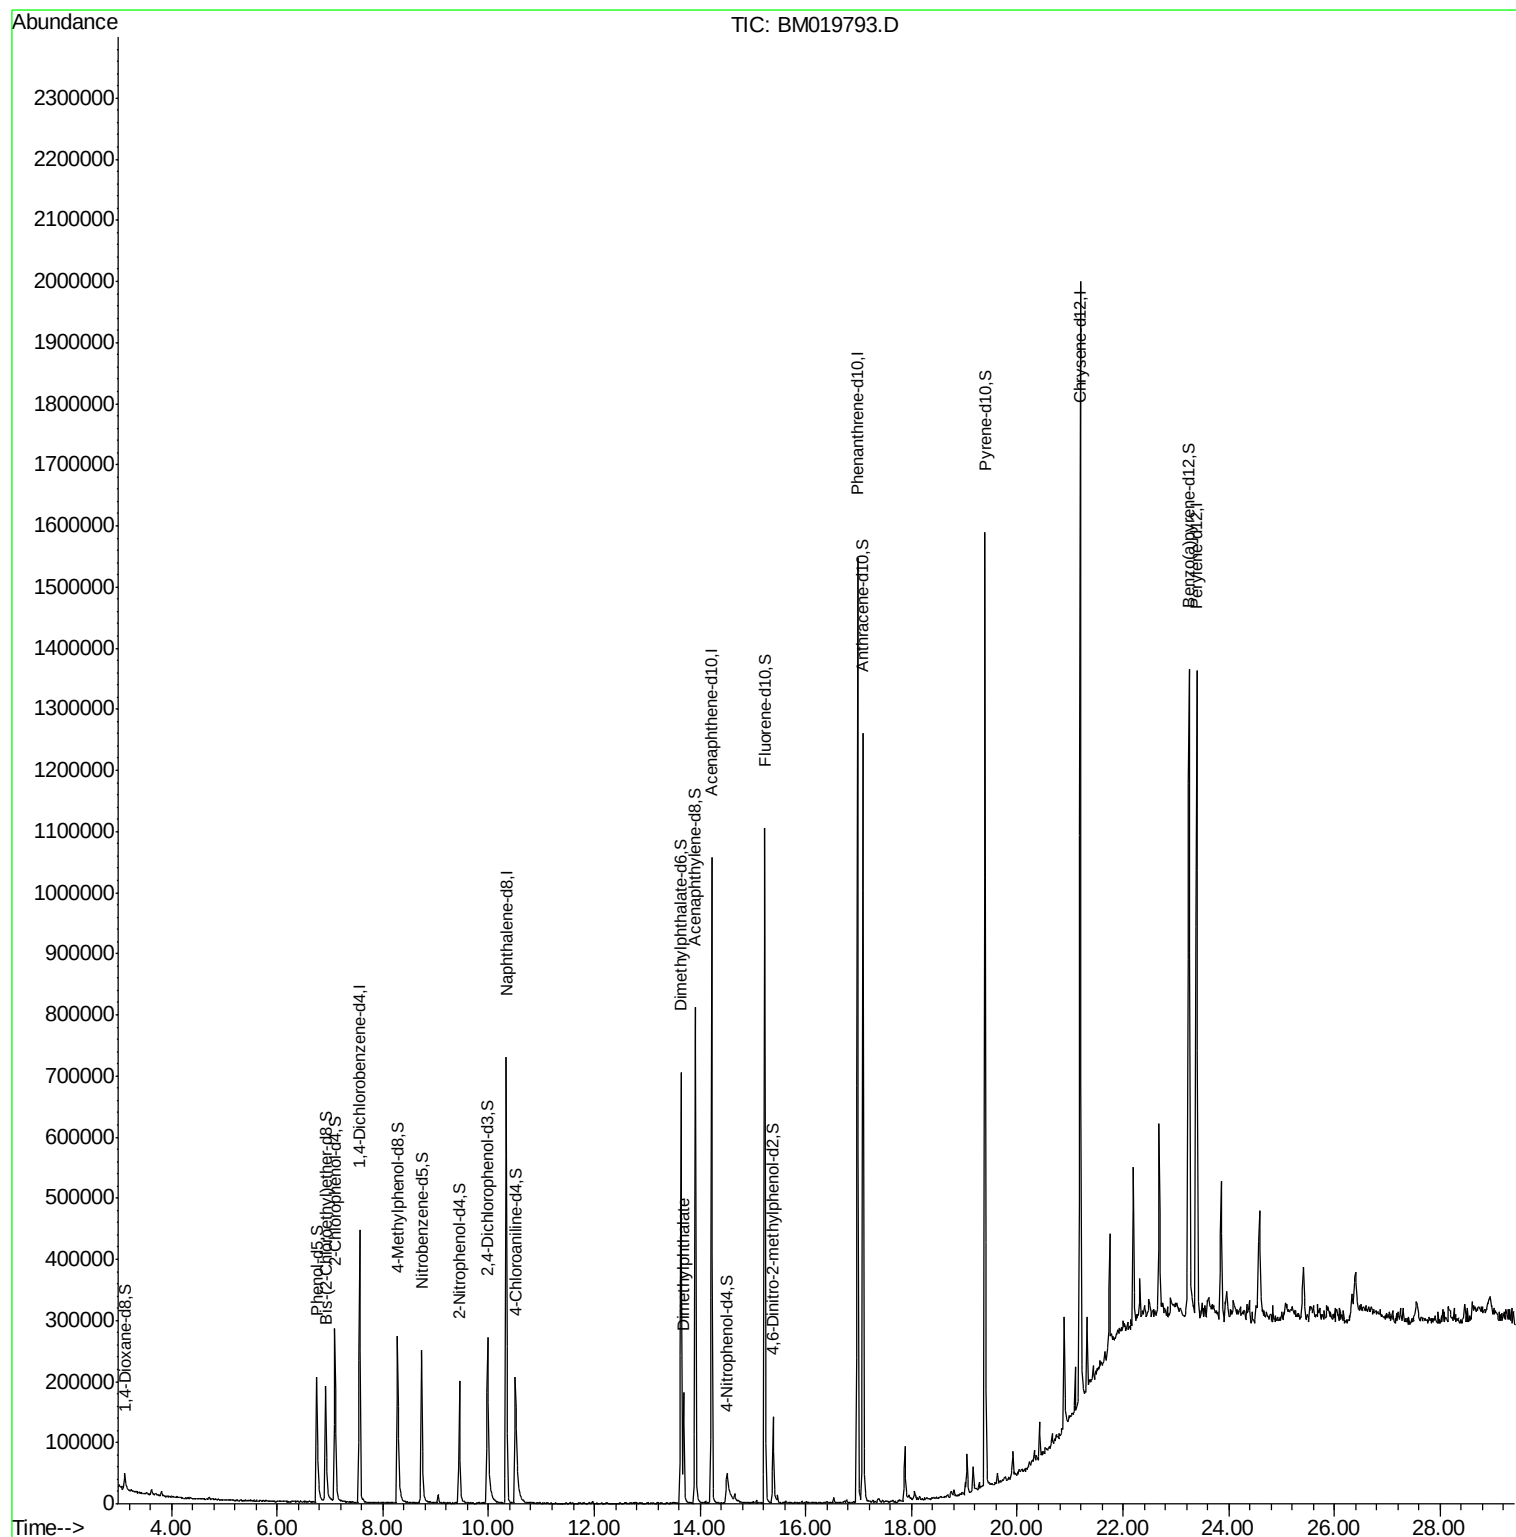

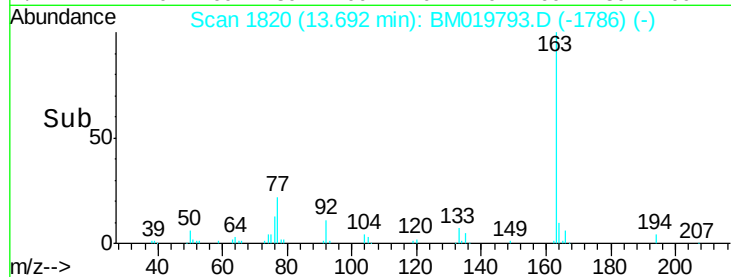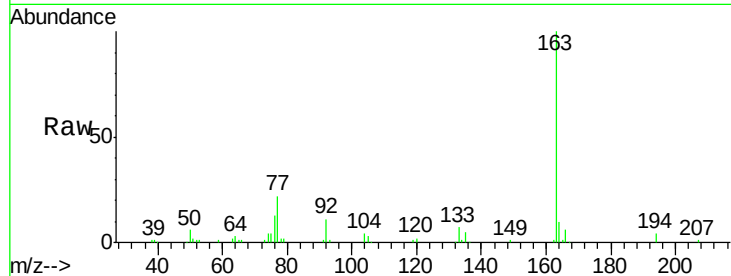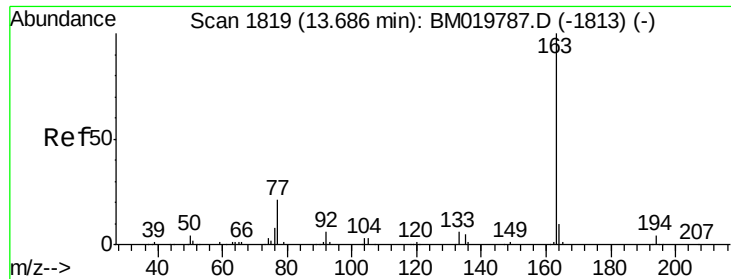

#45
 Dimethylphthalate
 Concen: 4.341 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BM019793.D
 Acq: 08 Apr 2019 14:05

Instrument :
 BNA_M
 ClientSampleId :
 BFC38

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	3.9	4.0	6.0#
164	9.9	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:25 PM

