

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019798.D
 Acq On : 08 Apr 2019 17:09
 Operator : JU/SJ
 Sample : K2254-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC32

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:29 PM

Quant Time: Apr 09 07:40:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 07:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	132924	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	623685	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	390244	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	893408	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	890508	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	782289	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	19478	5.74	ng/uL	0.00
5) Phenol-d5	6.75	99	156895	13.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	106661	13.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	132272	14.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	106410	11.98	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	65090	14.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	77395	15.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	138813	14.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	165588	14.76	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	497865	15.81	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	584655	14.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	50014m	10.13	ng/ul	0.03
58) Fluorene-d10	15.22	176	447278	16.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	55908	9.46	ng/ul	0.00
71) Anthracene-d10	17.08	188	667452	15.57	ng/ul	0.00
79) Pyrene-d10	19.39	212	693001	16.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	578767	13.96	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	106260	3.363	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019798.D
Acq On : 08 Apr 2019 17:09
Operator : JU/SJ
Sample : K2254-12
Misc :
ALS Vial : 12 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BFC32

Quant Time: Apr 09 07:40:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 07:14:39 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/10/2019 6:16:29 PM

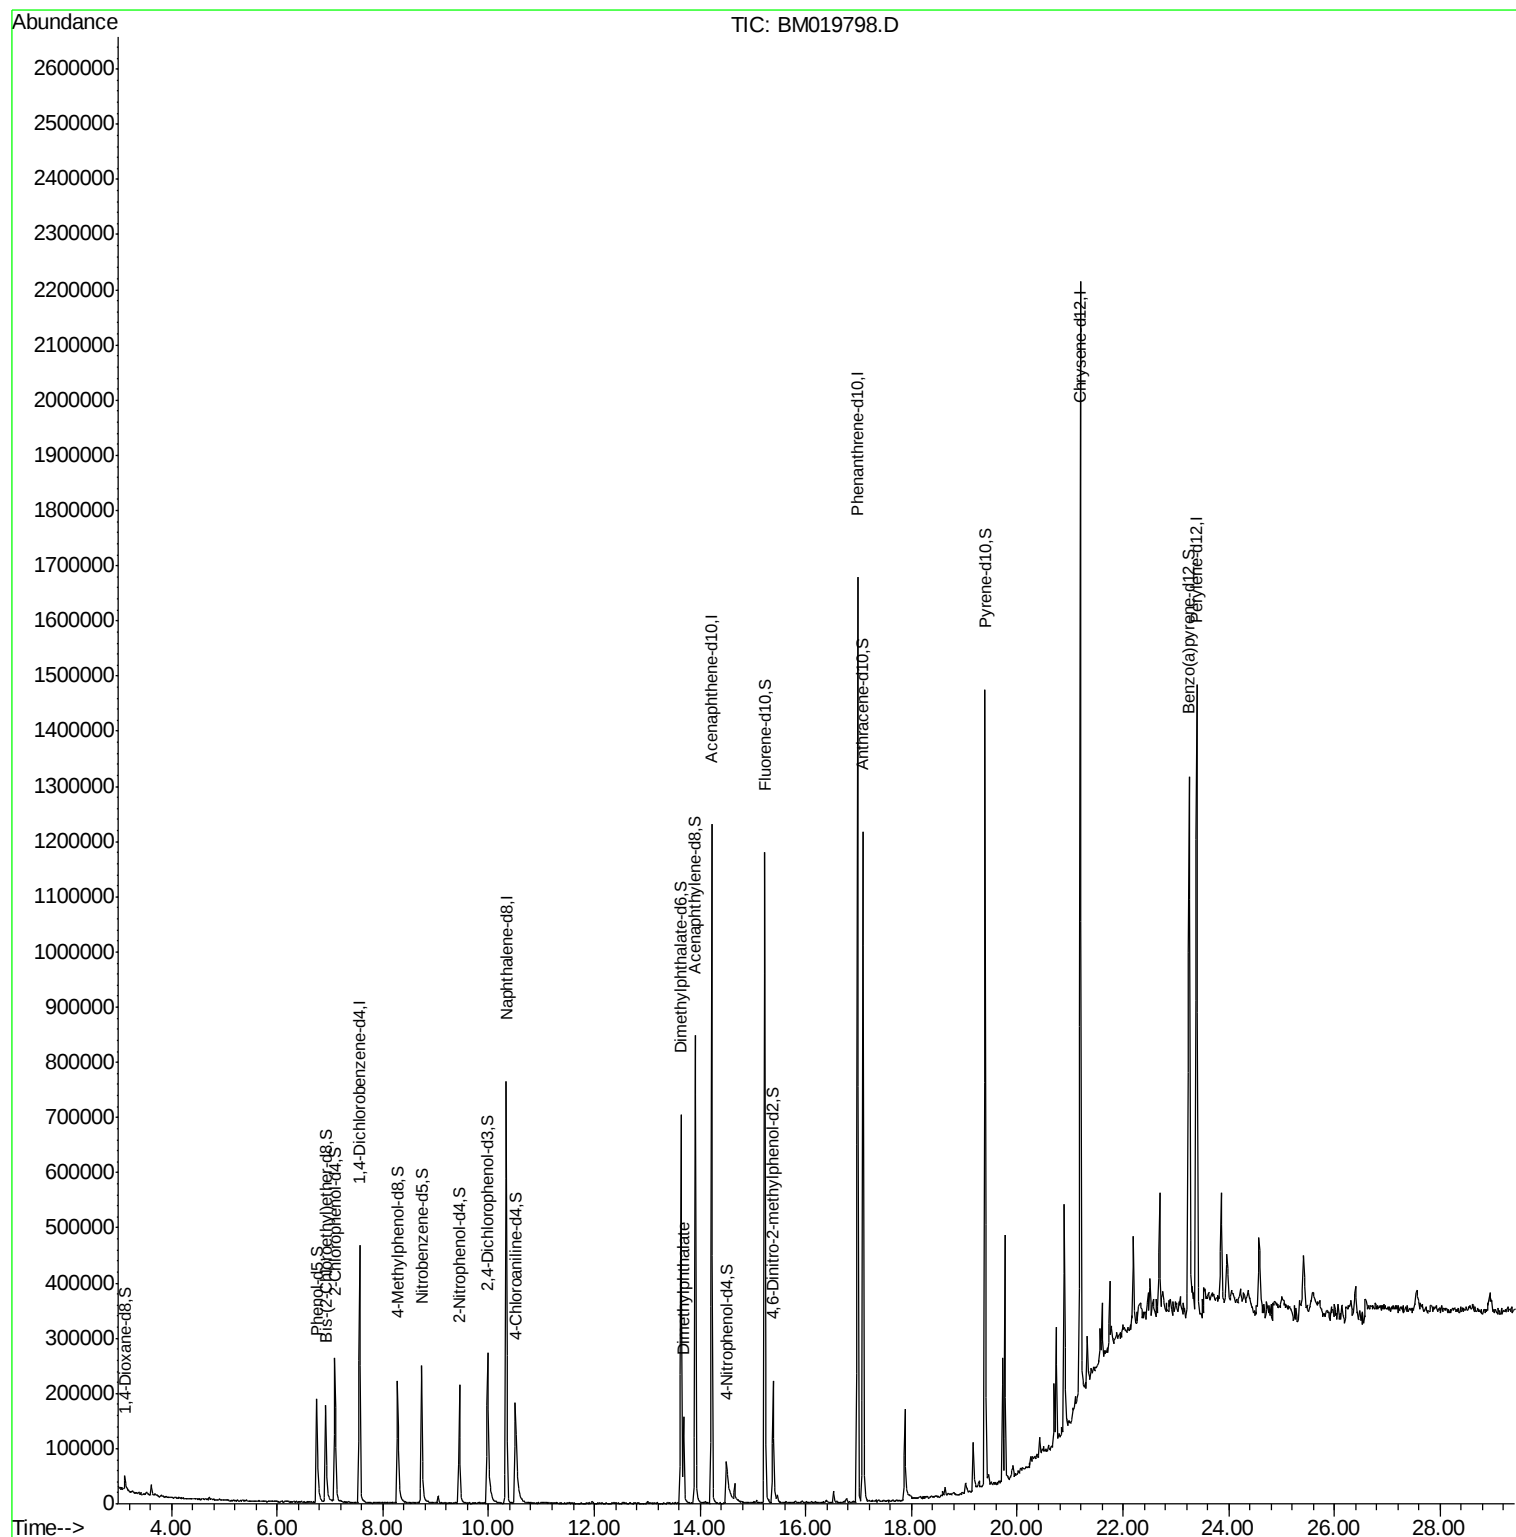

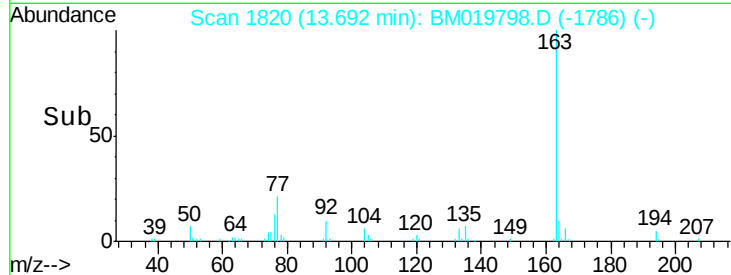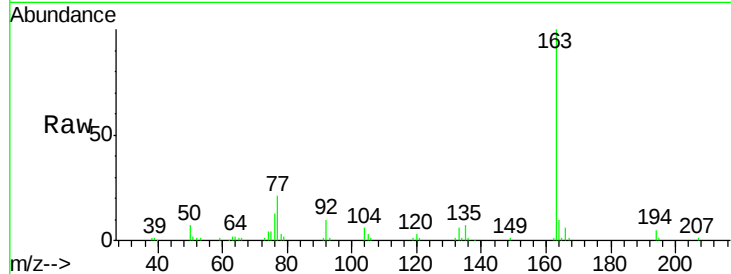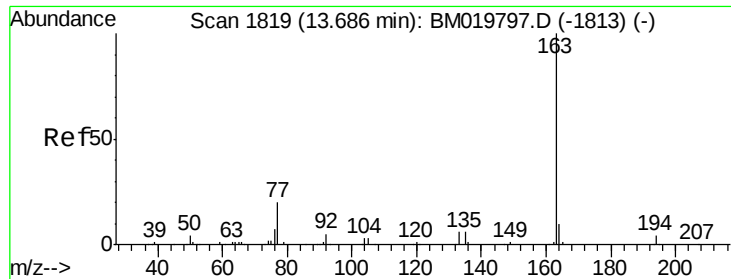

#45
 Dimethylphthalate
 Concen: 3.363 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. 0.00 min
 Lab File: BM019798.D
 Acq: 08 Apr 2019 17:09

Instrument :
 BNA_M
 ClientSampleId :
 BFC32

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.5	4.0	6.0
164	10.3	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:29 PM

