

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019799.D
 Acq On : 08 Apr 2019 17:46
 Operator : JU/SJ
 Sample : K2254-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC33

Quant Time: Apr 09 07:17:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 07:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	141740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	655357	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	388366	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	911767	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	935079	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	846456	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	18277	5.05	ng/uL	0.00
5) Phenol-d5	6.75	99	173911	13.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	114940	13.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	144879	15.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	110815	11.70	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	69937	14.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	81768	15.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	137246	13.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	176674	14.99	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	510425	16.29	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	608572	15.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	39075	7.95	ng/ul	0.03
58) Fluorene-d10	15.22	176	457776	16.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	48648	8.07	ng/ul	0.00
71) Anthracene-d10	17.08	188	657407	15.03	ng/ul	0.00
79) Pyrene-d10	19.39	212	731102	16.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	593969	13.24	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.69	163	107584	3.422	ng/ul#	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019799.D
Acq On : 08 Apr 2019 17:46
Operator : JU/SJ
Sample : K2254-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC33

Quant Time: Apr 09 07:17:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 07:14:39 2019
Response via : Initial Calibration

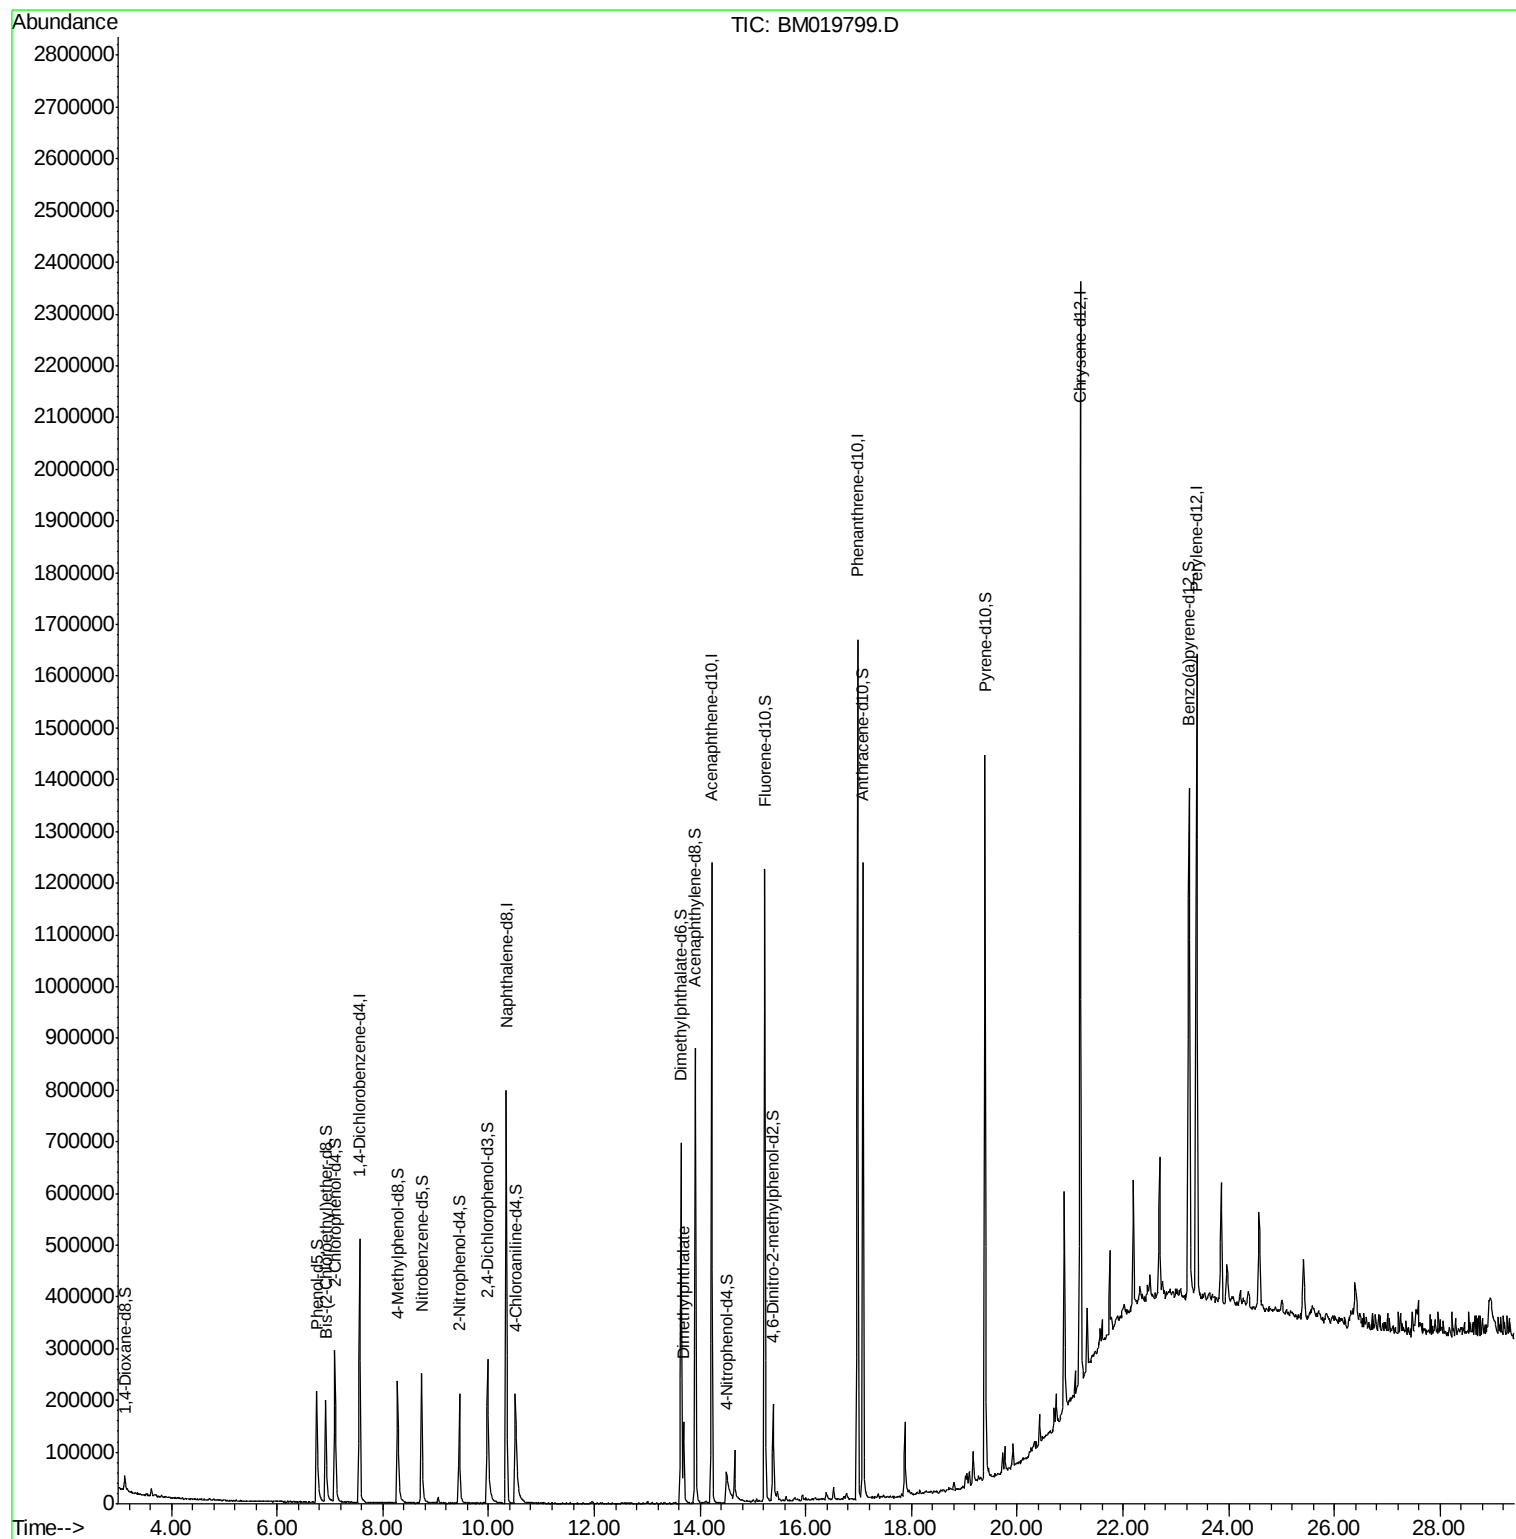

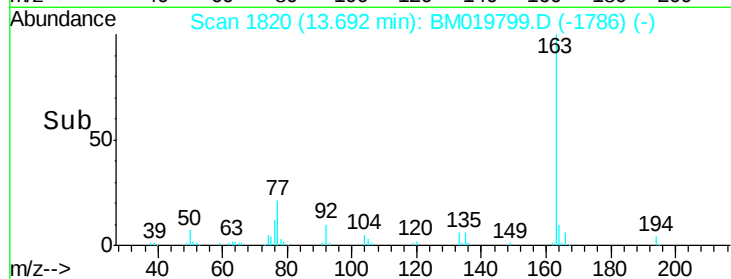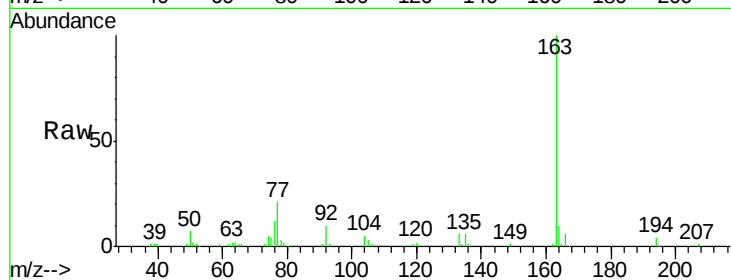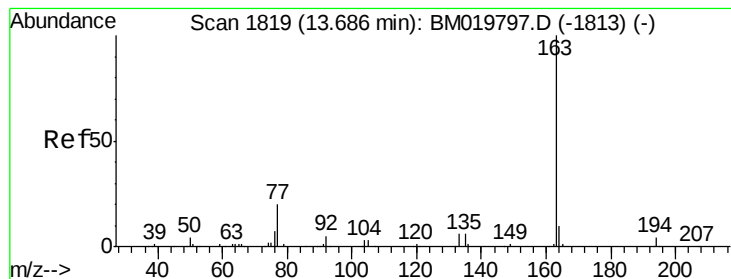

#45

Dimethylphthalate

Concen: 3.422 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BM019799.D

Acq: 08 Apr 2019 17:46

Instrument :

BNA_M

ClientSampleId :

BFC33

Tgt Ion:163 Resp: 107584

Ion Ratio Lower Upper

163 100

194 4.0 4.0 6.0#

164 10.2 8.4 12.6

