

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019804.D
 Acq On : 08 Apr 2019 20:49
 Operator : JU/SJ
 Sample : K2217-15DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF605DL

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:33 PM

Quant Time: Apr 09 08:38:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 07:14:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	113691	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	544670	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	336168	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	789846	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	830513	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	750595	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	2007m	0.69	ng/uL	0.01
5) Phenol-d5	6.76	99	24475m	2.42	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.93	67	23230	3.43	ng/ul	0.01
9) 2-Chlorophenol-d4	7.10	132	23518	3.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	10426m	1.37	ng/ul	0.03
19) Nitrobenzene-d5	8.75	128	13346m	3.43	ng/ul	0.01
22) 2-Nitrophenol-d4	9.45	143	14522m	3.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	19740m	2.42	ng/ul	0.05
29) 4-Chloroaniline-d4	10.55	131	20832	2.13	ng/ul	0.05
44) Dimethylphthalate-d6	13.65	166	105673	3.90	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	120659	3.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	2296	0.54	ng/ul	0.09
58) Fluorene-d10	15.23	176	94959	4.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	5717	1.09	ng/ul	0.02
71) Anthracene-d10	17.08	188	141978	3.75	ng/ul	0.00
79) Pyrene-d10	19.39	212	163992	4.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	140088	3.52	ng/ul	0.00

Target Compounds					Qvalue	
84) Bis(2-ethylhexyl)phthalate	21.10	149	1283491	44.760	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019804.D
Acq On : 08 Apr 2019 20:49
Operator : JU/SJ
Sample : K2217-15DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF605DL

Manual Integrations
APPROVED

Sohil
4/10/2019 6:16:33 PM

Quant Time: Apr 09 08:38:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 07:14:39 2019
Response via : Initial Calibration

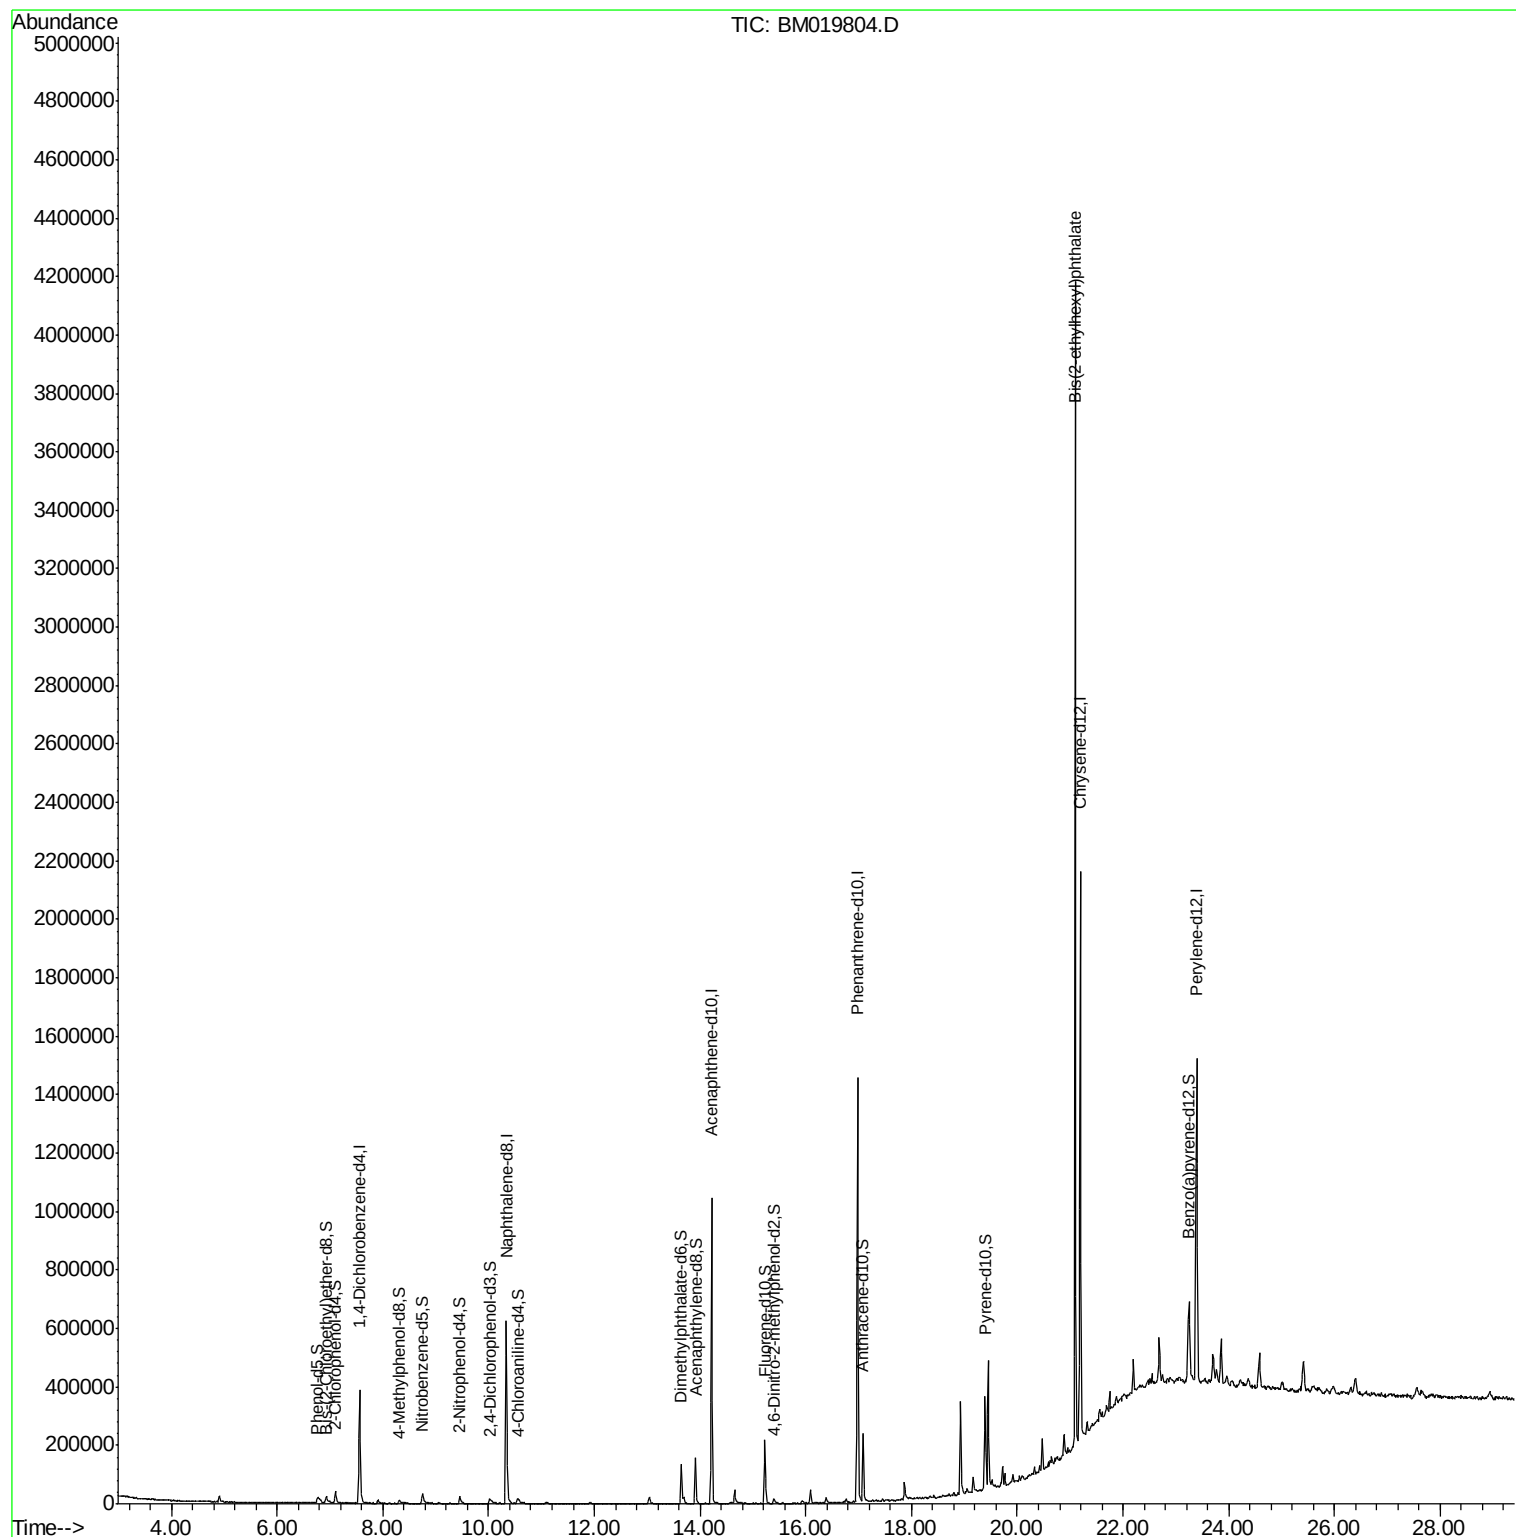

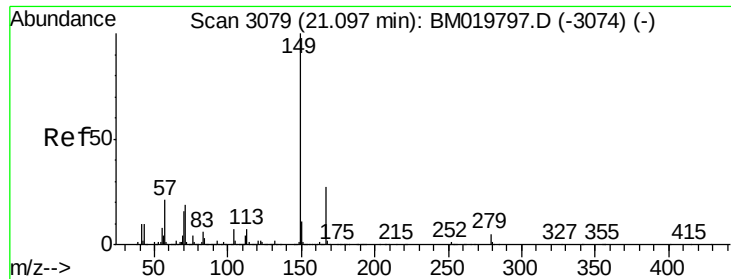

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 44.760 ng/ul
 RT: 21.10 min Scan# 3079
 Delta R.T. -0.00 min
 Lab File: BM019804.D
 Acq: 08 Apr 2019 20:49

Instrument :
 BNA_M
 ClientSampleId :
 BF605DL

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	1283491		
167	26.6		23.0	34.6
279	4.5		4.3	6.5

Manual Integrations
 APPROVED

Sohil
 4/10/2019 6:16:33 PM

