

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019812.D
 Acq On : 09 Apr 2019 01:42
 Operator : JU/SJ
 Sample : K2254-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	19	22	34	rVB	42821	68916	3.00%	0.309%
2	3.528	89	92	99	rVB4	7743	11129	0.48%	0.050%
3	3.616	104	107	116	rBV	33008	46647	2.03%	0.209%
4	3.810	136	140	146	rBV3	12161	18259	0.79%	0.082%
5	4.057	180	182	184	rBV2	3450	2734	0.12%	0.012%
6	4.181	201	203	205	rBV2	2594	2462	0.11%	0.011%
7	4.363	232	234	236	rBV3	2770	2532	0.11%	0.011%
8	4.704	289	292	295	rBV	4958	5297	0.23%	0.024%
9	6.092	525	528	531	rBV4	1817	2427	0.11%	0.011%
10	6.751	634	640	659	rBV	168201	369374	16.06%	1.658%
11	6.916	662	668	679	rBV	168528	308655	13.42%	1.386%
12	7.092	692	698	715	rVB	256096	441147	19.18%	1.981%
13	7.557	770	777	786	rBV	560062	949807	41.29%	4.265%
14	8.281	894	900	918	rBV	164957	351668	15.29%	1.579%
15	8.733	970	977	996	rBV	198992	389539	16.93%	1.749%
16	9.045	1024	1030	1036	rVV2	16126	27323	1.19%	0.123%
17	9.122	1040	1043	1045	rVB2	2081	2326	0.10%	0.010%
18	9.439	1091	1097	1111	rBV	162017	318759	13.86%	1.431%
19	9.833	1161	1164	1168	rVB2	2245	3625	0.16%	0.016%
20	9.875	1168	1171	1174	rBV	2392	3632	0.16%	0.016%
21	9.980	1182	1189	1210	rBV	191894	468743	20.38%	2.105%
22	10.333	1242	1249	1265	rBV	793453	1320669	57.41%	5.930%
23	10.516	1273	1280	1294	rBV	108926	301095	13.09%	1.352%
24	11.898	1511	1515	1522	rBV	15169	31048	1.35%	0.139%
25	11.951	1522	1524	1529	rVB3	3297	4827	0.21%	0.022%
26	13.004	1701	1703	1710	rVB2	2623	3340	0.15%	0.015%
27	13.639	1805	1811	1816	rBV	471677	697075	30.30%	3.130%
28	13.686	1816	1819	1829	rVB	121360	197987	8.61%	0.889%
29	13.910	1851	1857	1871	rBV	535512	837551	36.41%	3.761%
30	14.092	1887	1888	1895	rBV3	2223	3025	0.13%	0.014%
31	14.215	1903	1909	1919	rBV2	1017637	1605049	69.77%	7.207%
32	14.515	1953	1960	1977	rBV4	36645	157650	6.85%	0.708%
33	14.651	1977	1983	1990	rVB5	27806	51474	2.24%	0.231%
34	15.004	2041	2043	2048	rVB2	5514	6354	0.28%	0.029%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
 Data File : BM019812.D
 Acq On : 09 Apr 2019 01:42
 Operator : JU/SJ
 Sample : K2254-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	15.057	2048	2052	2055	rBV3	4166	5854	0.25%	0.026%
36	15.221	2074	2080	2089	rBV	742658	1107742	48.15%	4.974%
37	15.386	2102	2108	2118	rBV	83786	156639	6.81%	0.703%
38	15.462	2118	2121	2126	rVB4	9250	12925	0.56%	0.058%
39	15.580	2137	2141	2144	rBV3	2093	2939	0.13%	0.013%
40	15.745	2162	2169	2170	rBV4	1814	2843	0.12%	0.013%
41	15.798	2177	2178	2181	rVB2	3540	2778	0.12%	0.012%
42	15.833	2181	2184	2187	rVB3	1908	2393	0.10%	0.011%
43	15.874	2187	2191	2195	rBV2	1569	3349	0.15%	0.015%
44	15.927	2196	2200	2202	rVV4	3587	4846	0.21%	0.022%
45	15.951	2202	2204	2207	rVB3	2279	2393	0.10%	0.011%
46	16.009	2212	2214	2220	rVB3	2384	3289	0.14%	0.015%
47	16.109	2226	2231	2232	rBV3	3219	4065	0.18%	0.018%
48	16.180	2240	2243	2245	rVB2	2921	2862	0.12%	0.013%
49	16.274	2255	2259	2262	rVB3	1620	2441	0.11%	0.011%
50	16.333	2265	2269	2270	rBV2	2884	3147	0.14%	0.014%
51	16.386	2275	2278	2283	rVV3	9236	13911	0.60%	0.062%
52	16.445	2286	2288	2291	rBV4	2871	3032	0.13%	0.014%
53	16.533	2299	2303	2306	rBV3	7611	10691	0.46%	0.048%
54	16.580	2308	2311	2314	rVB	2935	2596	0.11%	0.012%
55	16.651	2322	2323	2326	rBV3	3417	3592	0.16%	0.016%
56	16.721	2331	2335	2337	rBV3	3355	5086	0.22%	0.023%
57	16.756	2337	2341	2342	rBV2	3865	4128	0.18%	0.019%
58	16.774	2342	2344	2347	rVB	6424	4675	0.20%	0.021%
59	16.798	2347	2348	2355	rVB4	4889	6294	0.27%	0.028%
60	16.851	2355	2357	2360	rBV2	3002	3164	0.14%	0.014%
61	16.886	2360	2363	2368	rBV4	2996	5204	0.23%	0.023%
62	16.980	2373	2379	2384	rBV2	1304642	1830457	79.57%	8.219%
63	17.021	2384	2386	2391	rVV	113256	134111	5.83%	0.602%
64	17.080	2391	2396	2407	rVB	802768	1110049	48.25%	4.984%
65	17.274	2425	2429	2431	rVB4	3729	4154	0.18%	0.019%
66	17.462	2458	2461	2464	rVB4	2599	3477	0.15%	0.016%
67	17.574	2476	2480	2483	rBV4	3912	5040	0.22%	0.023%
68	17.868	2523	2530	2536	rBV3	106690	173914	7.56%	0.781%
69	17.951	2540	2544	2549	rVB	57103	73642	3.20%	0.331%
70	18.045	2557	2560	2561	rBV3	7344	7301	0.32%	0.033%
71	18.374	2614	2616	2620	rBV4	4446	5095	0.22%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019812.D
Acq On : 09 Apr 2019 01:42
Operator : JU/SJ
Sample : K2254-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Title : SVOA CALIBRATION

72	18.439	2625	2627	2631	rVB6	9481	10497	0.46%	0.047%
73	19.021	2723	2726	2727	rBV3	14805	14128	0.61%	0.063%
74	19.050	2727	2731	2736	rVB	98991	147888	6.43%	0.664%
75	19.162	2746	2750	2760	rBV	74715	131934	5.74%	0.592%
76	19.392	2783	2789	2797	rBV	885924	1400525	60.88%	6.288%
77	19.450	2797	2799	2804	rVB	44412	59184	2.57%	0.266%
78	19.721	2842	2845	2849	rBV	86187	99347	4.32%	0.446%
79	19.762	2849	2852	2856	rVB	133320	138881	6.04%	0.624%
80	20.327	2945	2948	2951	rVB2	53825	59428	2.58%	0.267%
81	20.703	3009	3012	3014	rBV	44841	47446	2.06%	0.213%
82	20.733	3015	3017	3021	rVV2	66328	70250	3.05%	0.315%
83	20.886	3040	3043	3052	rVB4	114099	166471	7.24%	0.747%
84	21.186	3089	3094	3100	rBV	1568329	2132091	92.68%	9.573%
85	23.250	3438	3445	3461	rVB2	799375	1751133	76.12%	7.863%
86	23.391	3463	3469	3481	rVB2	1191047	2300487	100.00%	10.329%


Sum of corrected areas: 22271953

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019812.D
Acq On : 09 Apr 2019 01:42
Operator : JU/SJ
Sample : K2254-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC37

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

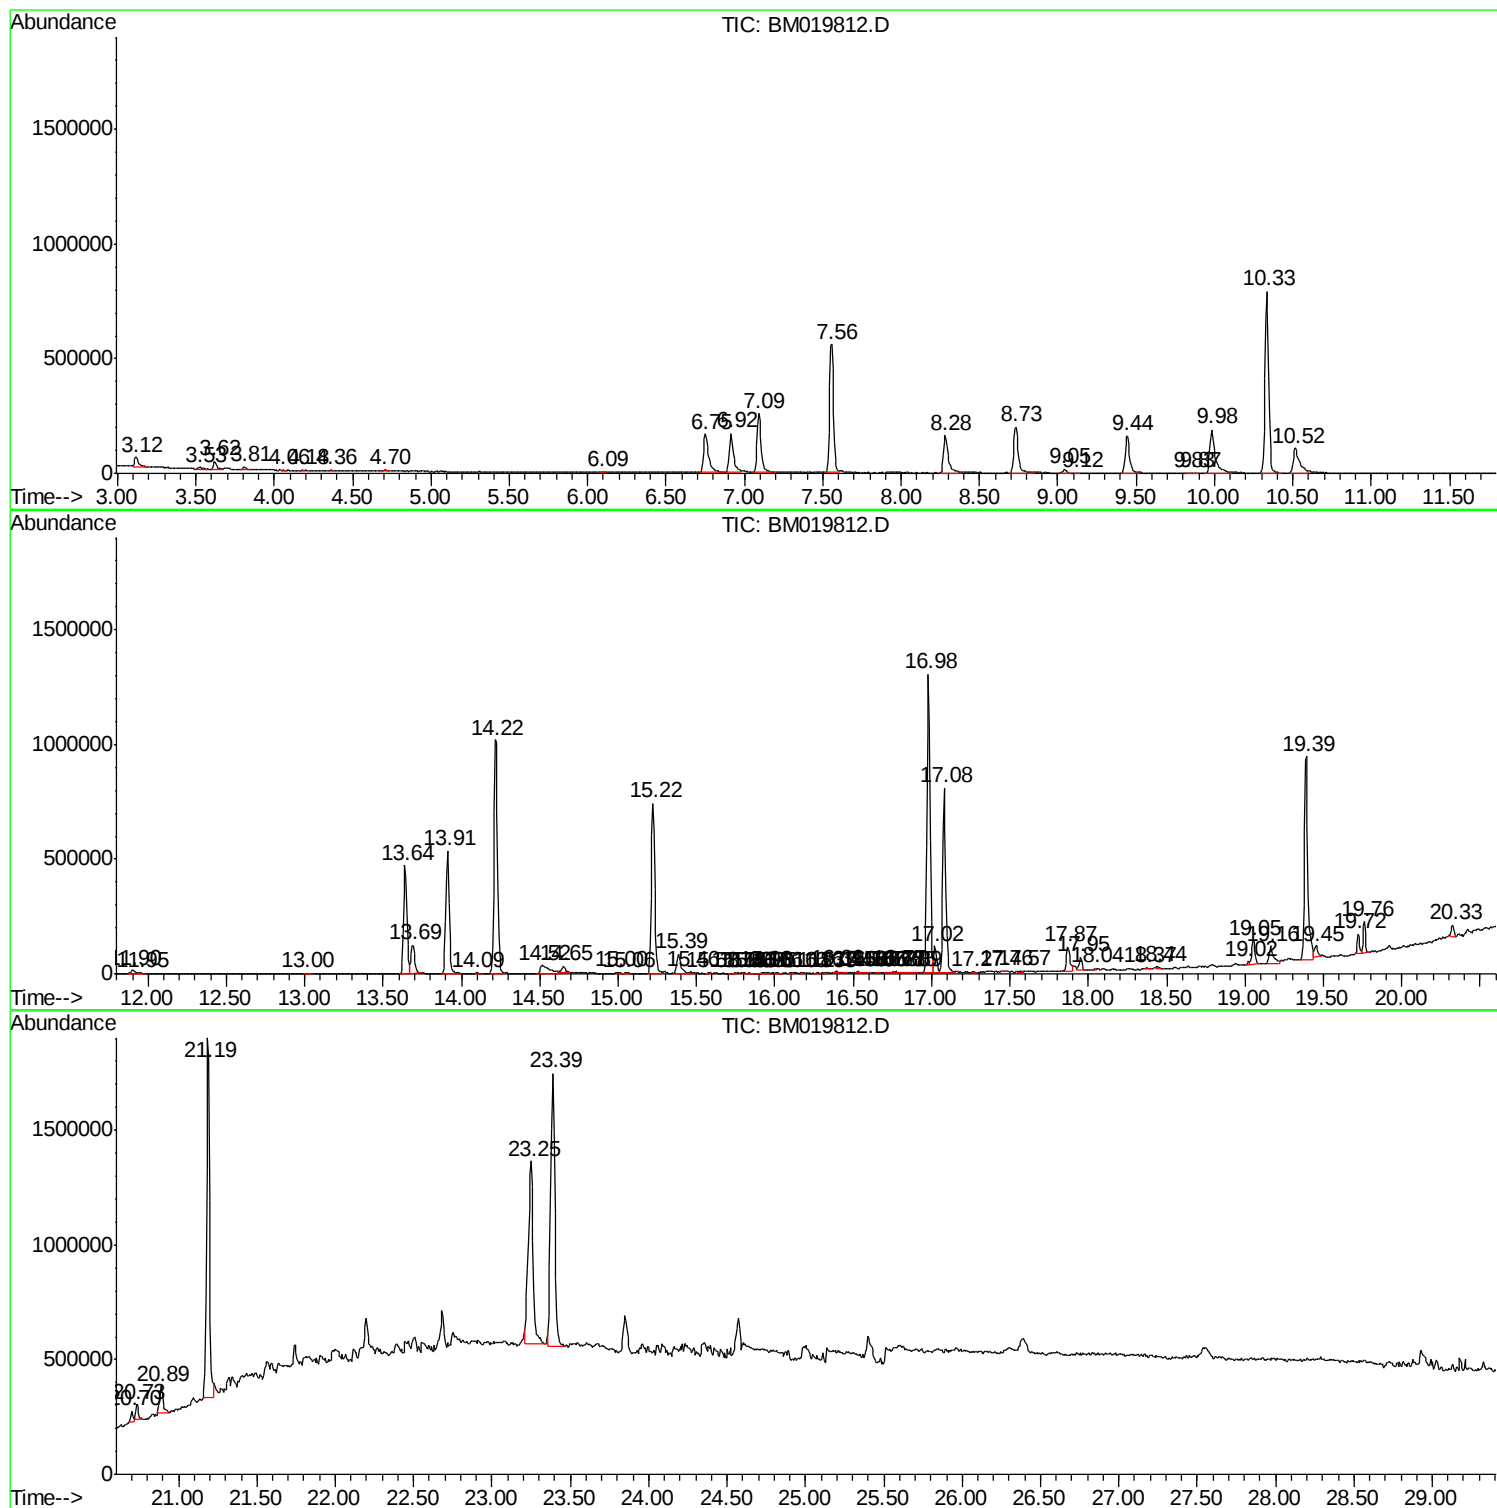

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019812.D
Acq On : 09 Apr 2019 01:42
Operator : JU/SJ
Sample : K2254-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC37

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040819\
Data File : BM019812.D
Acq On : 09 Apr 2019 01:42
Operator : JU/SJ
Sample : K2254-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFC37

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc