




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 03:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

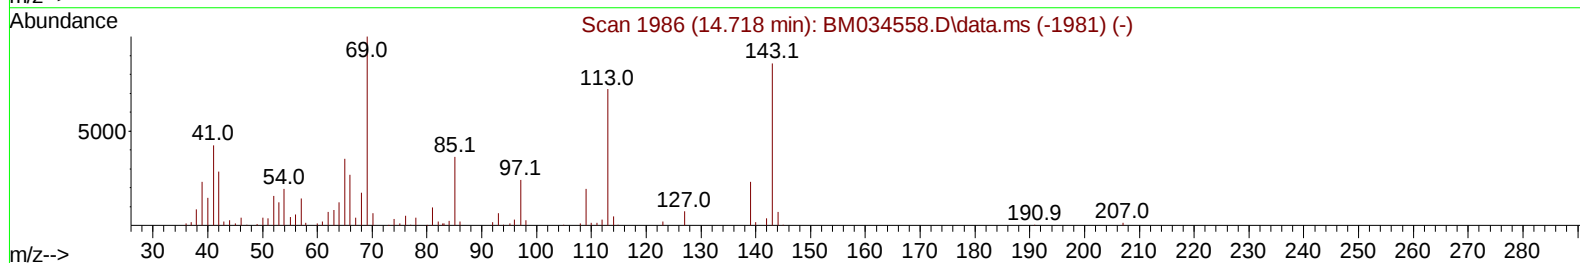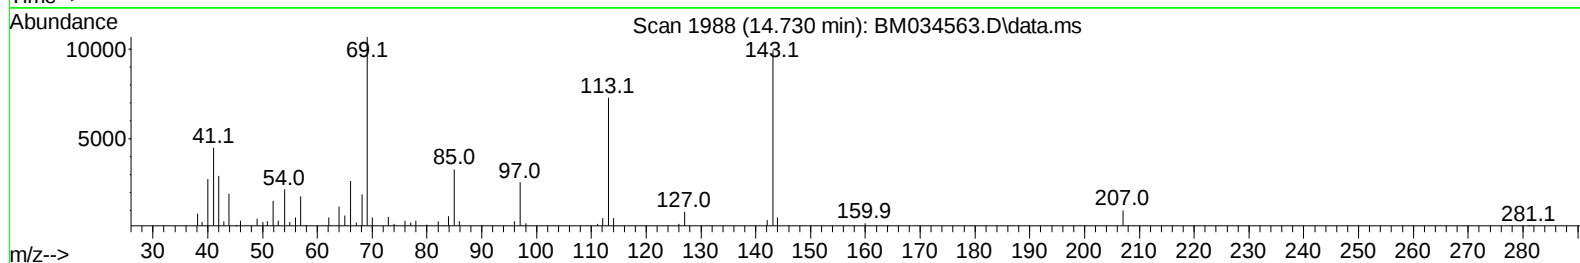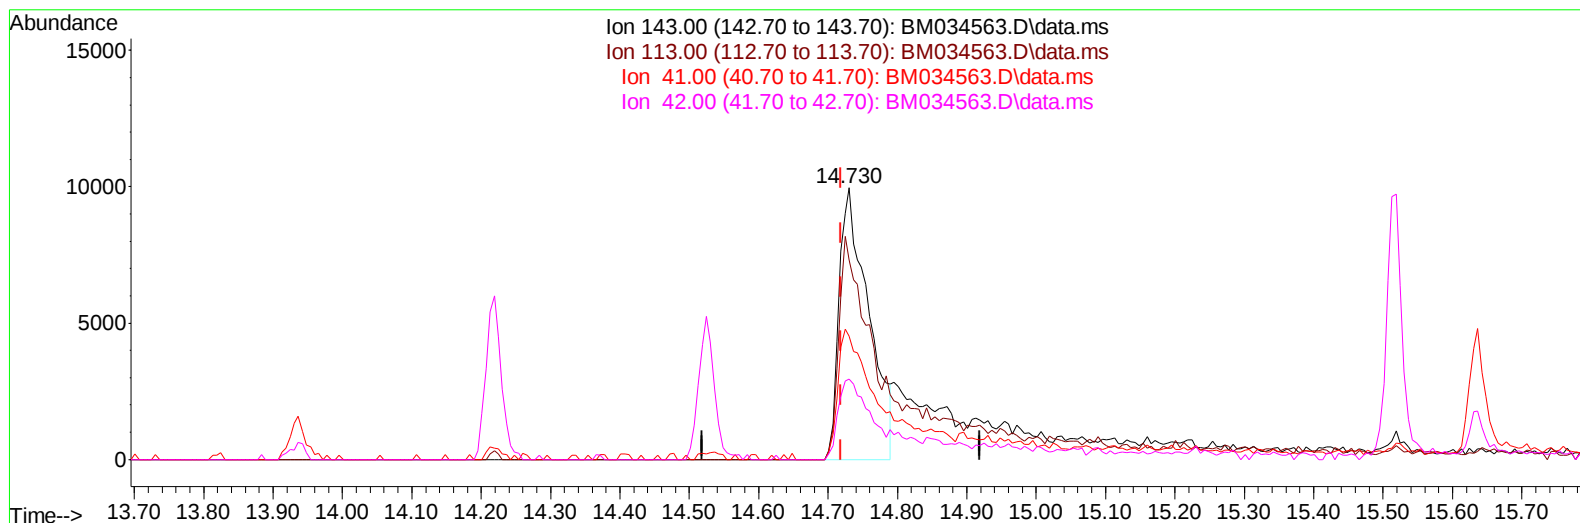

TIC: BM034563.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.730min (+ 0.012) 12.99 ng/u1

response 29261

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	73.34
41.00	31.90	45.31#
42.00	19.10	29.59#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

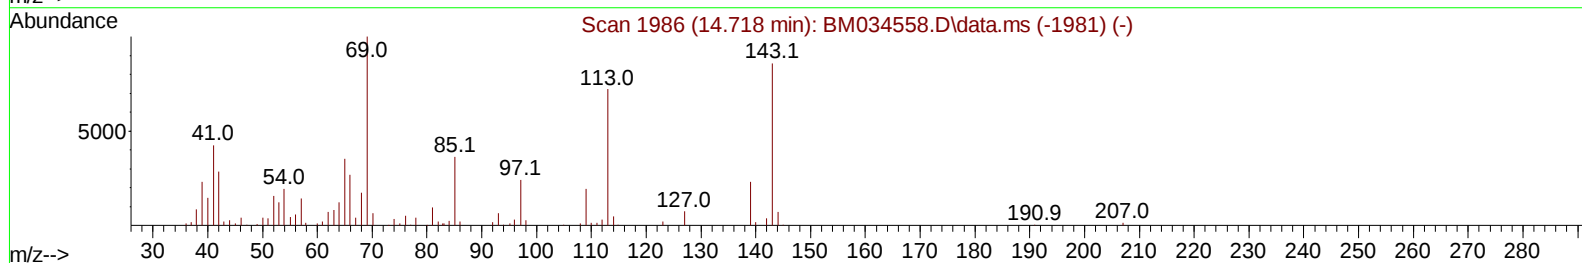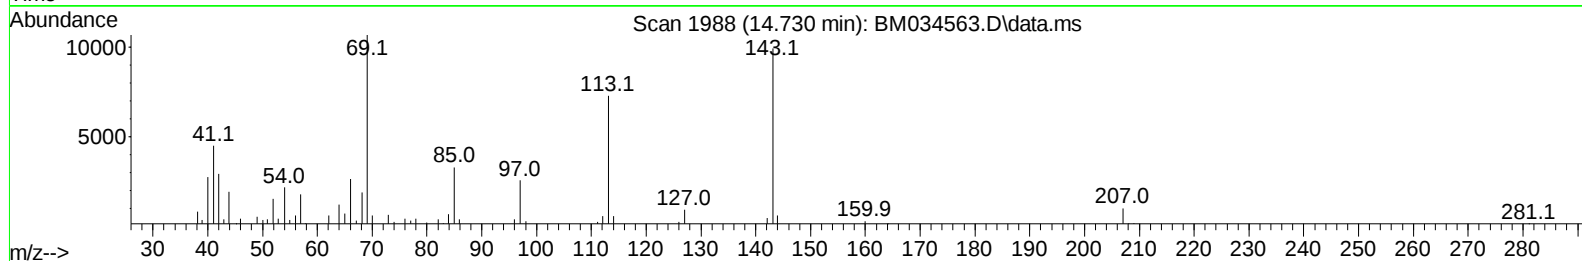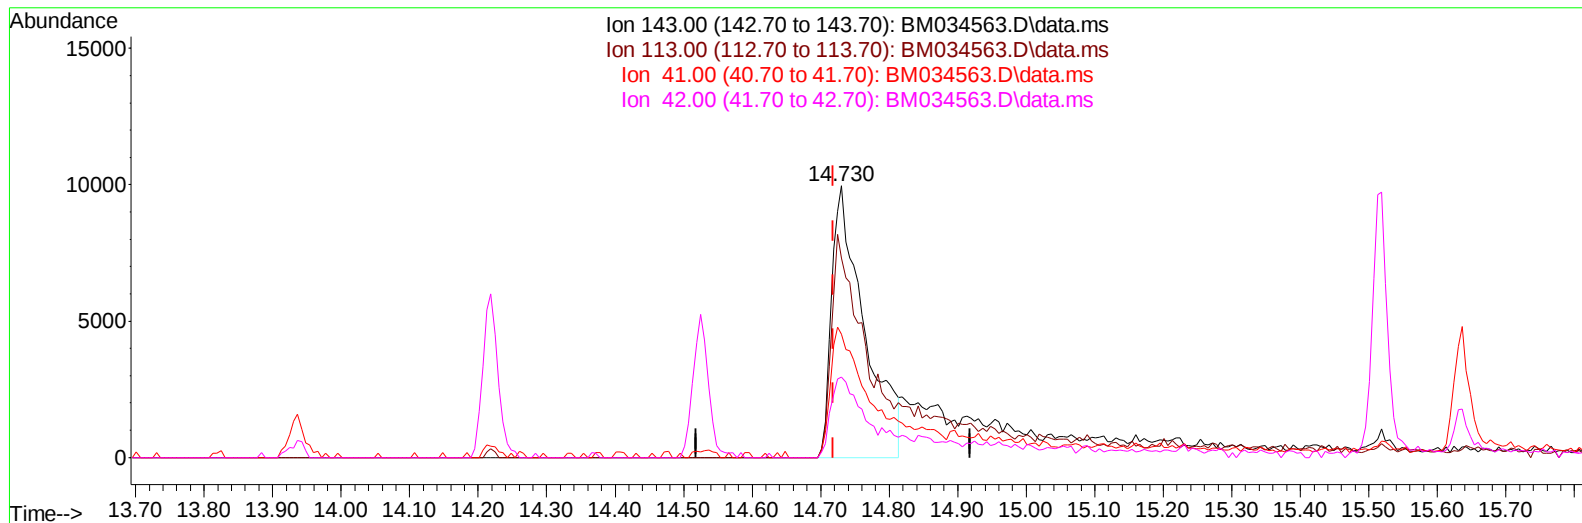

TIC: BM034563.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.730min (+ 0.012) 14.57 ng/ul m

response 32836

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	73.34
41.00	31.90	45.31#
42.00	19.10	29.59#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034563.D
 Acq On : 08 Apr 2022 16:06
 Operator : CG/JU
 Sample : PB143957BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK957

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

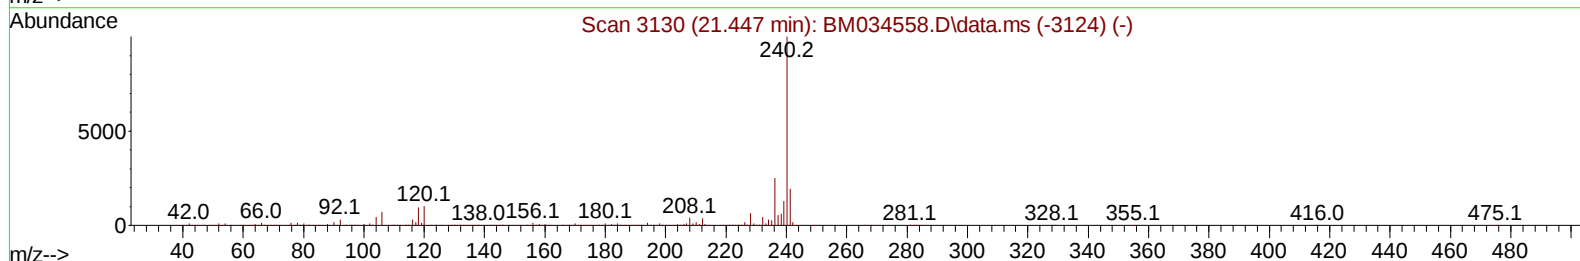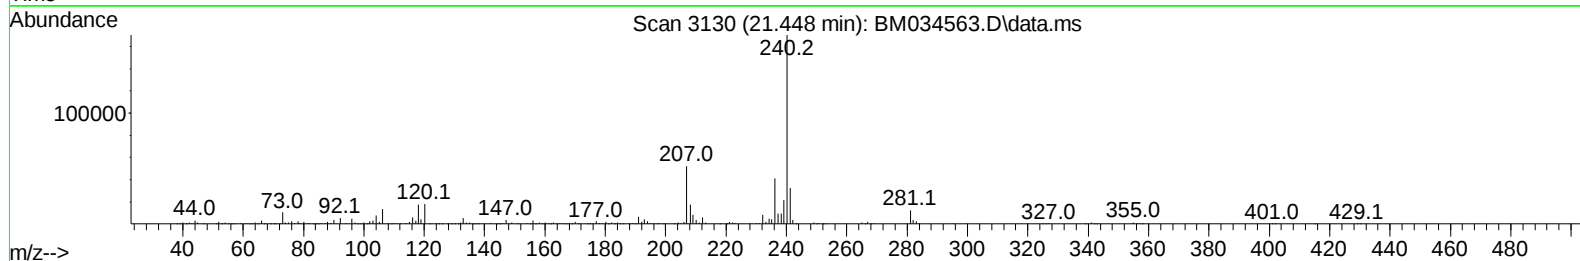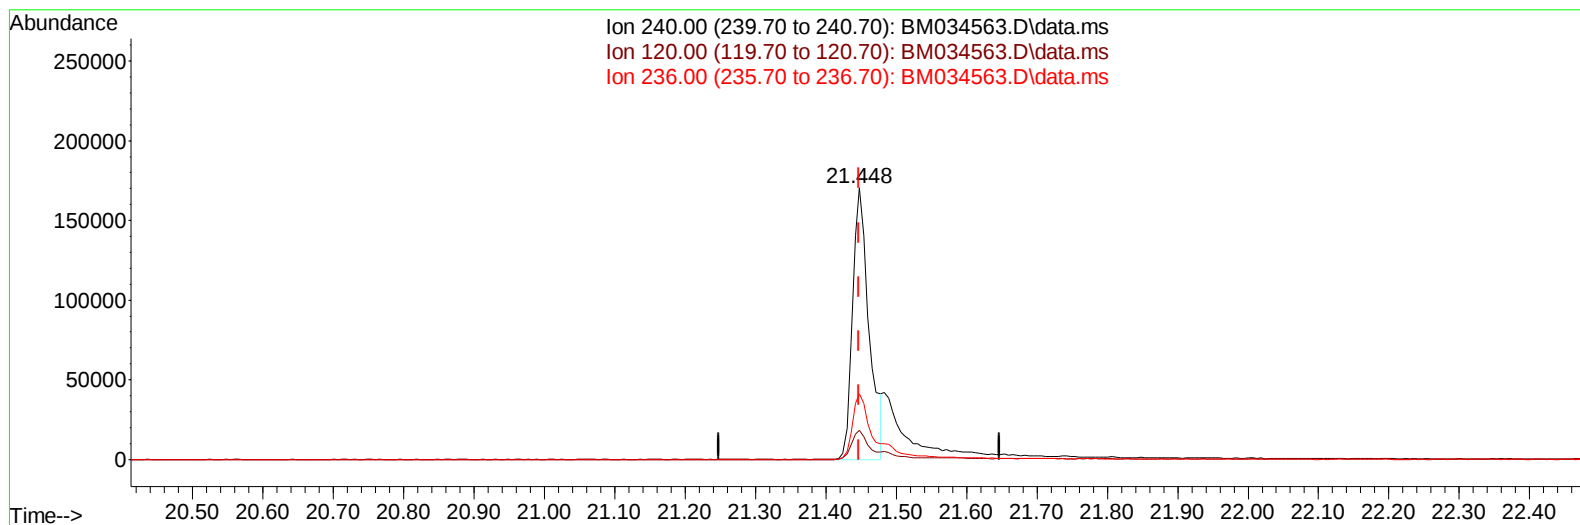

TIC: BM034563.D\data.ms

(79) Chrysene-d12 (I)

21.448min (+ 0.000) 20.00 ng/u1

response 274843

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.66#
236.00	24.80	24.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034563.D
 Acq On : 08 Apr 2022 16:06
 Operator : CG/JU
 Sample : PB143957BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK957

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

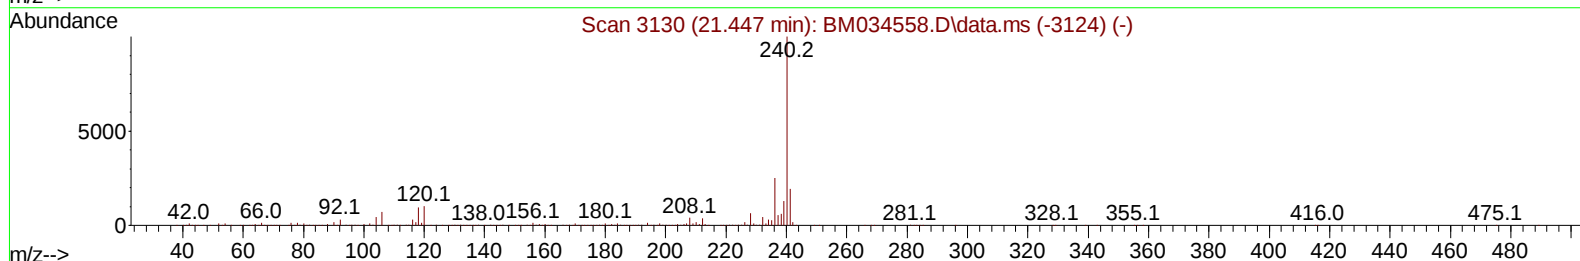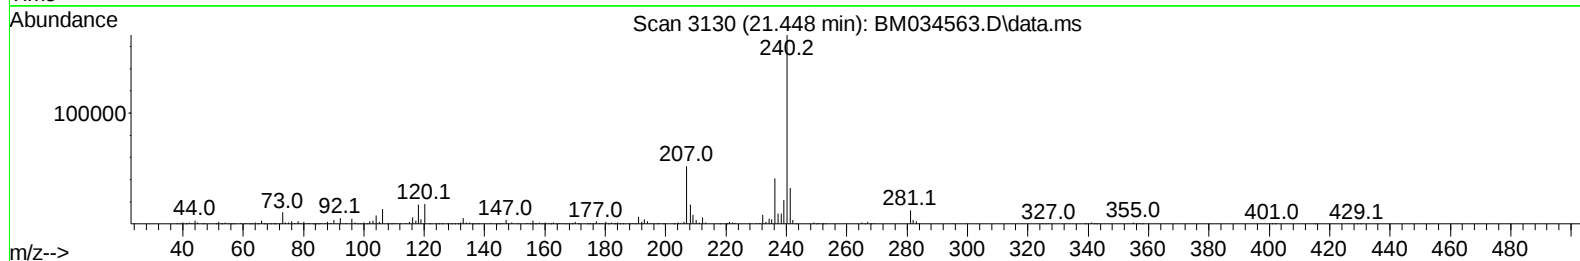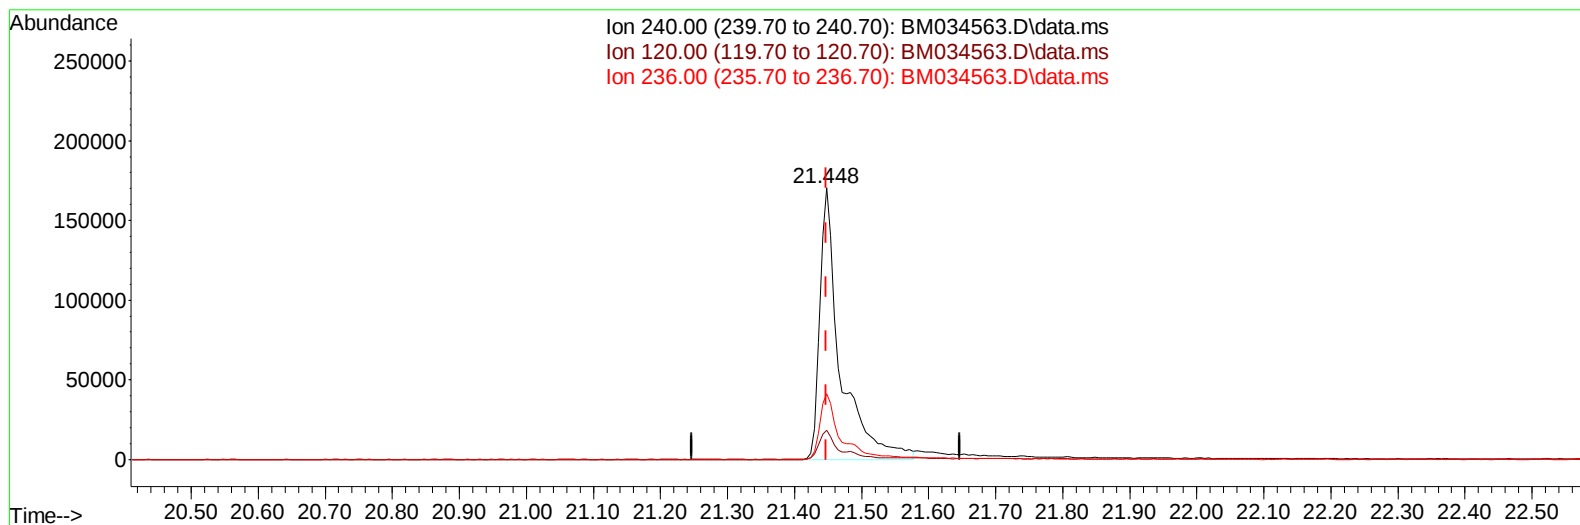

TIC: BM034563.D\data.ms

(79) Chrysene-d12 (I)

21.448min (+ 0.000) 20.00 ng/ul m

response 363904

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.66#
236.00	24.80	24.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034563.D
 Acq On : 08 Apr 2022 16:06
 Operator : CG/JU
 Sample : PB143957BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK957

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 03:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	91241	20.000	ng/ul	0.00
20) Naphthalene-d8	10.690	136	366808	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.525	164	204484	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.266	188	398454	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.448	240	363904m	20.000	ng/ul	0.00
88) Perylene-d12	23.824	264	425585	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.249	96	18188	7.108	ng/uL	0.00
4) Pyridine-d5	3.678	84	199739	32.347	ng/ul	0.00
7) Phenol-d5	7.037	99	230797	30.392	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.202	67	172946	34.176	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132	202768	34.540	ng/ul	0.00
15) 4-Methylphenol-d8	8.590	113	190764	32.158	ng/ul	0.00
21) Nitrobenzene-d5	9.043	128	92912	34.465	ng/ul	0.00
24) 2-Nitrophenol-d4	9.772	143	95153	33.902	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.313	165	158344	29.961	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131	213714	29.311	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	536433	36.305	ng/ul	0.00
49) Acenaphthylene-d8	14.219	160	630210	33.185	ng/ul	0.00
54) 4-Nitrophenol-d4	14.730	143	32836m	14.575	ng/ul	0.01
60) Fluorene-d10	15.519	176	451857	35.388	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	67229	27.638	ng/ul	0.00
73) Anthracene-d10	17.366	188	683523	35.980	ng/ul	0.00
81) Pyrene-d10	19.660	212	780902	39.317	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264	735233	34.344	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 03:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

