




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

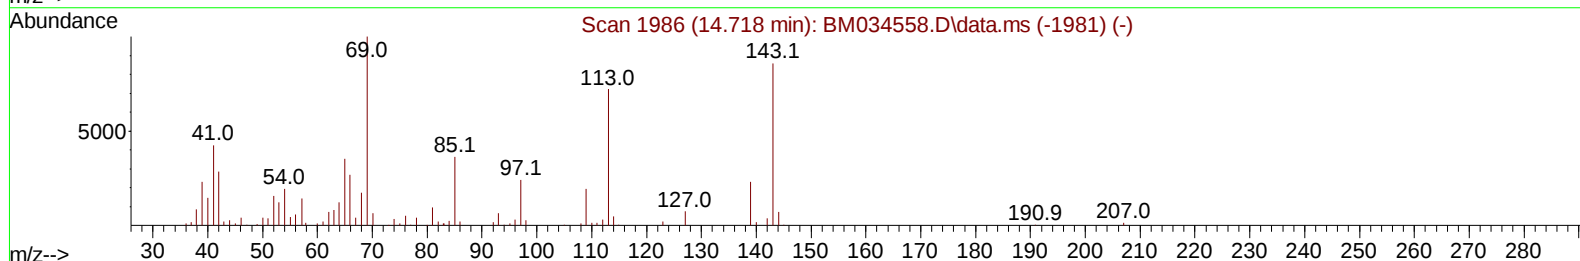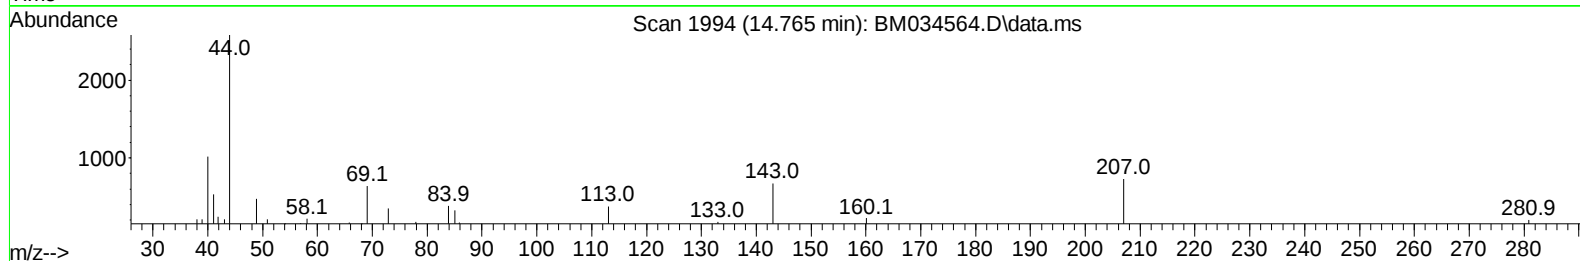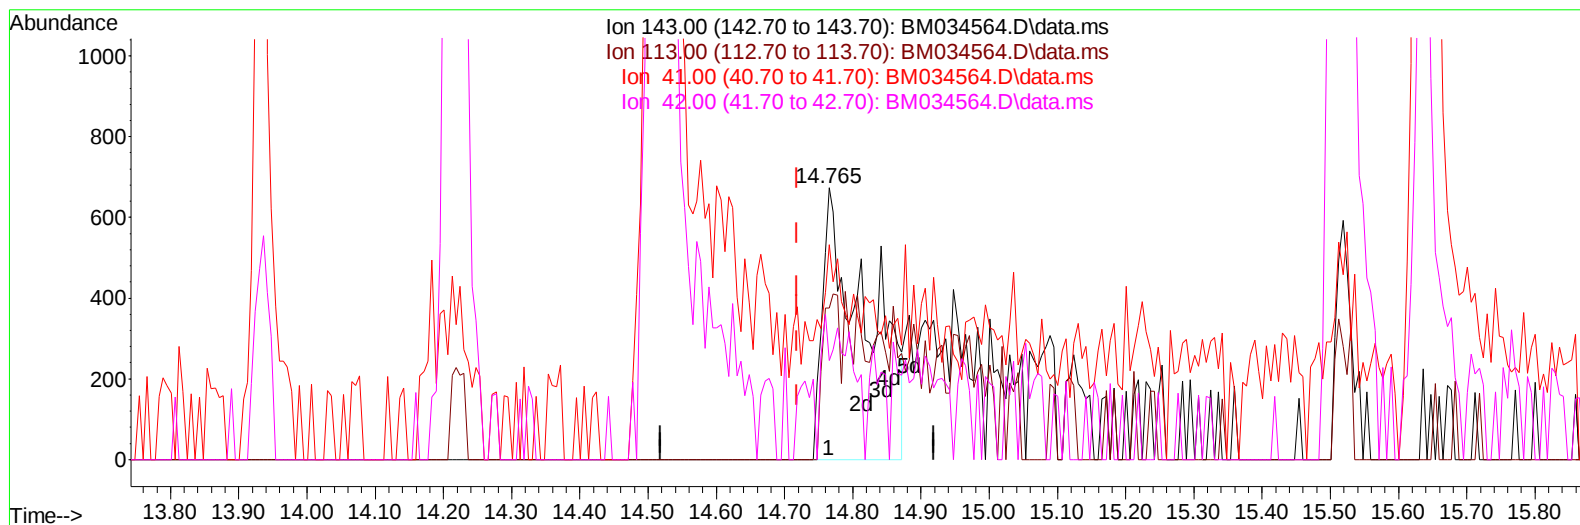

TIC: BM034564.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.765min (+ 0.047) 1.37 ng/ul m

response 2948

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	55.87#
41.00	31.90	79.05#
42.00	19.10	36.40#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

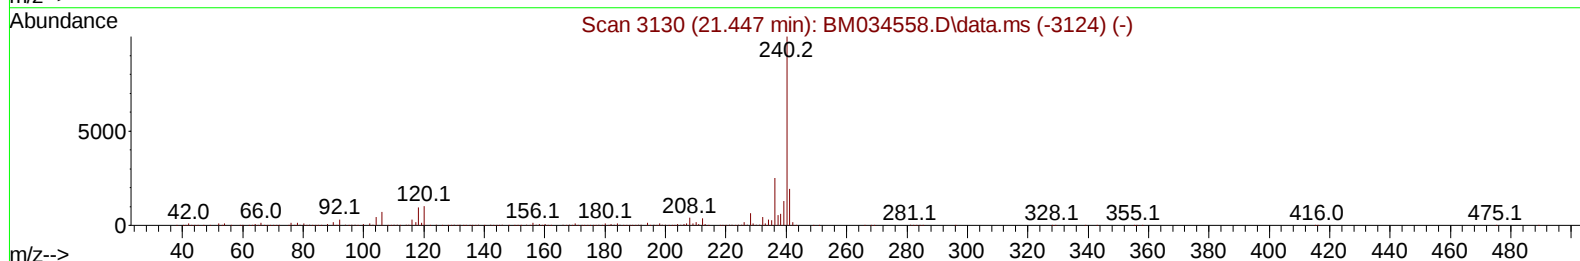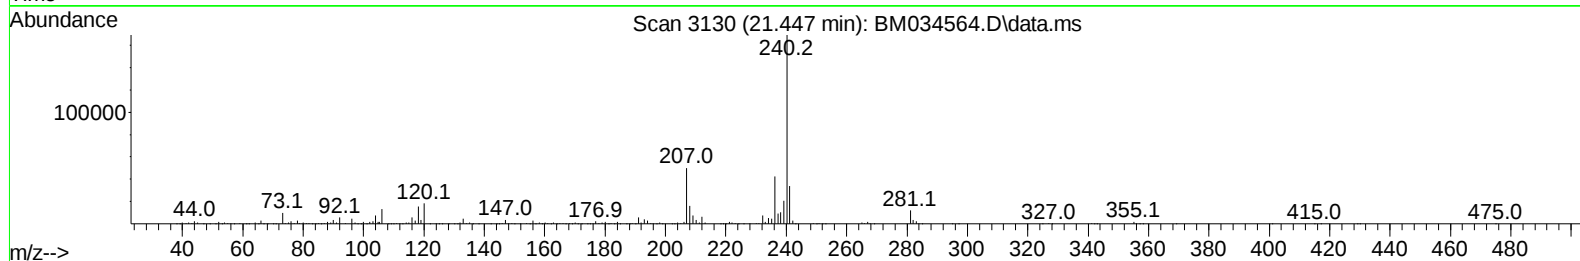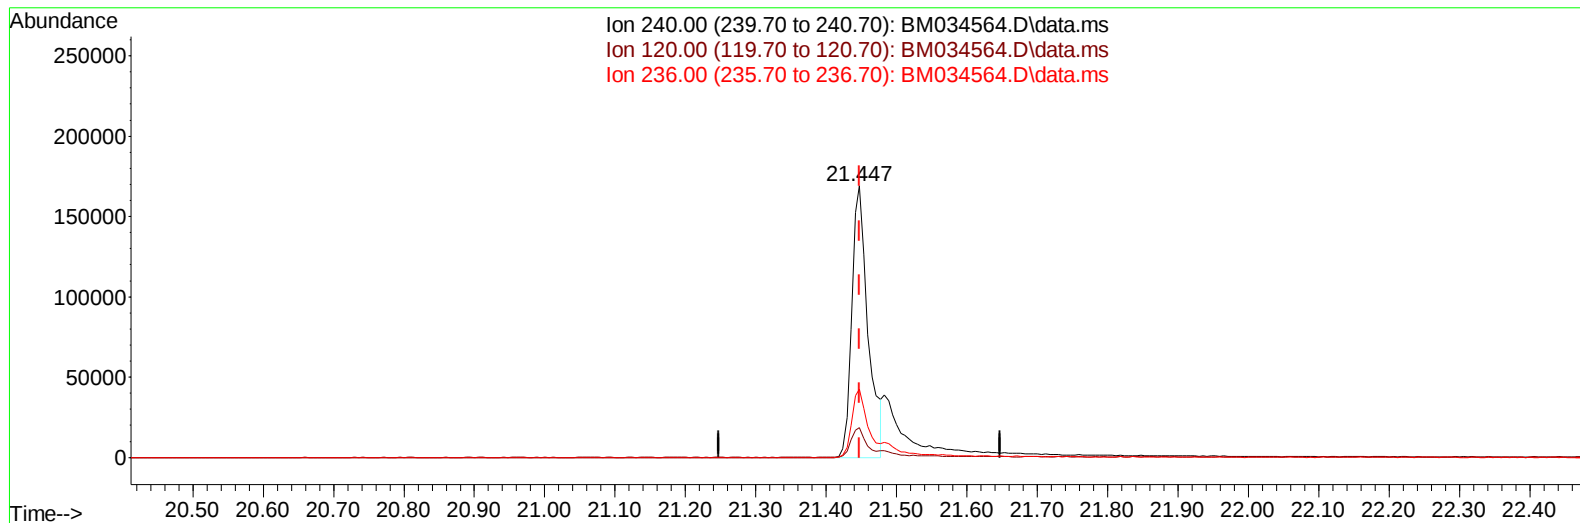

TIC: BM034564.D\data.ms

(79) Chrysene-d12 (I)

21.447min (-0.000) 20.00 ng/u1

response 267966

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.91#
236.00	24.80	25.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 03:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

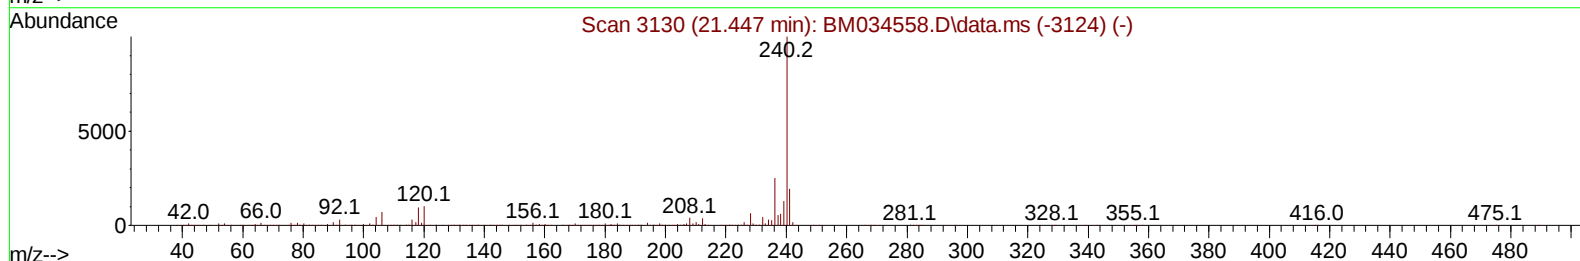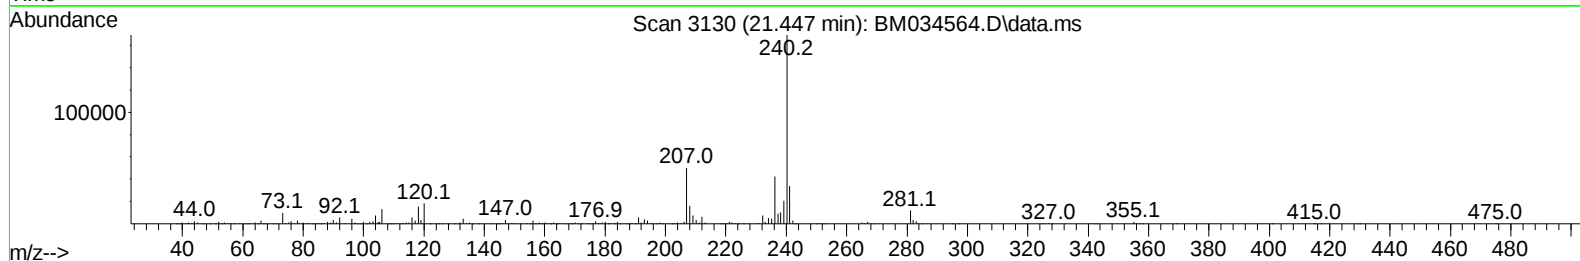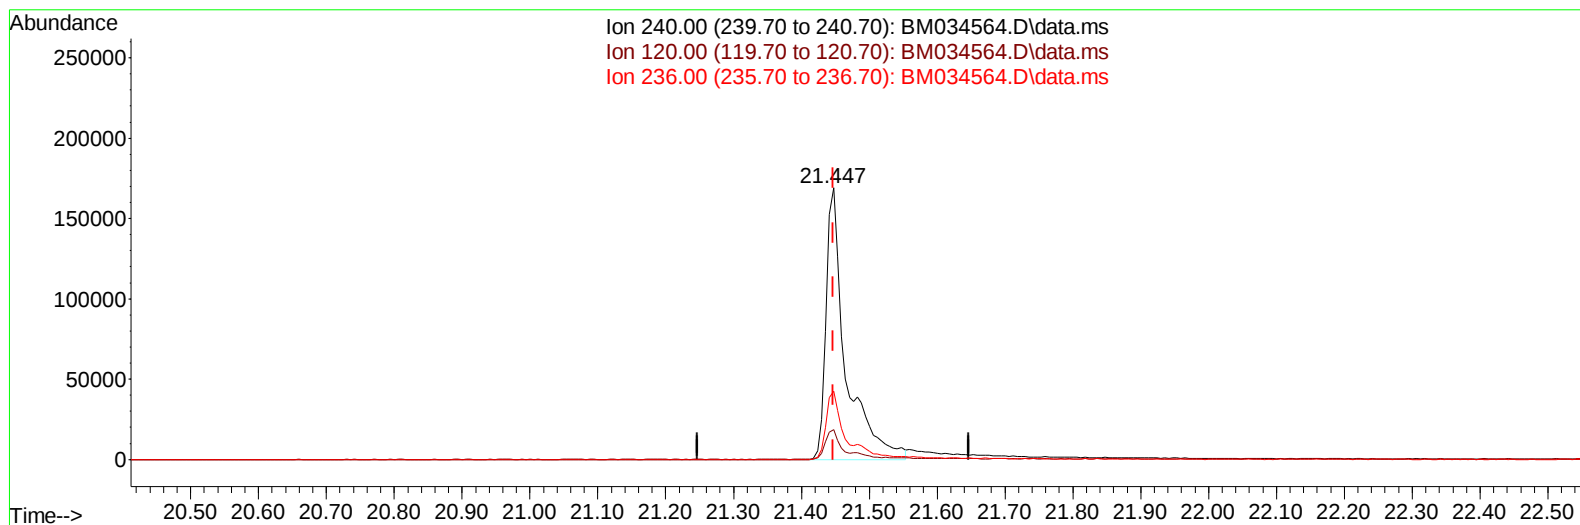

TIC: BM034564.D\data.ms

(79) Chrysene-d12 (I)

21.447min (-0.000) 20.00 ng/ul m

response 340444

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.91#
236.00	24.80	25.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034564.D
 Acq On : 08 Apr 2022 16:42
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 03:06:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	90100	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.689	136	350798	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.524	164	196006	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188	375248	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.447	240	340444m	20.000	ng/ul	0.00
88) Perylene-d12	23.824	264	410755	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	12926	5.116	ng/uL	0.00
4) Pyridine-d5	3.684	84	55595	9.117	ng/ul	0.00
7) Phenol-d5	7.042	99	35258	4.702	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	163147	32.648	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132	135702	23.408	ng/ul	0.00
15) 4-Methylphenol-d8	8.589	113	73790	12.597	ng/ul	0.00
21) Nitrobenzene-d5	9.042	128	86343	33.490	ng/ul	0.00
24) 2-Nitrophenol-d4	9.772	143	84806	31.594	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	133905	26.493	ng/ul	0.00
31) 4-Chloroaniline-d4	10.824	131	163845	23.497	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	502571	35.485	ng/ul	0.00
49) Acenaphthylene-d8	14.218	160	609149	33.463	ng/ul	0.00
54) 4-Nitrophenol-d4	14.765	143	2948m	1.365	ng/ul	0.05
60) Fluorene-d10	15.518	176	448559	36.650	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	64538	28.173	ng/ul	0.00
73) Anthracene-d10	17.365	188	733170	40.981	ng/ul	0.00
81) Pyrene-d10	19.659	212	851449	45.823	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264	808743	39.142	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 03:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

