




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

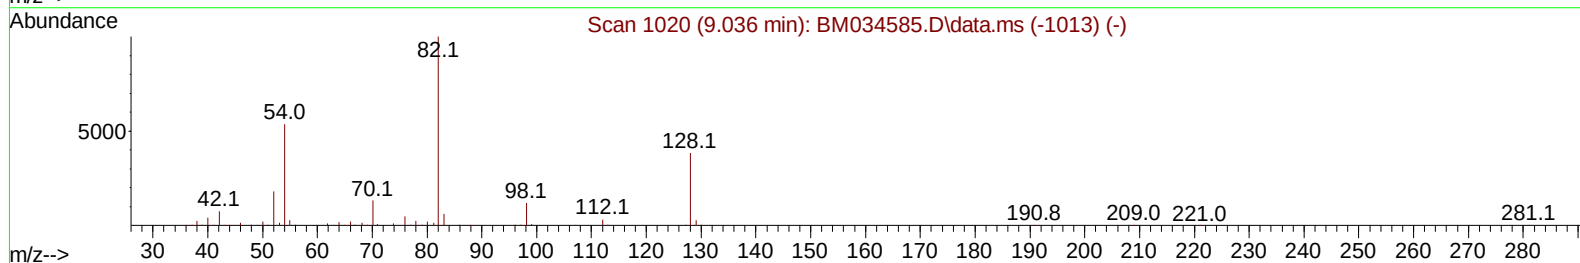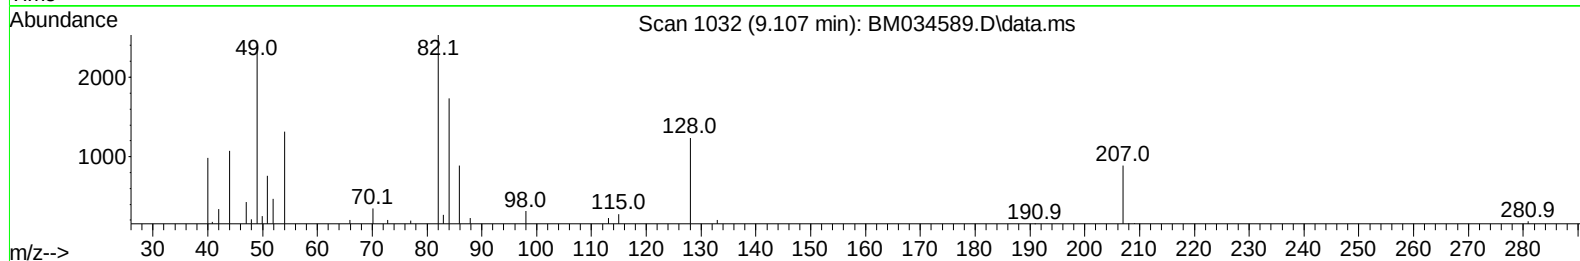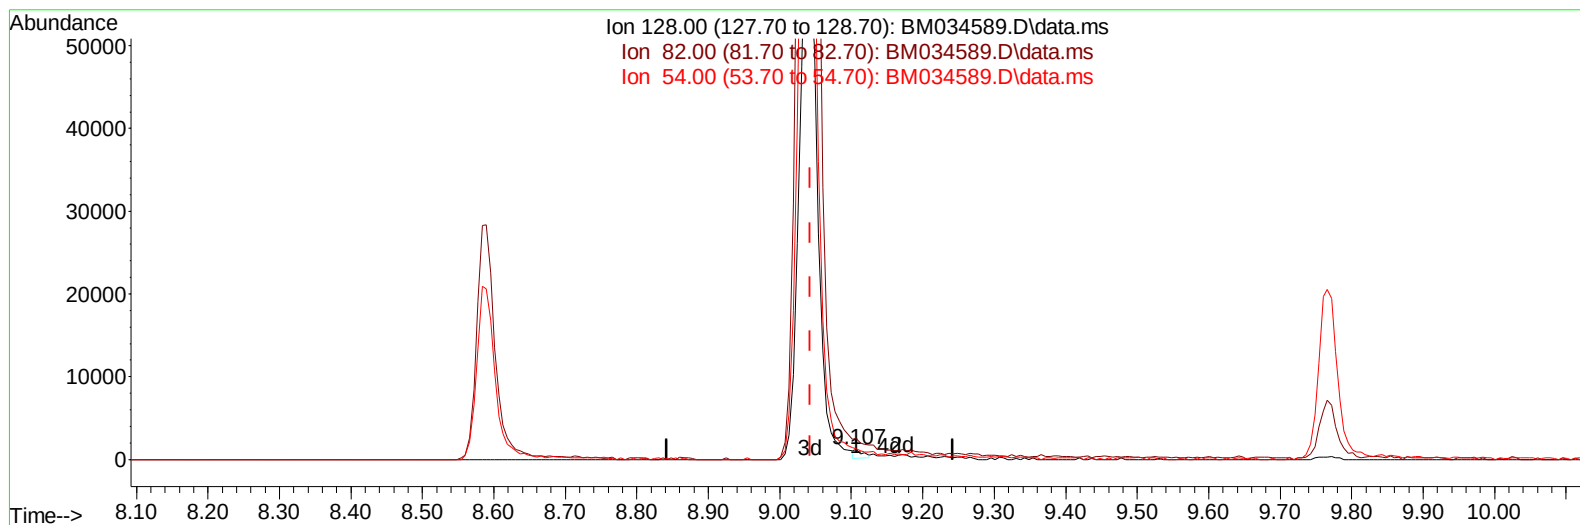

TIC: BM034589.D\data.ms

(21) Nitrobenzene-d5 (S)

9.107min (+ 0.065) 0.27 ng/u1

response 885

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	205.02
54.00	100.50	106.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034589.D
 Acq On : 09 Apr 2022 09:05
 Operator : CG/JU
 Sample : PB143959BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK959

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:58:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

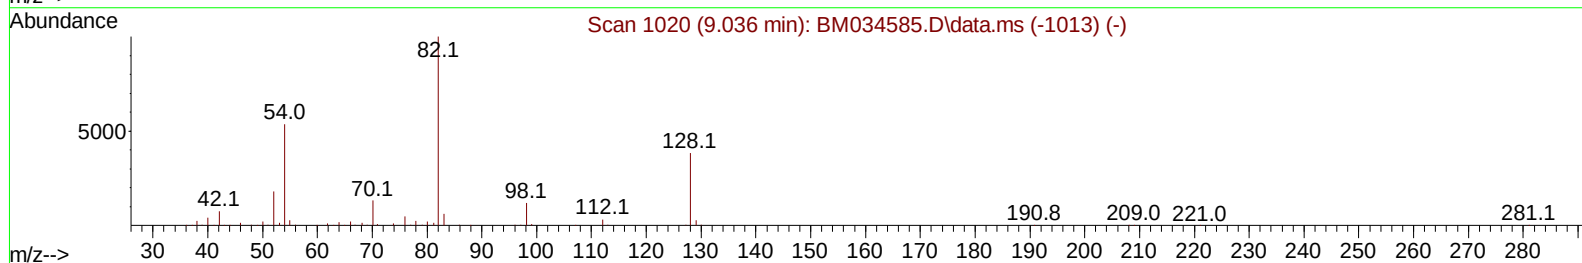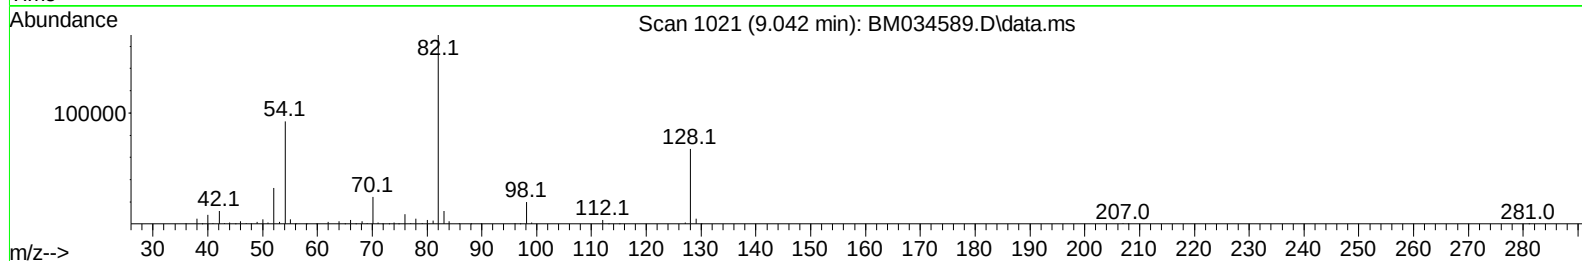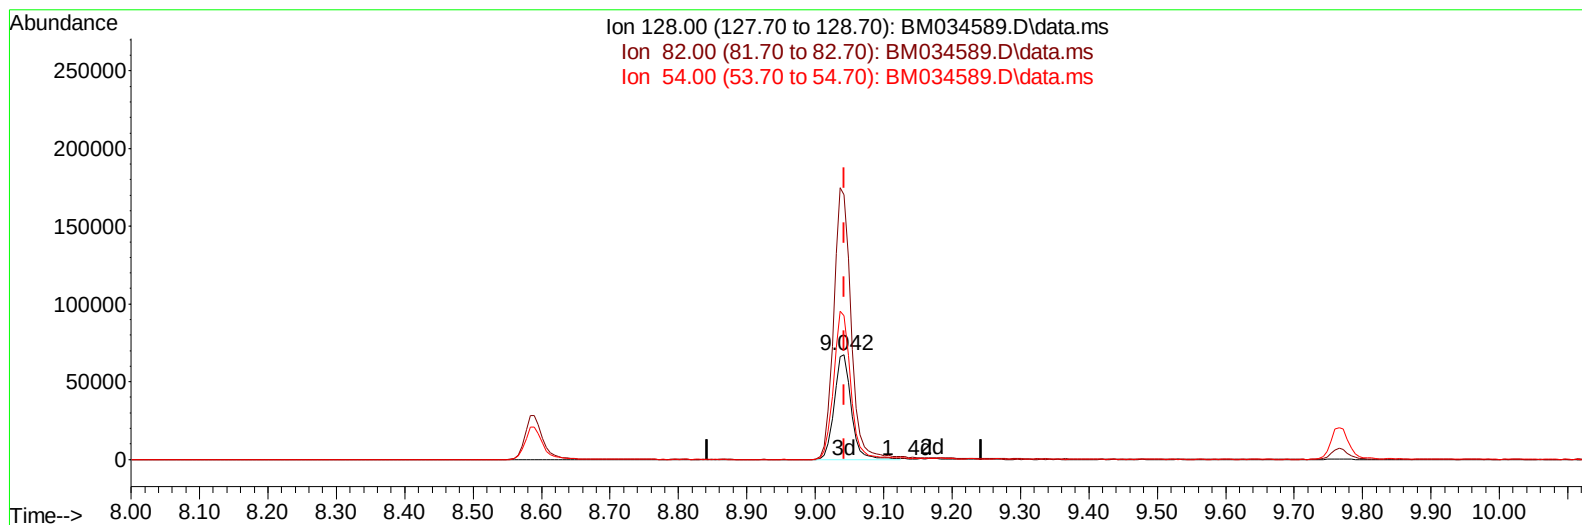

TIC: BM034589.D\data.ms

(21) Nitrobenzene-d5 (S)

9.042min (-0.000) 35.96 ng/ul m

response 116729

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	251.98
54.00	100.50	137.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

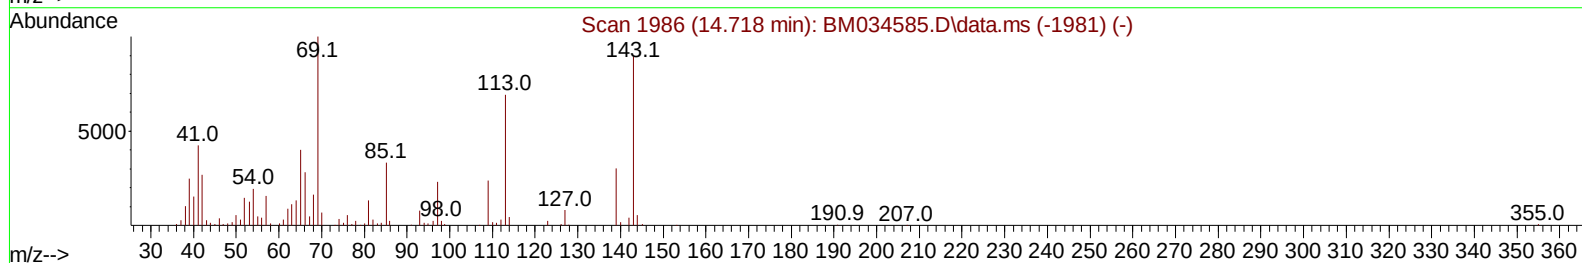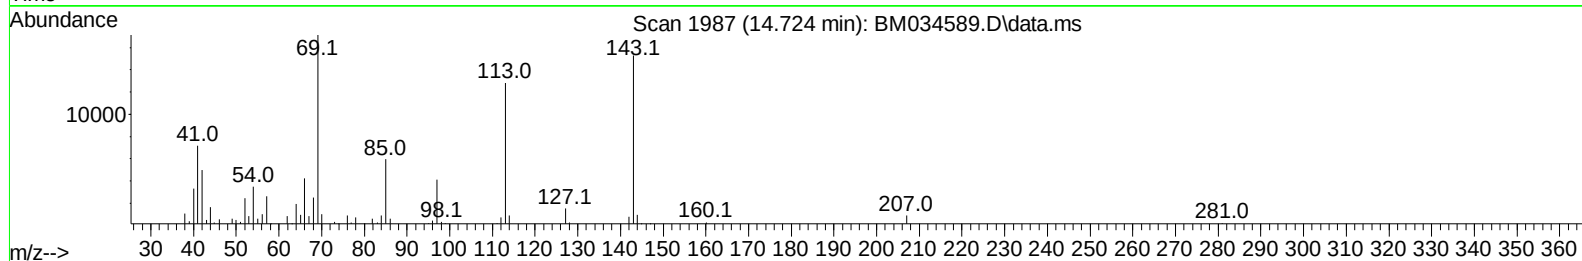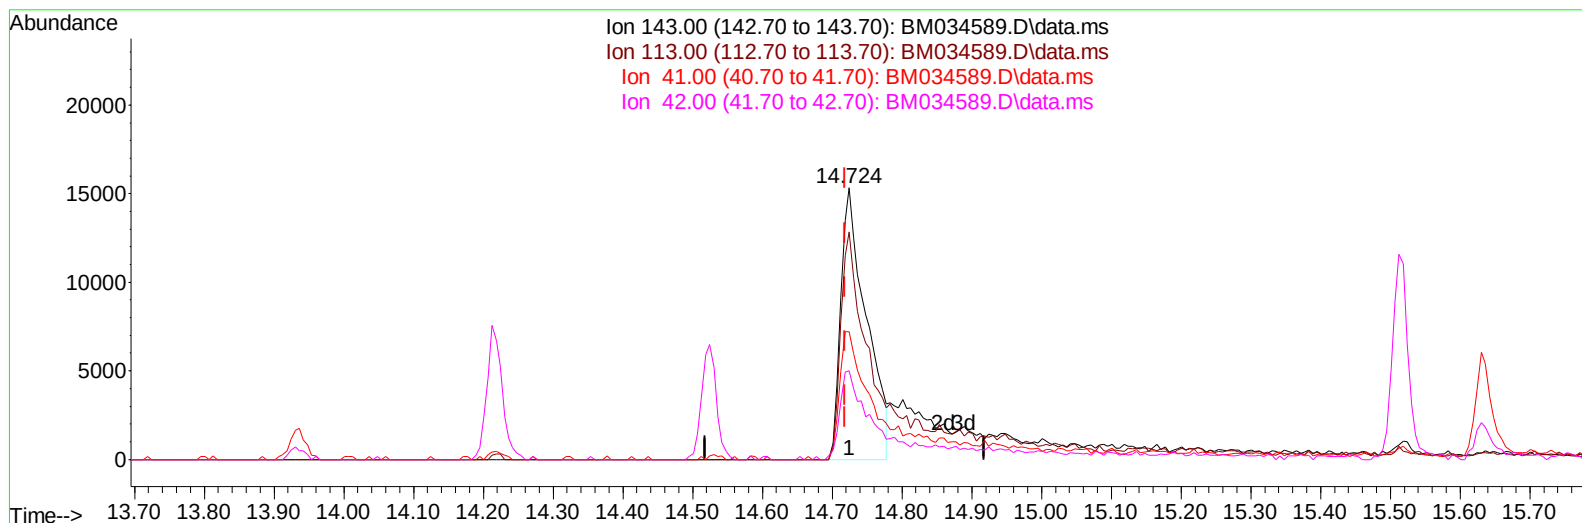

TIC: BM034589.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.724min (+ 0.006) 14.22 ng/ul

response 38489

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	83.79
41.00	31.90	47.03#
42.00	19.10	32.65#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

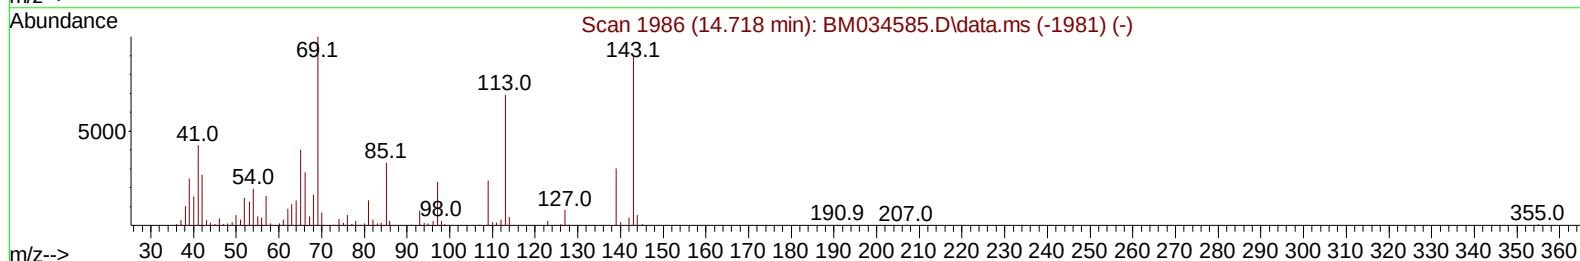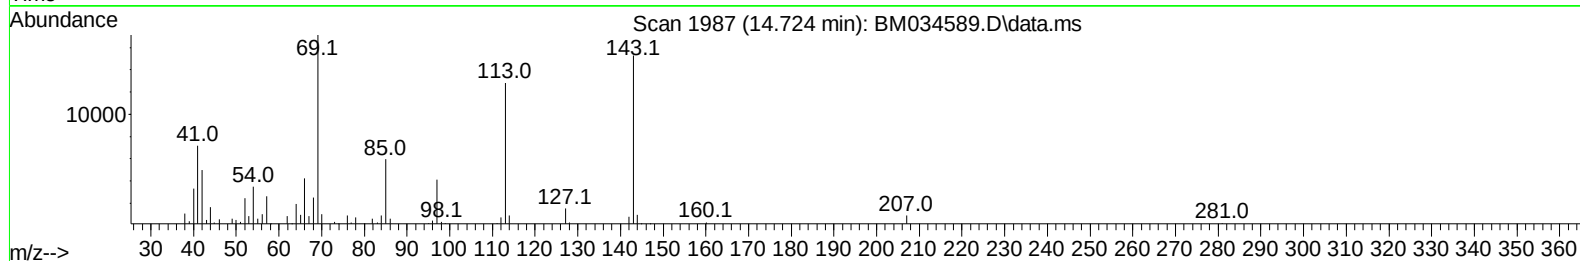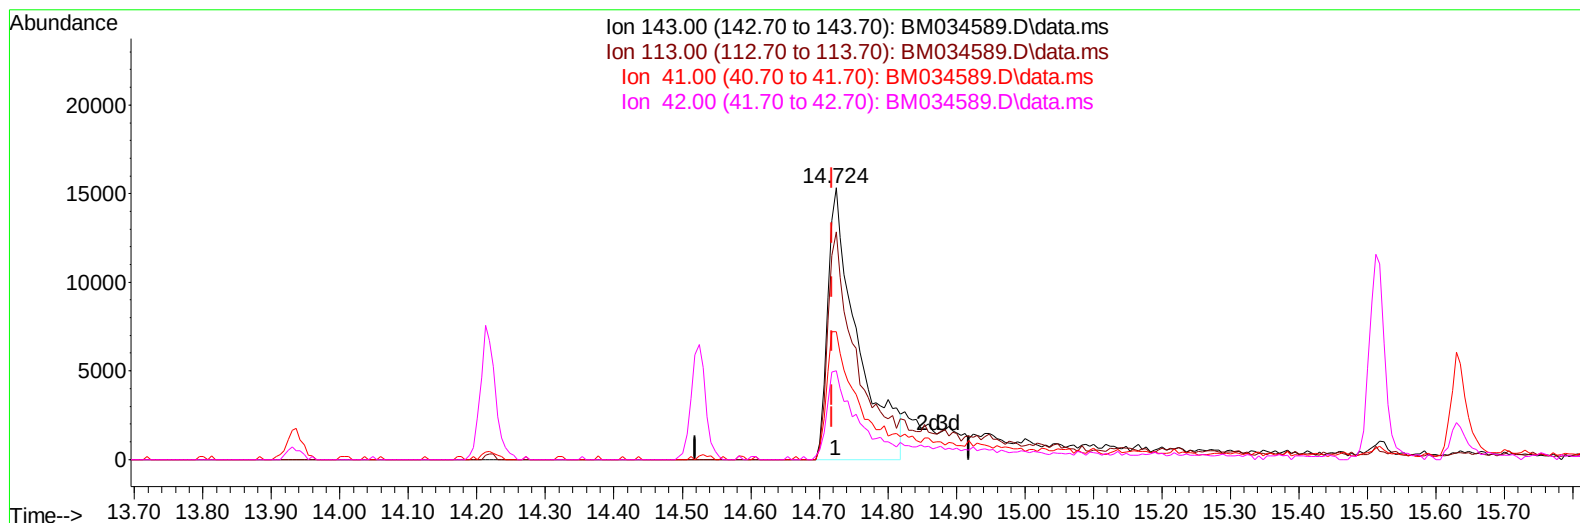

TIC: BM034589.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.724min (+ 0.006) 16.94 ng/ul m

response 45855

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	83.79
41.00	31.90	47.03#
42.00	19.10	32.65#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

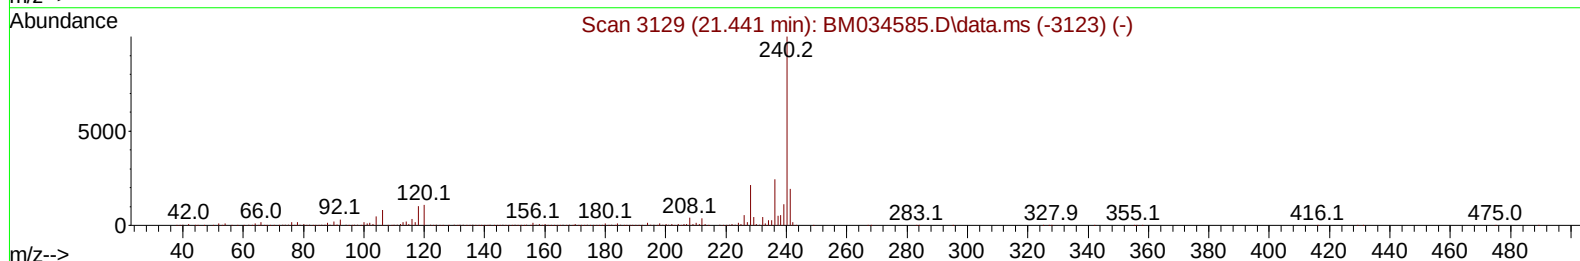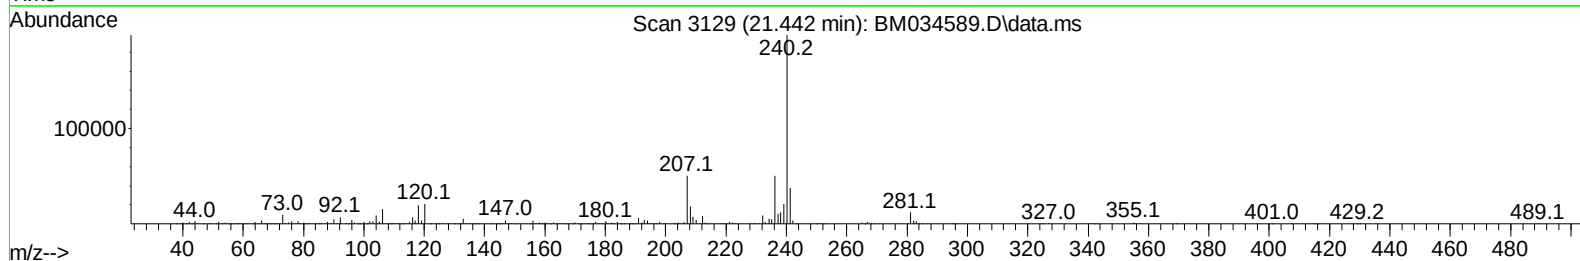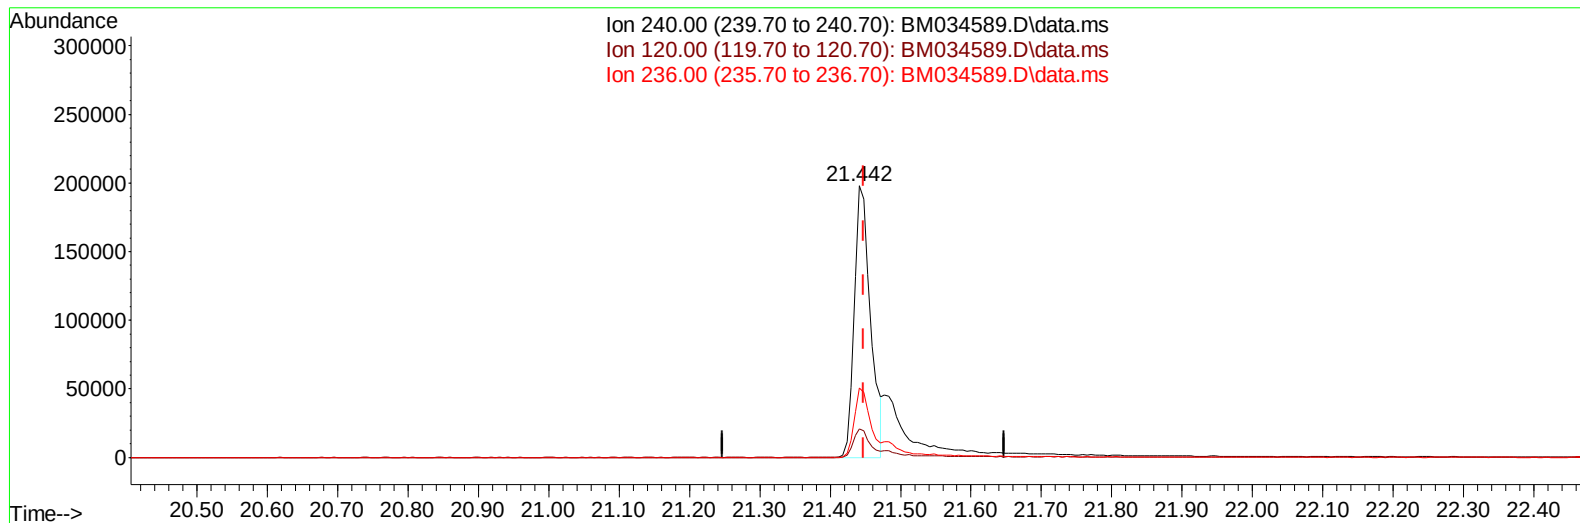

TIC: BM034589.D\data.ms

(79) Chrysene-d12 (I)

21.442min (-0.006) 20.00 ng/u1

response 315856

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.61#
236.00	24.80	25.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

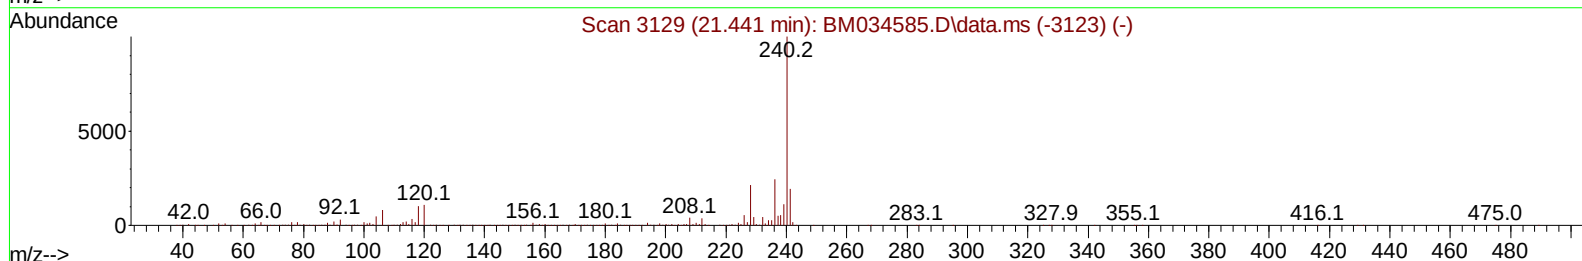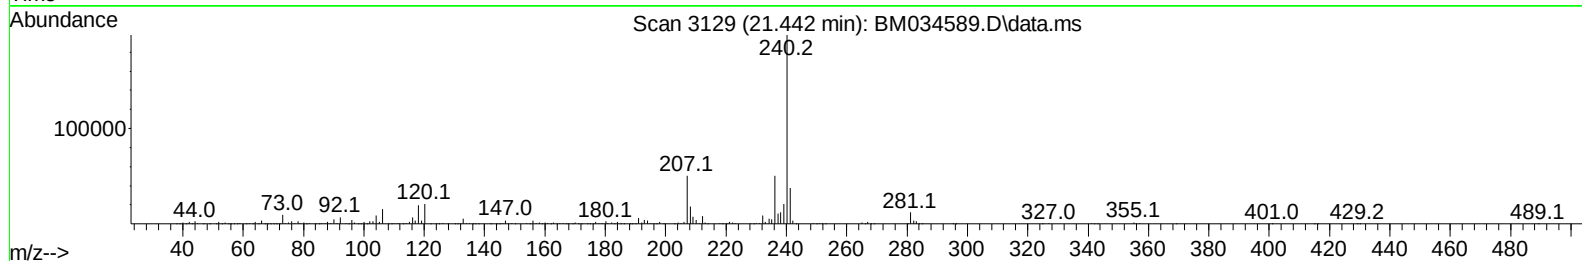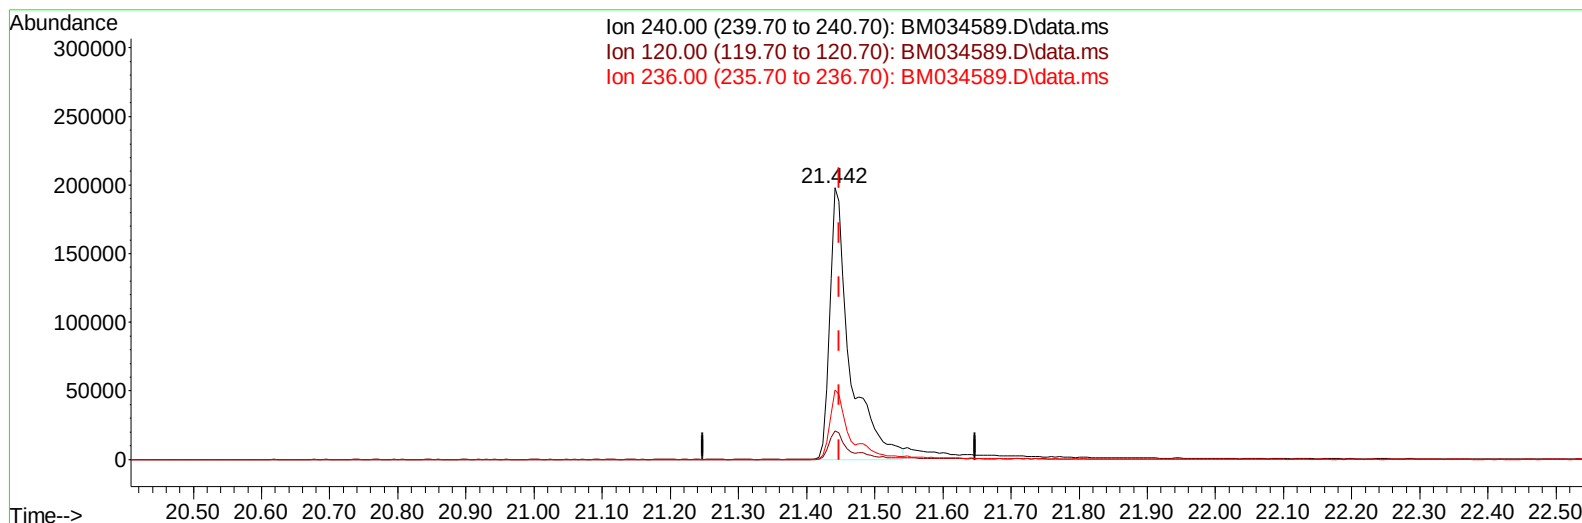

TIC: BM034589.D\data.ms

(79) Chrysene-d12 (I)

21.442min (-0.006) 20.00 ng/ul m

response 407896

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	10.61#
236.00	24.80	25.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034589.D
 Acq On : 09 Apr 2022 09:05
 Operator : CG/JU
 Sample : PB143959BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK959

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:58:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	112281	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.683	136	441630	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.524	164	245642	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188	461378	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.442	240	407896m	20.000	ng/ul	0.00
88) Perylene-d12	23.824	264	506256	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	21391	6.794	ng/uL	0.00
4) Pyridine-d5	3.678	84	247933	32.628	ng/ul	0.00
7) Phenol-d5	7.037	99	292123	31.259	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	214917	34.512	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132	251243	34.778	ng/ul	0.00
15) 4-Methylphenol-d8	8.589	113	235693	32.287	ng/ul	0.00
21) Nitrobenzene-d5	9.042	128	116729m	35.964	ng/ul	0.00
24) 2-Nitrophenol-d4	9.766	143	118292	35.006	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	193130	30.352	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131	271118	30.884	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	643063	36.230	ng/ul	0.00
49) Acenaphthylene-d8	14.218	160	774992	33.971	ng/ul	0.00
54) 4-Nitrophenol-d4	14.724	143	45855m	16.943	ng/ul	0.00
60) Fluorene-d10	15.512	176	547324	35.683	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	81200	28.829	ng/ul	0.00
73) Anthracene-d10	17.365	188	822642	37.398	ng/ul	0.00
81) Pyrene-d10	19.653	212	983076	44.158	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264	903936	35.496	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

