

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034591.D
 Acq On : 09 Apr 2022 10:18
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
 Patel
 04/12/2022

Quant Time: Apr 11 00:58:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

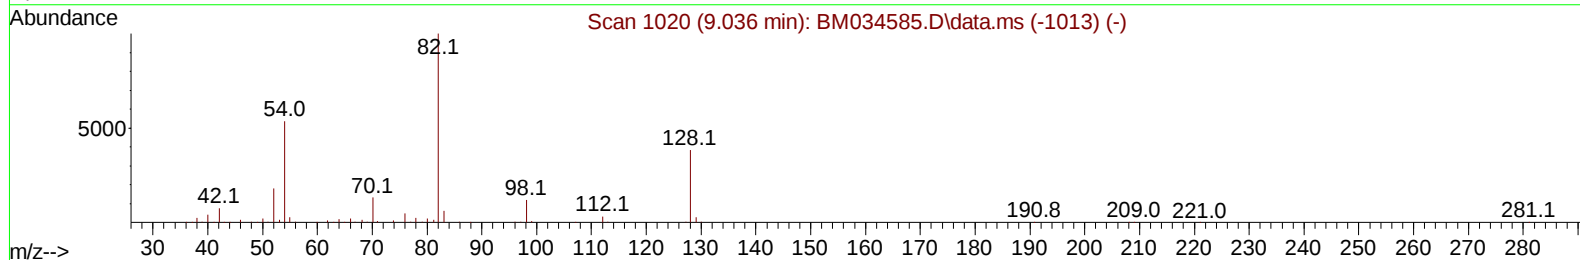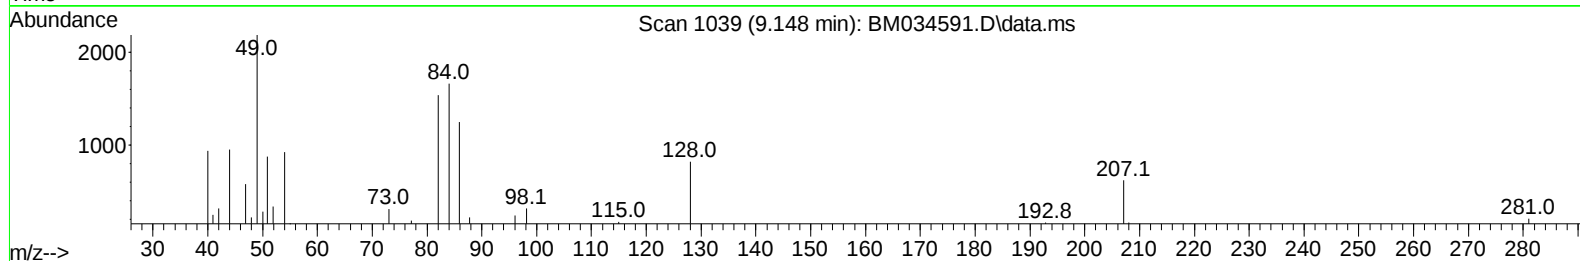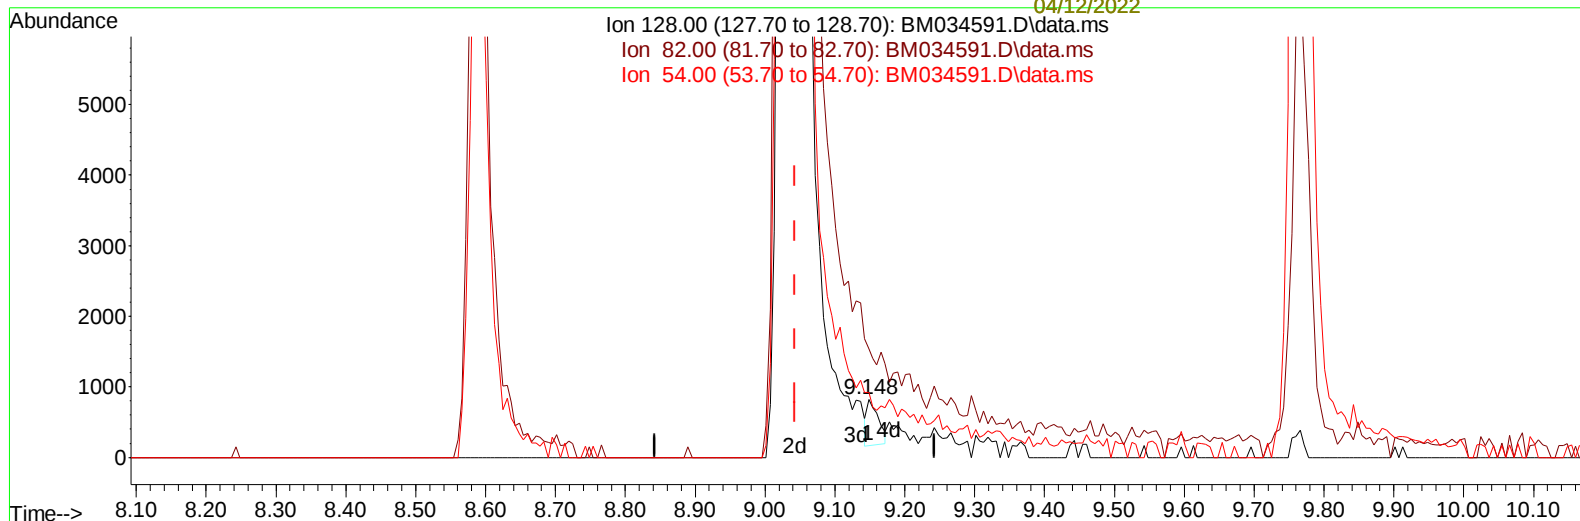

TIC: BM034591.D\data.ms

(21) Nitrobenzene-d5 (S)

9.148min (+ 0.106) 0.25 ng/u1

response 731

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	187.12
54.00	100.50	112.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034591.D
 Acq On : 09 Apr 2022 10:18
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 00:58:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Supervised By :Yogesh
 Patel
 04/12/2022

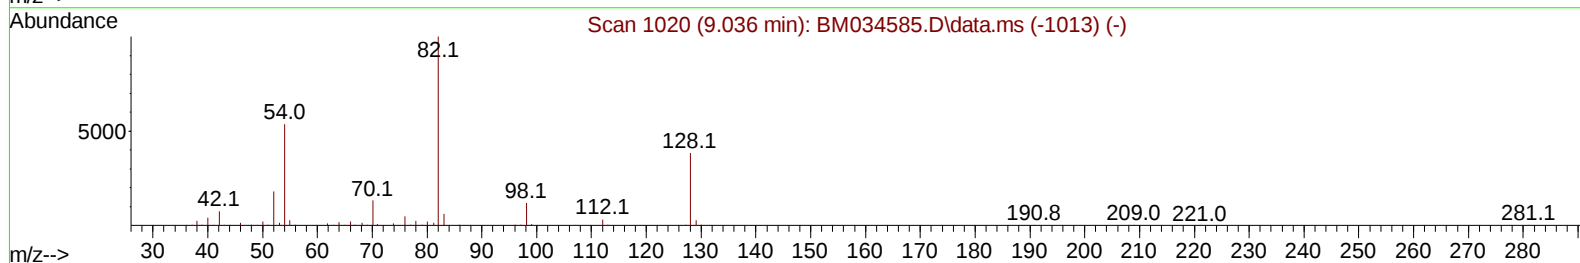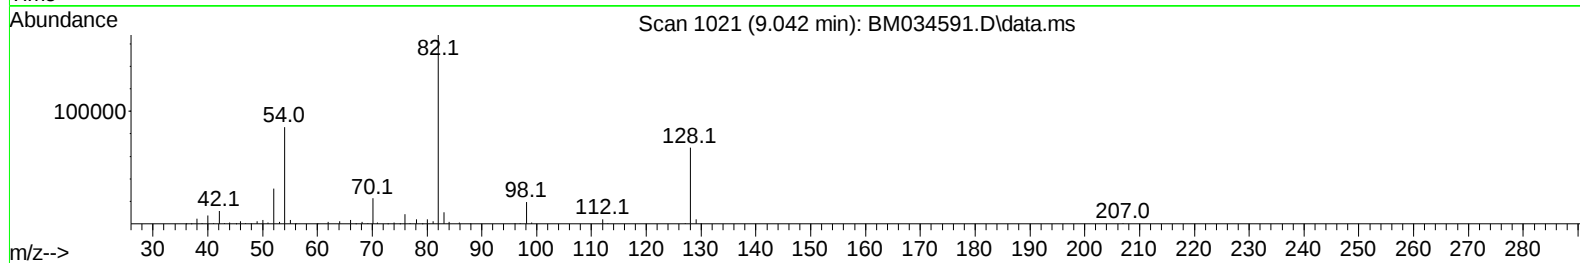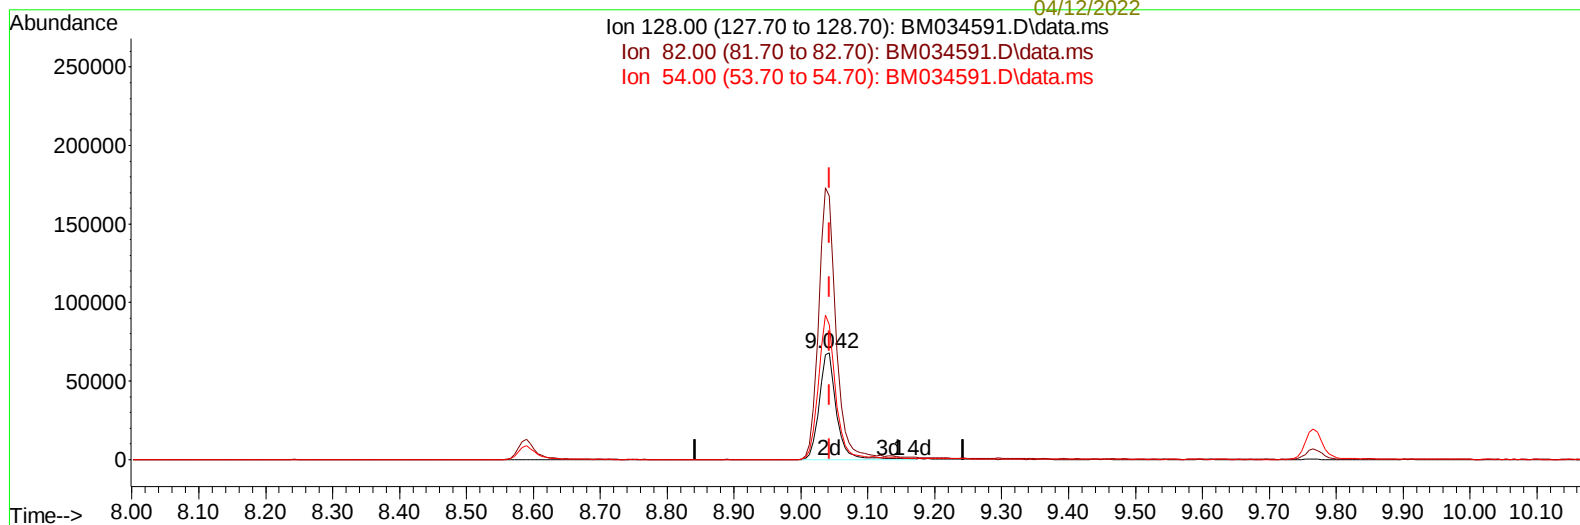

TIC: BM034591.D\data.ms

(21) Nitrobenzene-d5 (S)

9.042min (0.000) 42.15 ng/u1 m

response 121775

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	247.52
54.00	100.50	127.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034591.D
 Acq On : 09 Apr 2022 10:18
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
 Patel
 04/12/2022

Quant Time: Apr 11 00:58:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

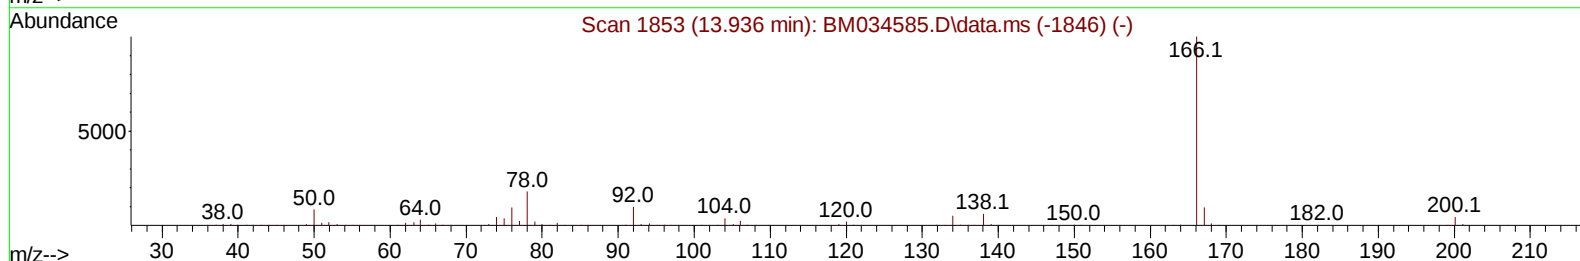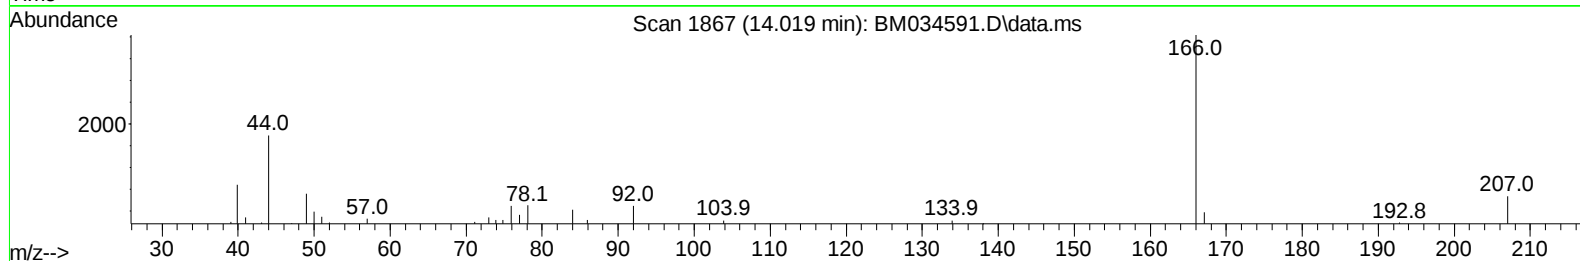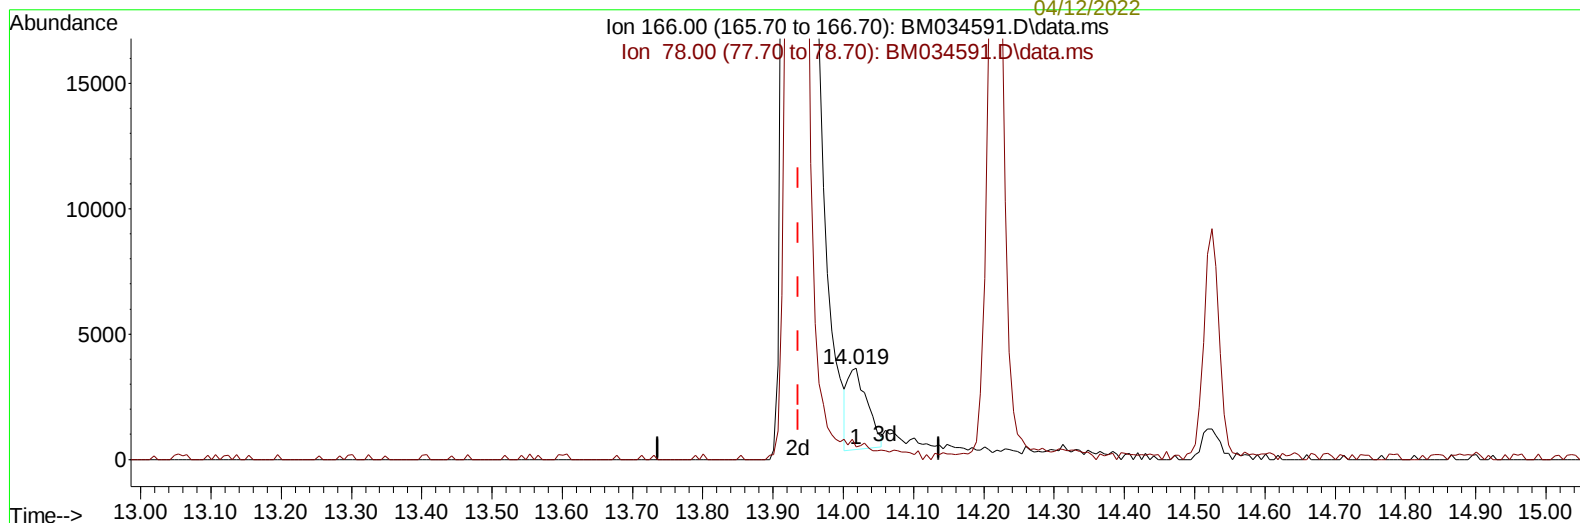

TIC: BM034591.D\data.ms

(46) Dimethylphthalate-d6 (S)

14.019min (+ 0.082) 0.39 ng/u1

response 6322

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	14.80	13.70
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034591.D
 Acq On : 09 Apr 2022 10:18
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H2




Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
 Patel
 04/12/2022

Quant Time: Apr 11 00:58:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Ion 166.00 (165.70 to 166.70): BM034591.D\data.ms
 Ion 78.00 (77.70 to 78.70): BM034591.D\data.ms

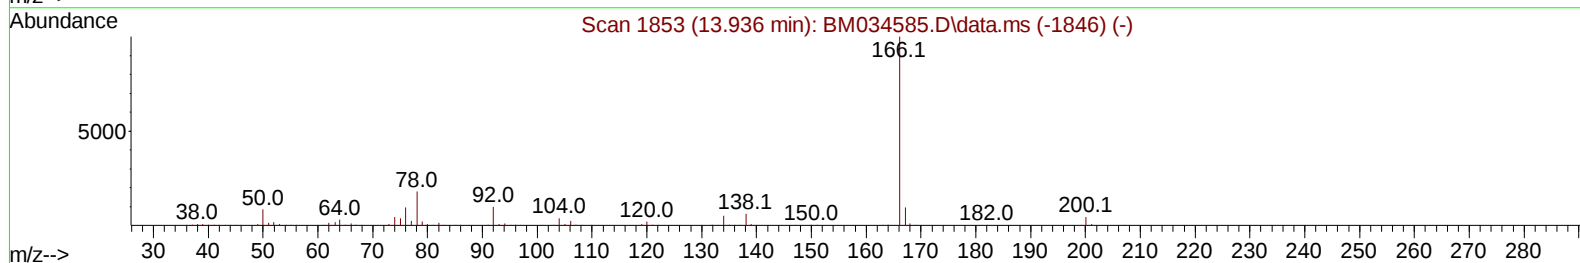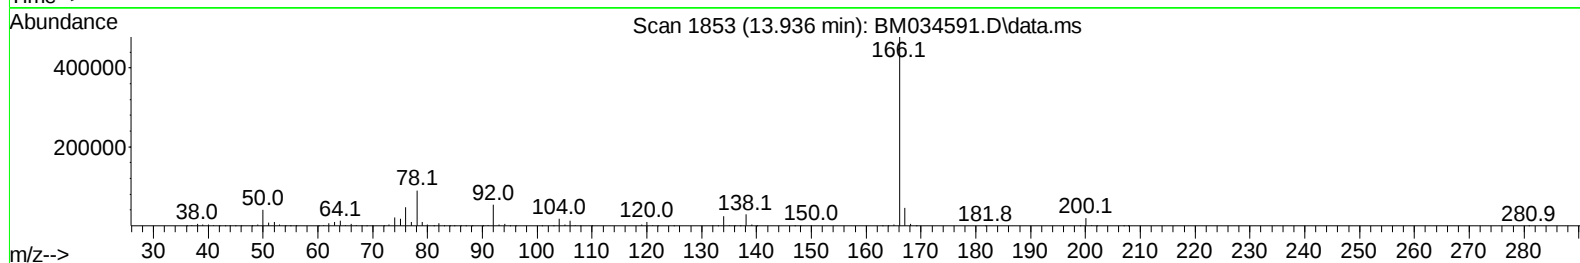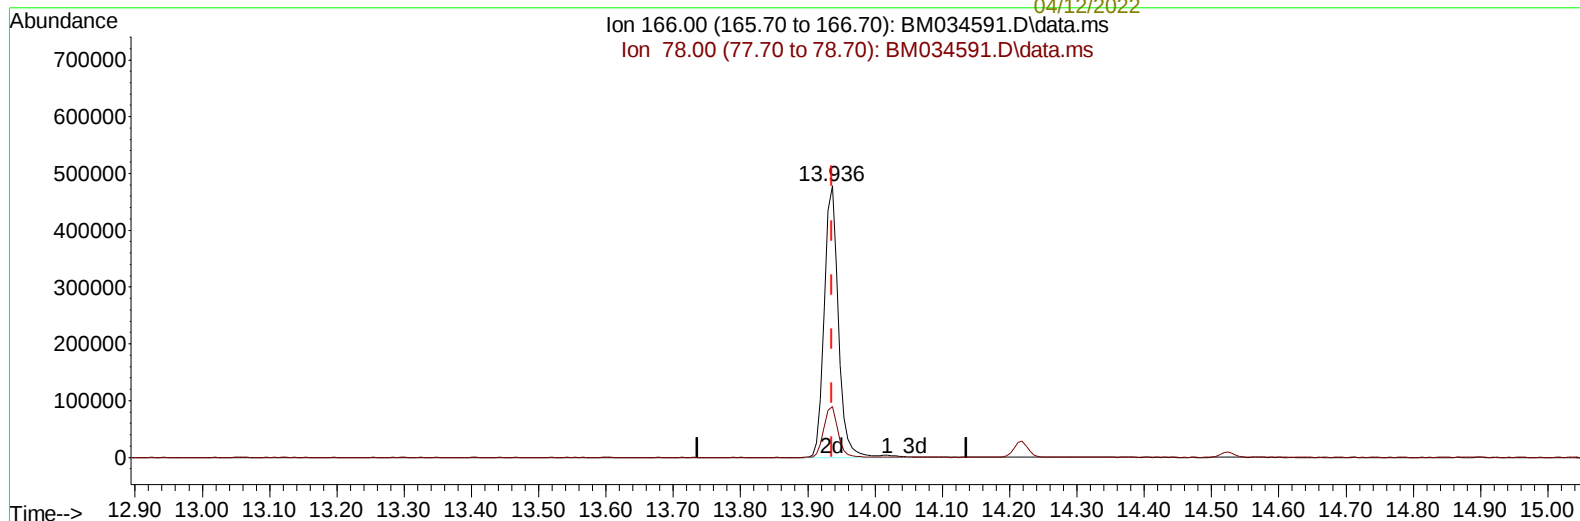

TIC: BM034591.D\data.ms

(46) Dimethylphthalate-d6 (S)

13.936min (0.000) 43.24 ng/ul m

response 696934

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	14.80	18.84#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034591.D
Acq On : 09 Apr 2022 10:18
Operator : CG/JU
Sample : N2319-05
Misc :
ALS Vial : 38 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
Patel
04/12/2022

Quant Time: Apr 11 00:58:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

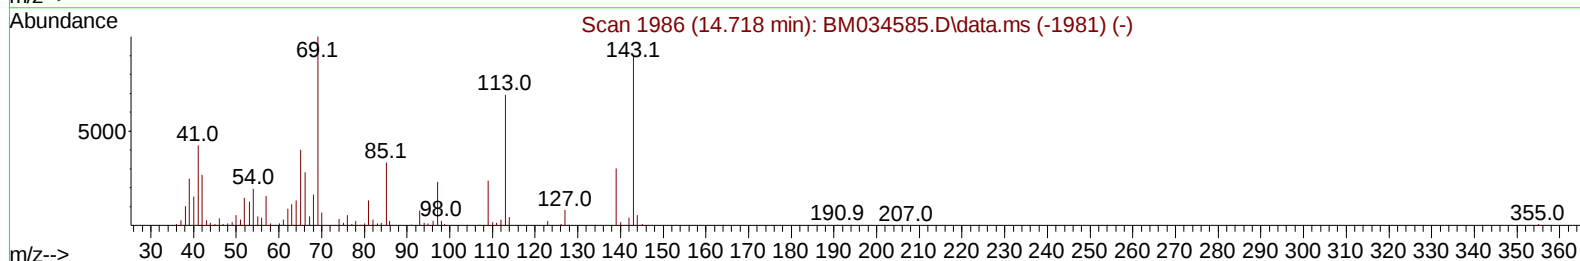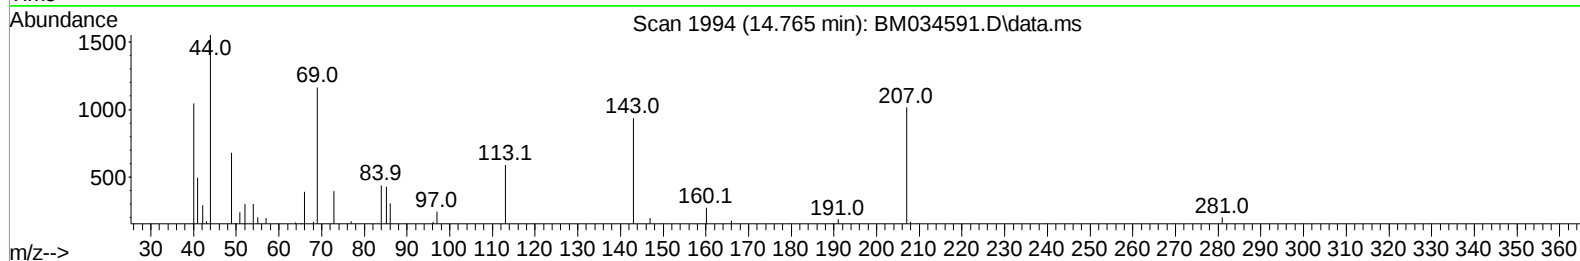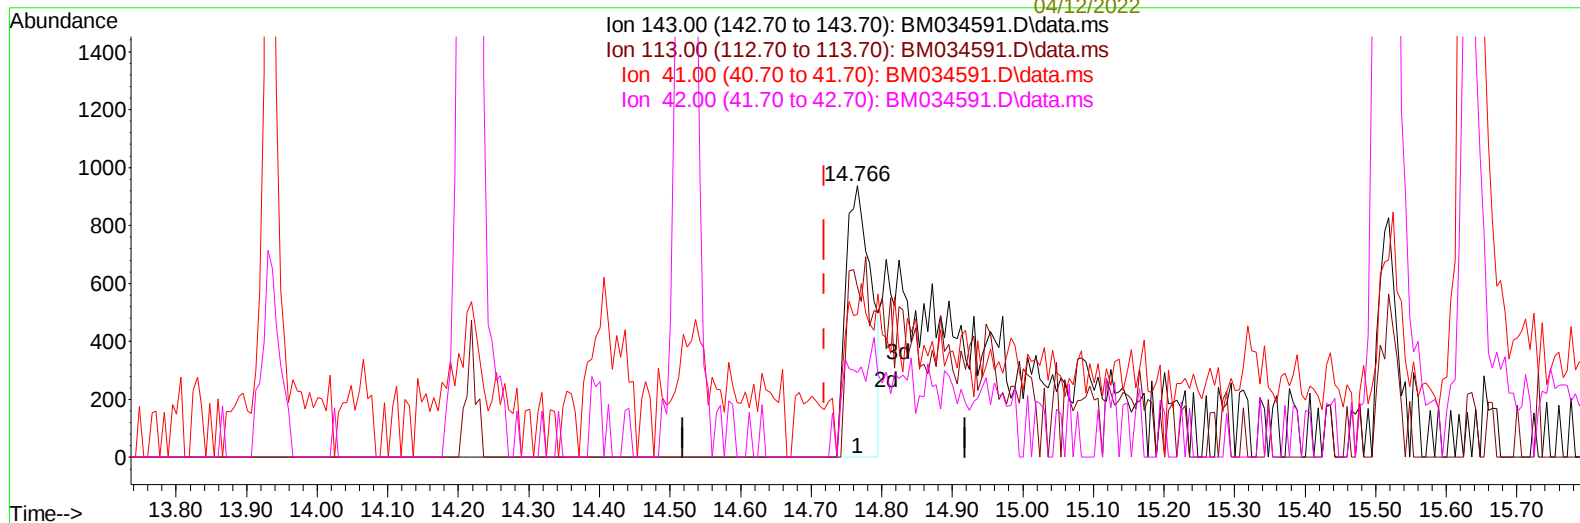

TIC: BM034591.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.765min (+ 0.047) 0.96 ng/u1****response 2369**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	62.86
41.00	31.90	52.61#
42.00	19.10	31.27#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034591.D
Acq On : 09 Apr 2022 10:18
Operator : CG/JU
Sample : N2319-05
Misc :
ALS Vial : 38 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
Patel
04/12/2022

Quant Time: Apr 11 00:58:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

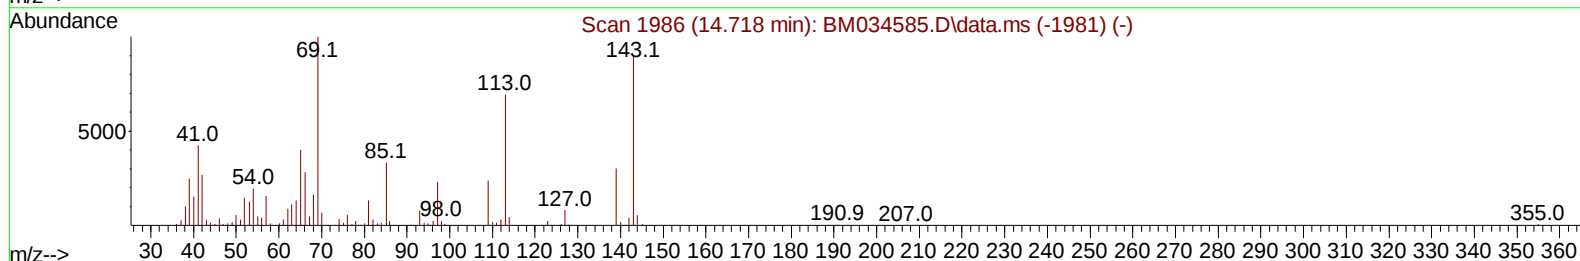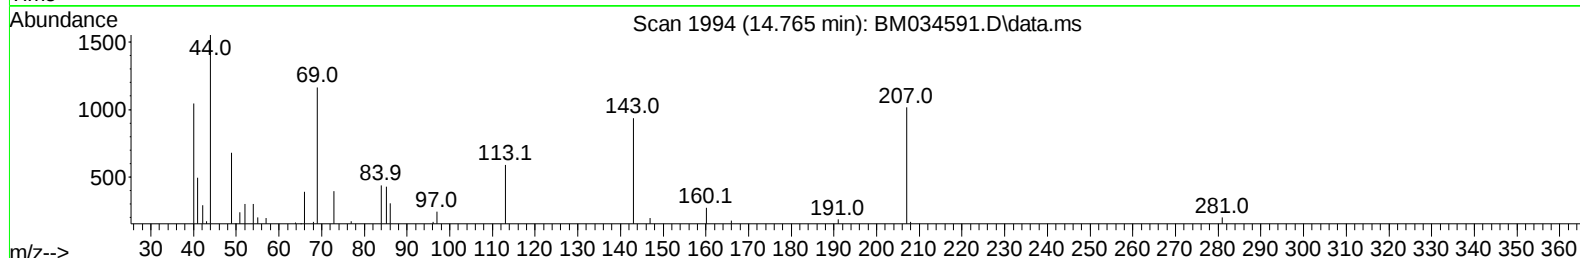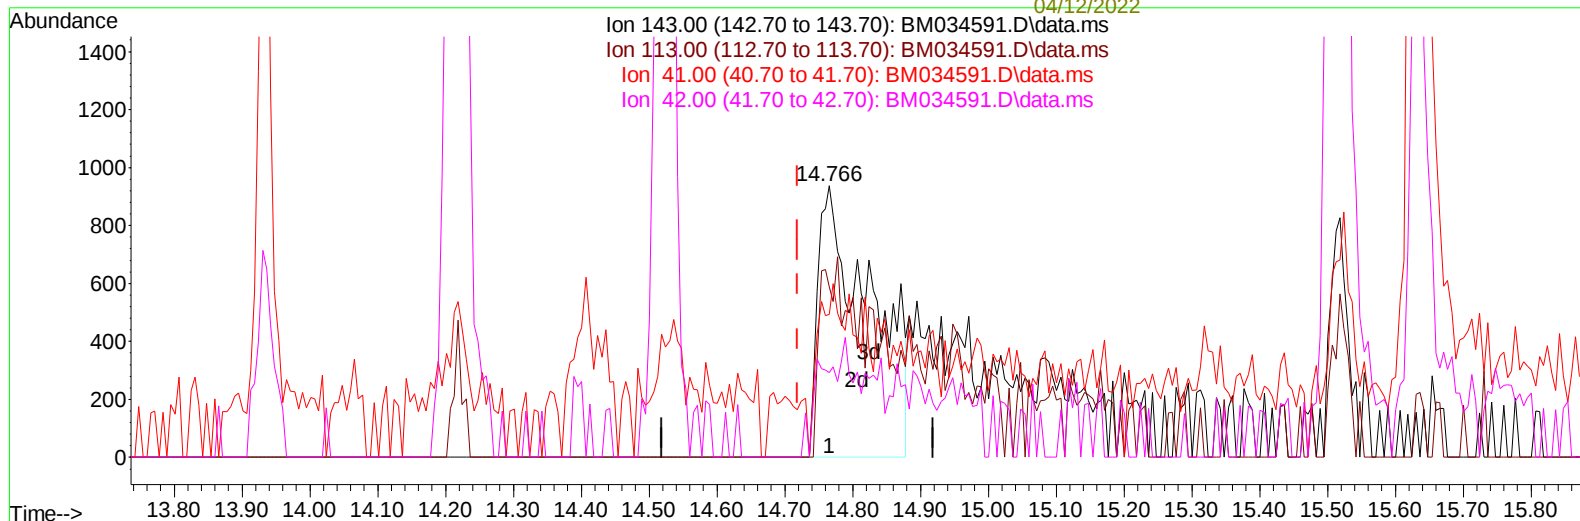

TIC: BM034591.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.765min (+ 0.047) 2.02 ng/ul m

response 4971

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	62.86
41.00	31.90	52.61#
42.00	19.10	31.27#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034591.D
 Acq On : 09 Apr 2022 10:18
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
 Patel
 04/12/2022

Quant Time: Apr 11 00:58:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	98585	20.000	ng/ul	0.00
20) Naphthalene-d8	10.683	136	393074	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.524	164	223077	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188	426855	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.447	240	428431	20.000	ng/ul	# 0.00
88) Perylene-d12	23.824	264	509468	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	14053	5.083	ng/uL	0.00
4) Pyridine-d5	3.684	84	64982	9.740	ng/ul	0.00
7) Phenol-d5	7.037	99	49437	6.025	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	218731	40.004	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132	188584	29.731	ng/ul	0.00
15) 4-Methylphenol-d8	8.589	113	105576	16.472	ng/ul	0.00
21) Nitrobenzene-d5	9.042	128	121775m	42.153	ng/ul	0.00
24) 2-Nitrophenol-d4	9.766	143	116889	38.863	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	178147	31.455	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131	228808	29.284	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	696934m	43.237	ng/ul	0.00
49) Acenaphthylene-d8	14.218	160	839712	40.531	ng/ul	0.00
54) 4-Nitrophenol-d4	14.765	143	4971m	2.023	ng/ul	0.05
60) Fluorene-d10	15.518	176	616238	44.240	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	92337	35.435	ng/ul	0.00
73) Anthracene-d10	17.365	188	981186	48.213	ng/ul	0.00
81) Pyrene-d10	19.653	212	1214096	51.921	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264	1226255	47.849	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034591.D
Acq On : 09 Apr 2022 10:18
Operator : CG/JU
Sample : N2319-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Supervised By :Yogesh
Patel
04/12/2022

Quant Time: Apr 11 00:58:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

