




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

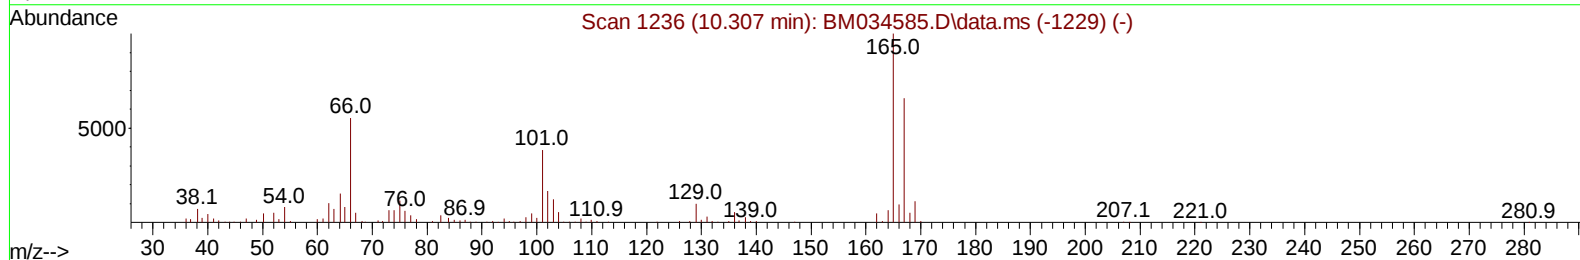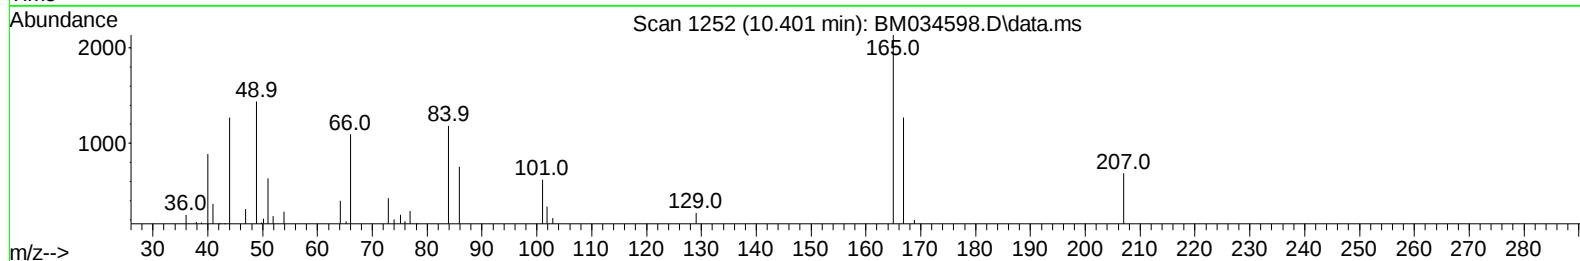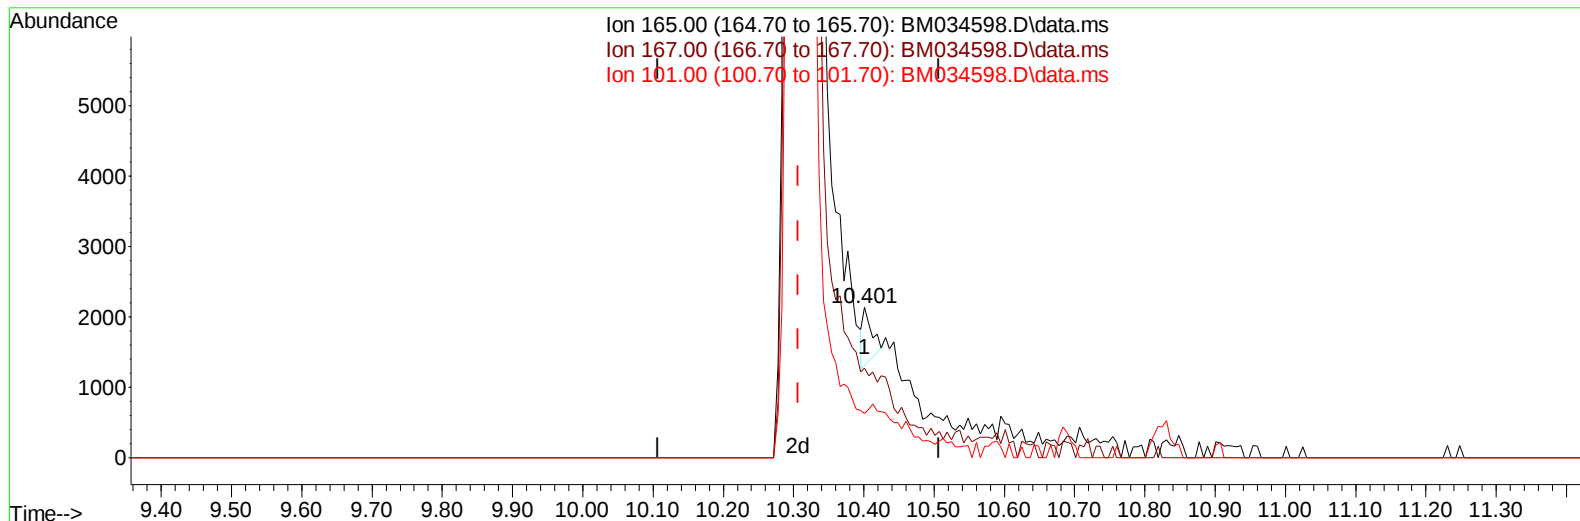

TIC: BM034598.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.401min (+ 0.094) 0.10 ng/u1

response 714

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.20	59.49
101.00	30.30	29.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034598.D
 Acq On : 09 Apr 2022 14:32
 Operator : CG/JU
 Sample : N2266-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

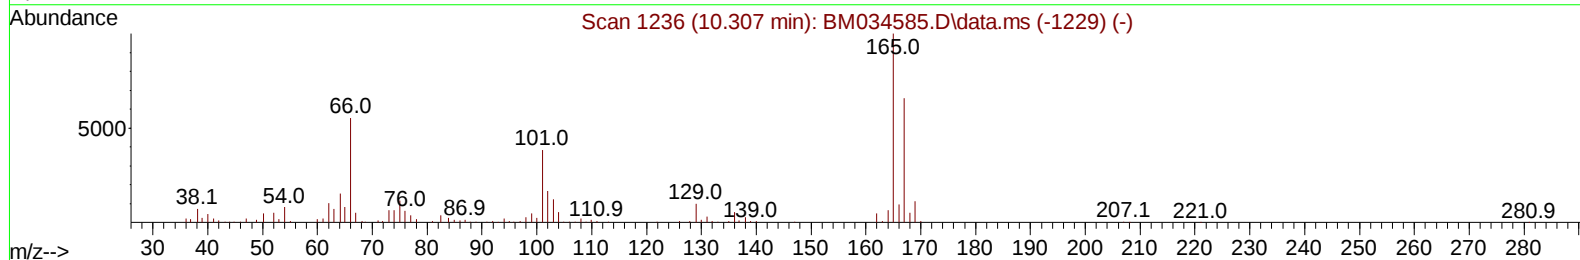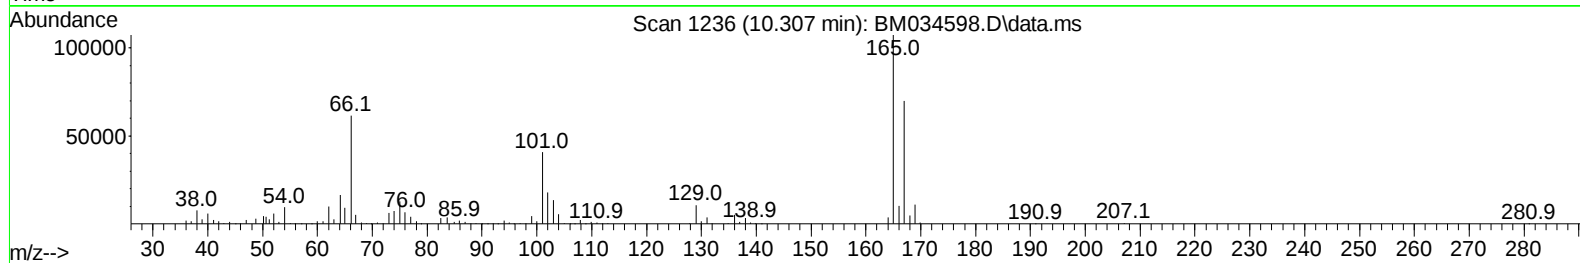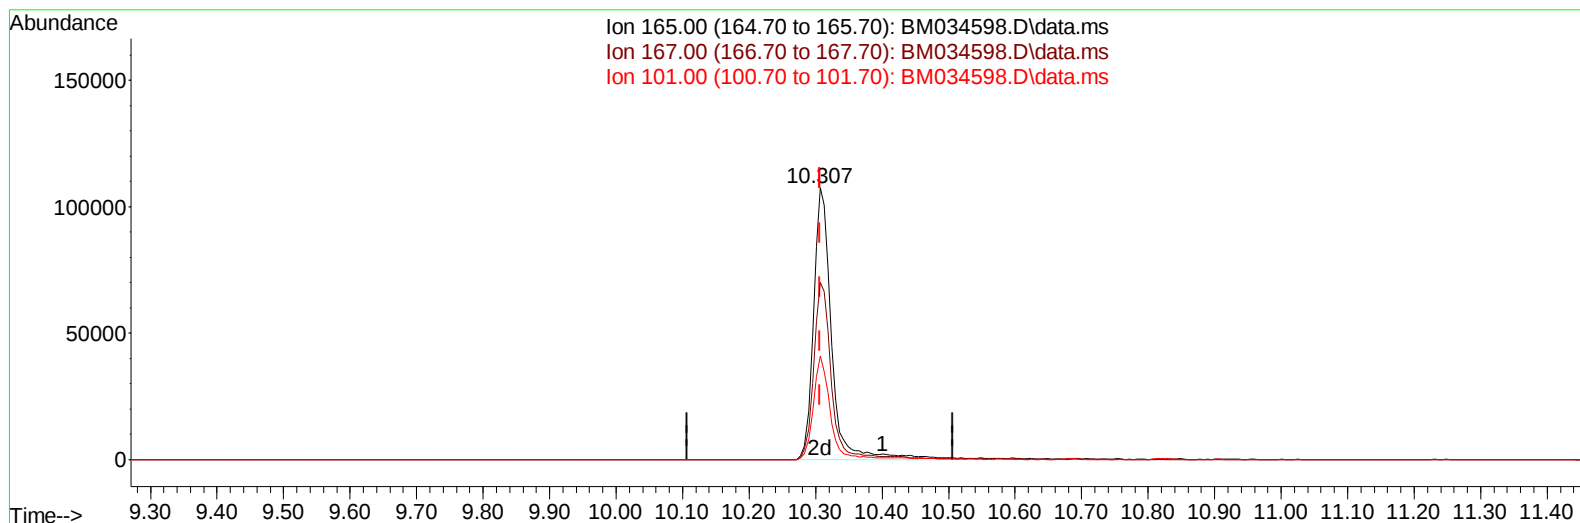

TIC: BM034598.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.307min (0.000) 28.96 ng/ul m

response 202163

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.20	65.18
101.00	30.30	38.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034598.D
 Acq On : 09 Apr 2022 14:32
 Operator : CG/JU
 Sample : N2266-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

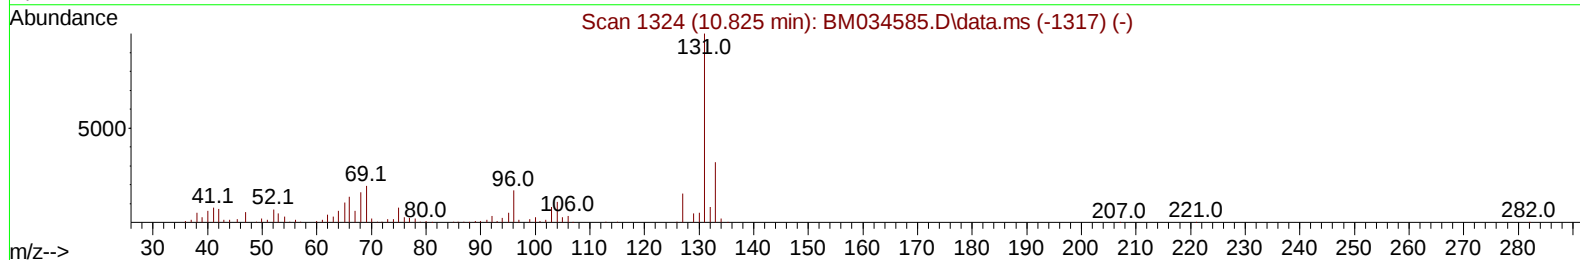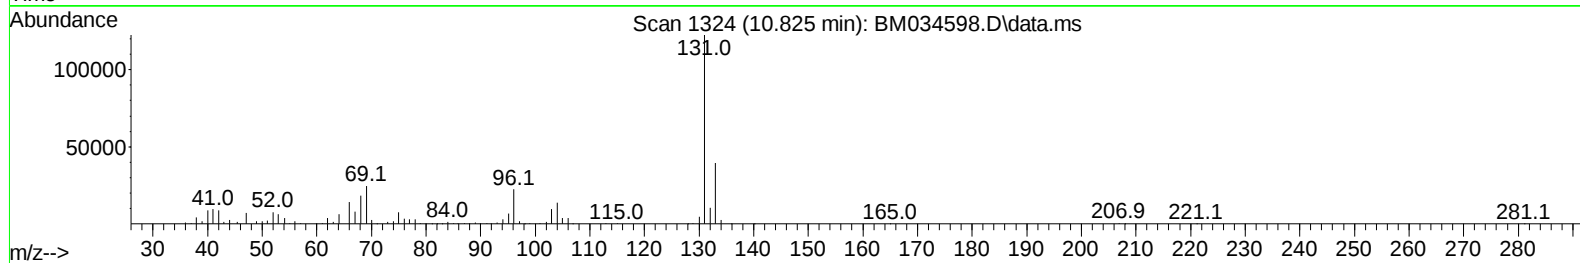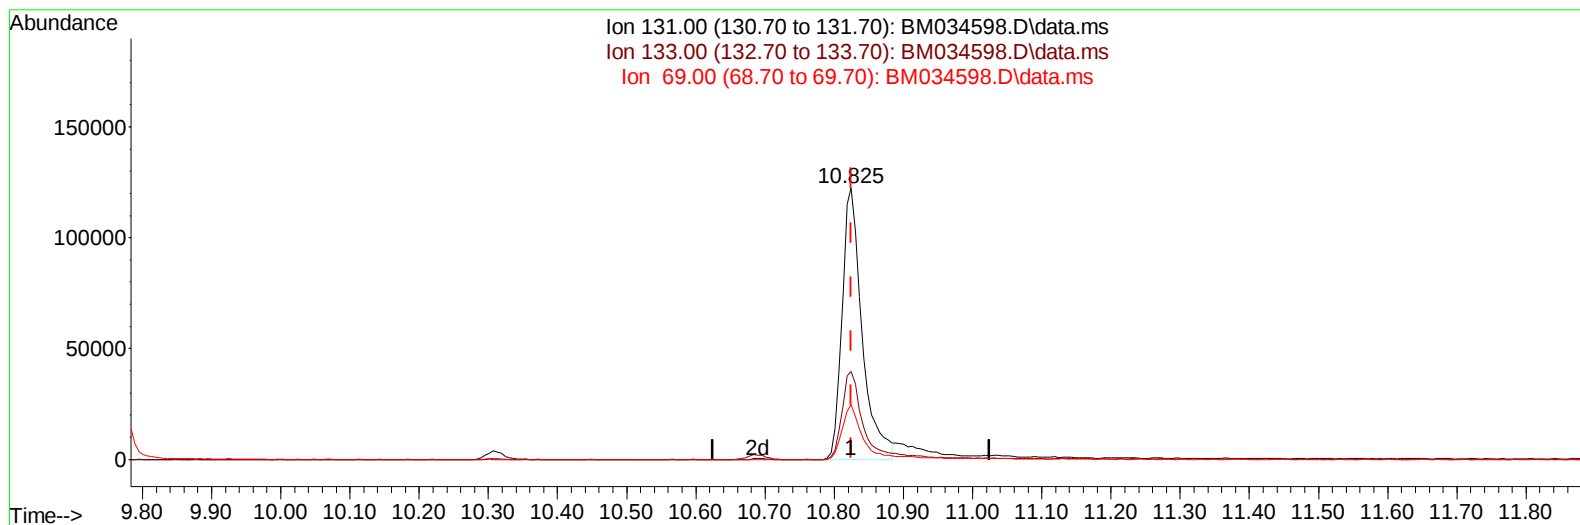

TIC: BM034598.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.825min (0.000) 25.50 ng/u1

response 245589

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.40
69.00	16.80	20.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

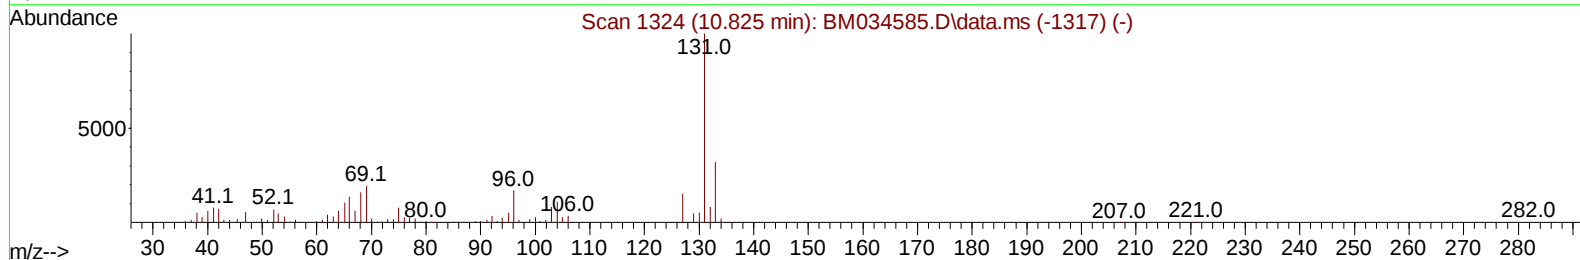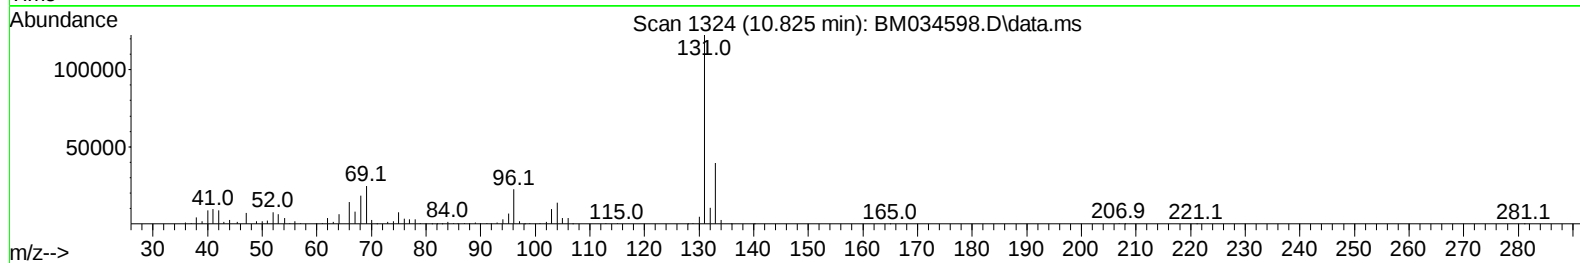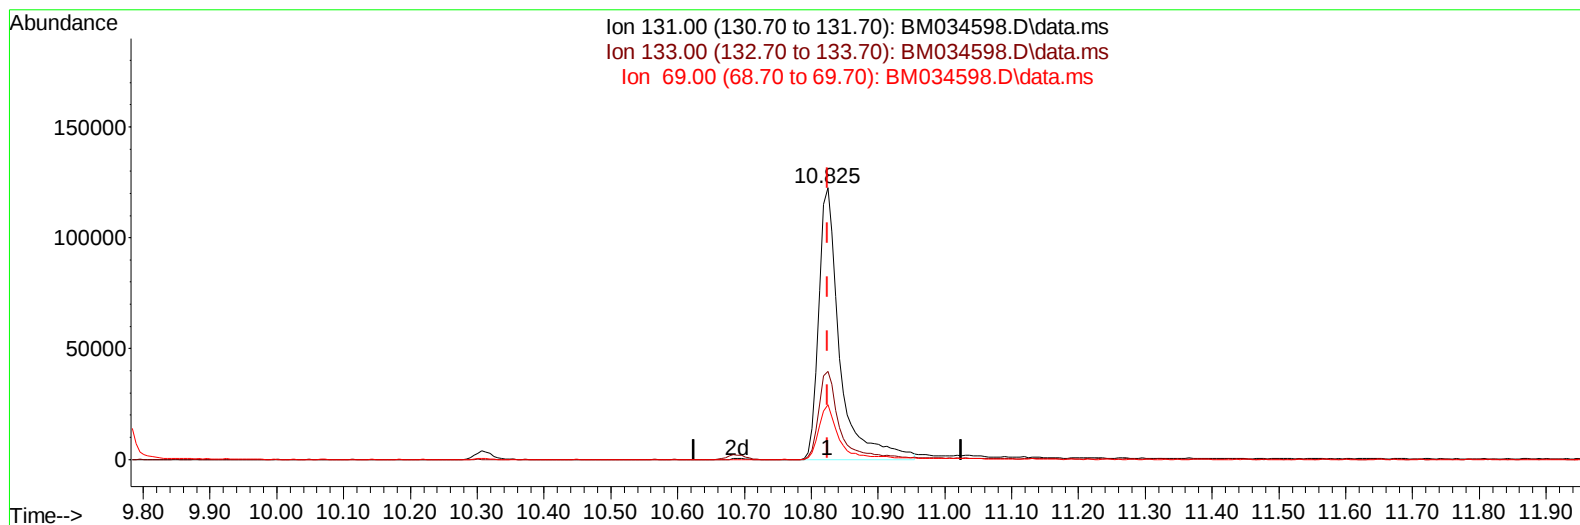

TIC: BM034598.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.825min (0.000) 27.69 ng/ul m

response 266593

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.40
69.00	16.80	20.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

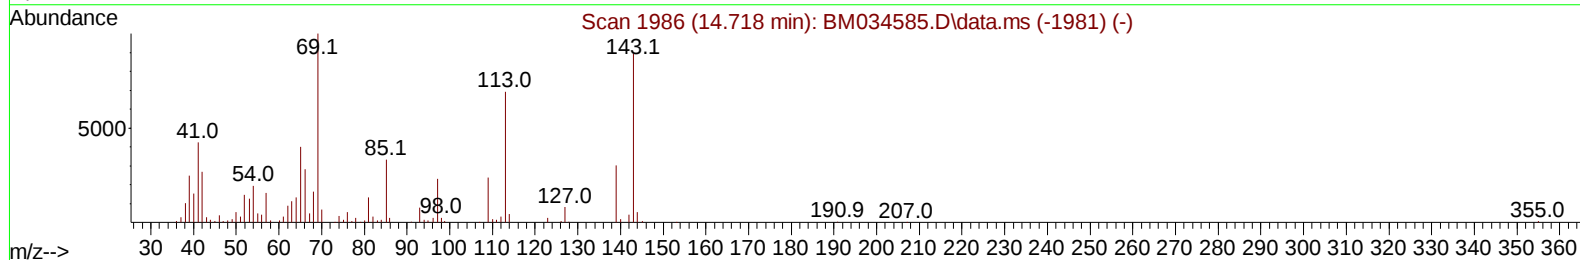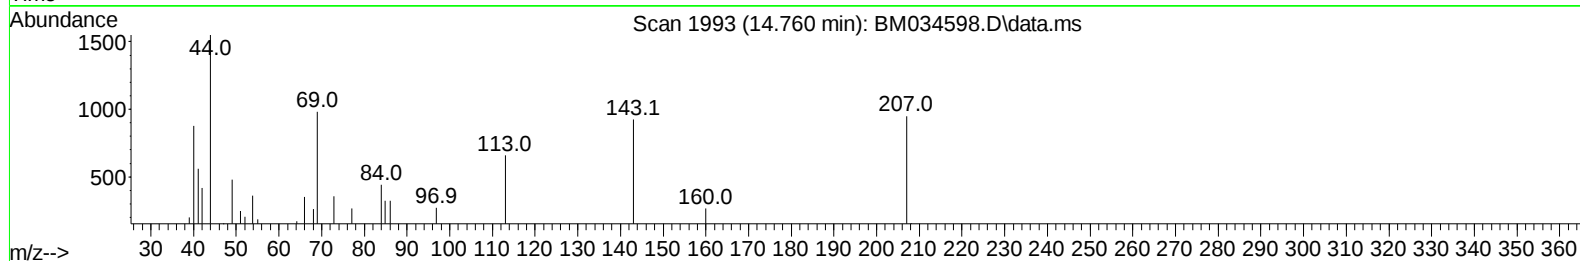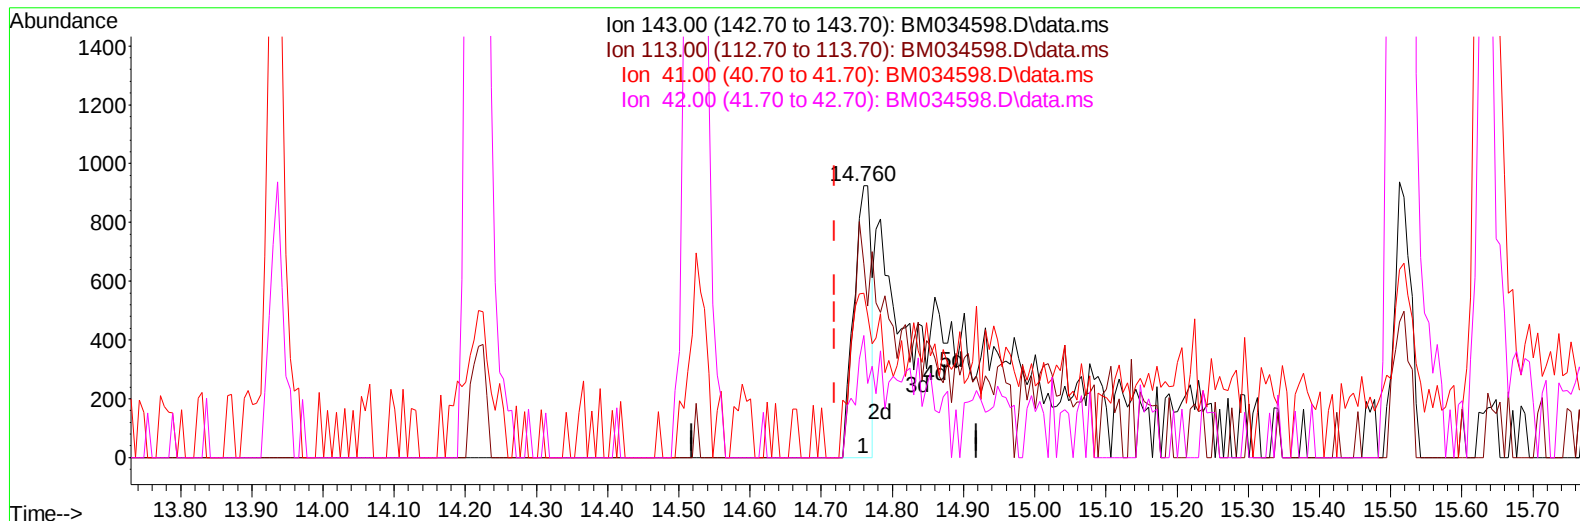

TIC: BM034598.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.760min (+ 0.041) 0.52 ng/u1

response 1587

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	71.32
41.00	31.90	60.61#
42.00	19.10	45.02#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

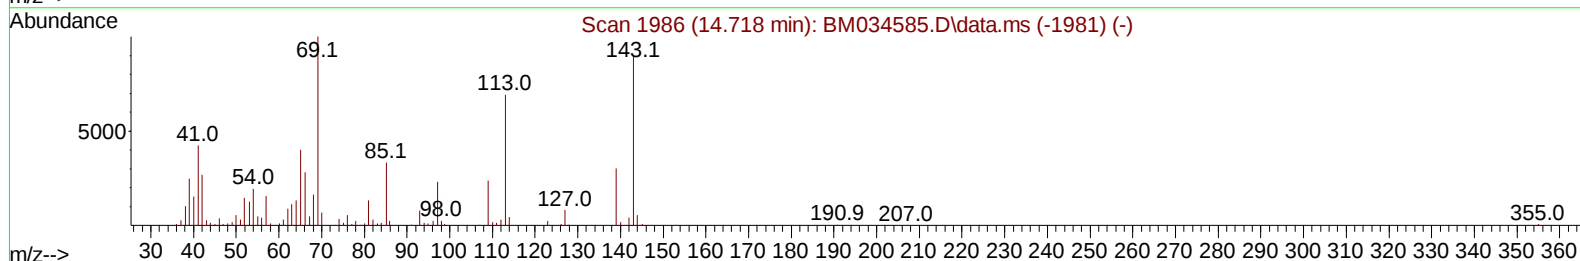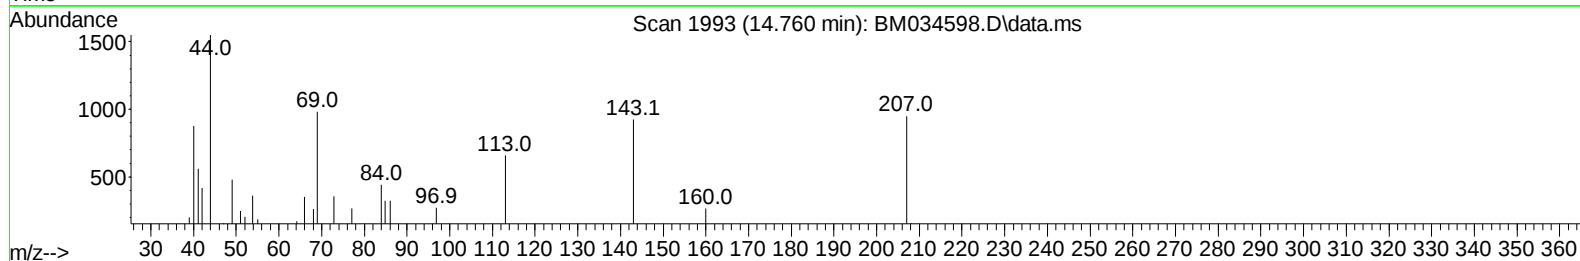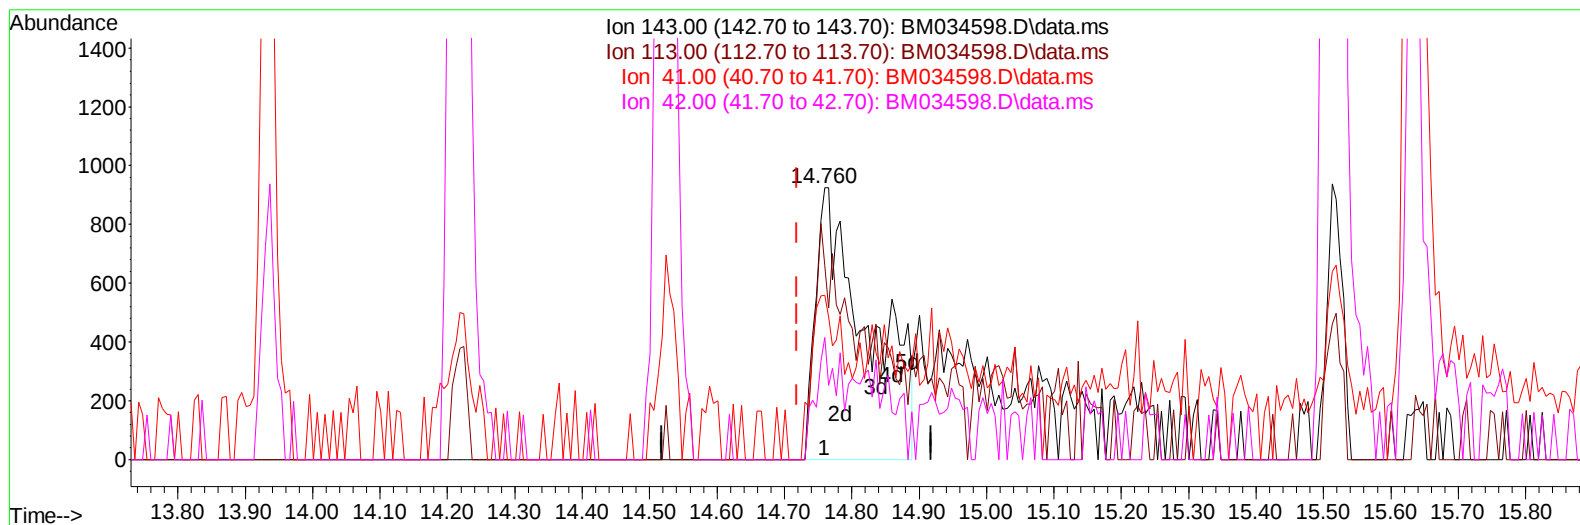

TIC: BM034598.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.760min (+ 0.041) 1.63 ng/ul m

response 4977

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	71.32
41.00	31.90	60.61#
42.00	19.10	45.02#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034598.D
 Acq On : 09 Apr 2022 14:32
 Operator : CG/JU
 Sample : N2266-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 01:00:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.878	152		120144	20.000	ng/ul	0.00
20) Naphthalene-d8	10.683	136		484423	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.524	164		276802	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188		537575	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.442	240		515297	20.000	ng/ul	# 0.00
88) Perylene-d12	23.824	264		620163	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.254	96		13362	3.966	ng/uL	0.00
4) Pyridine-d5	3.690	84		55118	6.779	ng/ul	0.01
7) Phenol-d5	7.042	99		51992	5.199	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67		238970	35.863	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132		198075	25.624	ng/ul	0.00
15) 4-Methylphenol-d8	8.589	113		109900	14.069	ng/ul	0.00
21) Nitrobenzene-d5	9.042	128		130710	36.714	ng/ul	0.00
24) 2-Nitrophenol-d4	9.766	143		122888	33.153	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.307	165		202163m	28.965	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131		266593m	27.686	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166		770739	38.535	ng/ul	0.00
49) Acenaphthylene-d8	14.218	160		922974	35.903	ng/ul	0.00
54) 4-Nitrophenol-d4	14.760	143		4977m	1.632	ng/ul	0.04
60) Fluorene-d10	15.513	176		673874	38.988	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200		92315	28.130	ng/ul	0.00
73) Anthracene-d10	17.365	188		1091486	42.586	ng/ul	0.00
81) Pyrene-d10	19.653	212		1323912	47.073	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264		1239721	39.740	ng/ul	0.00
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.359	149		43229	2.181	ng/ul#	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

