




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034599.D
 Acq On : 09 Apr 2022 15:08
 Operator : CG/JU
 Sample : N2266-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

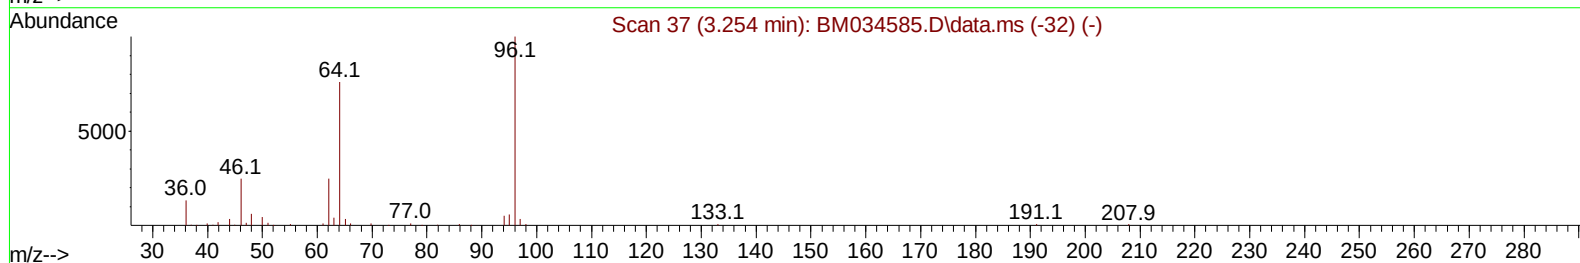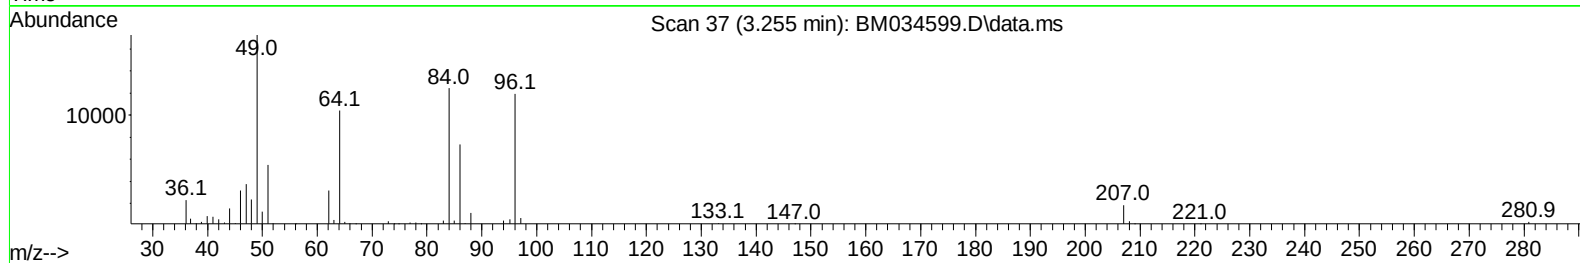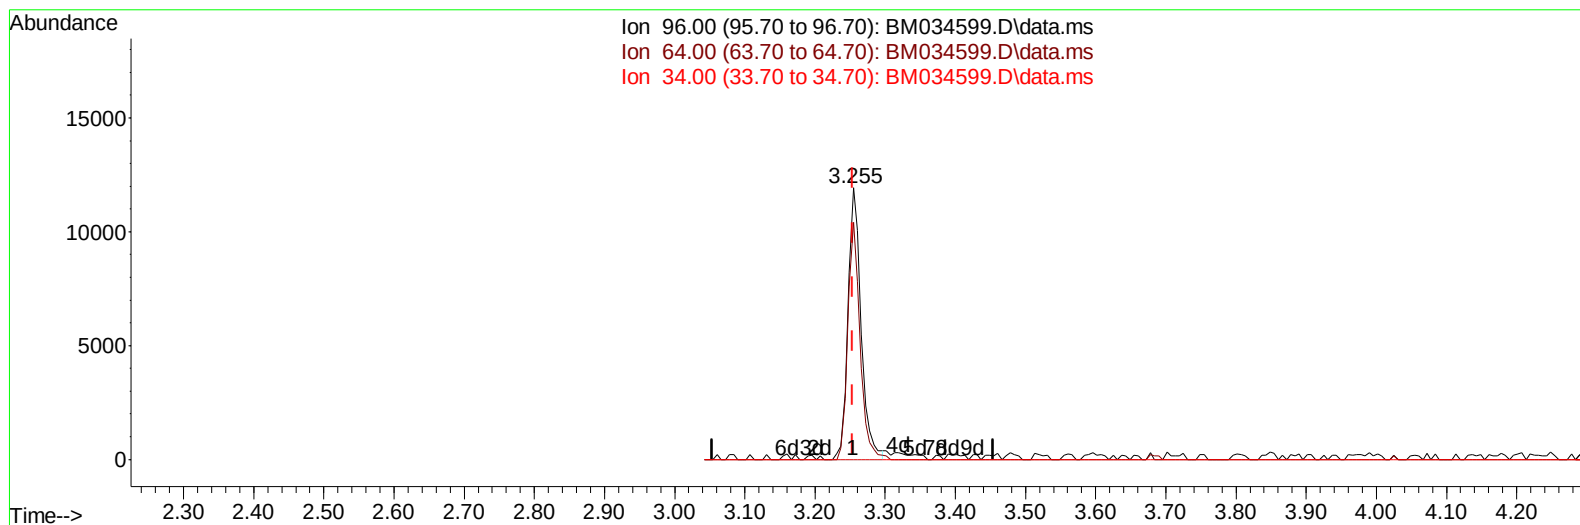

TIC: BM034599.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.255min (+ 0.001) 4.73 ng/uL

response 15678

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	87.26#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

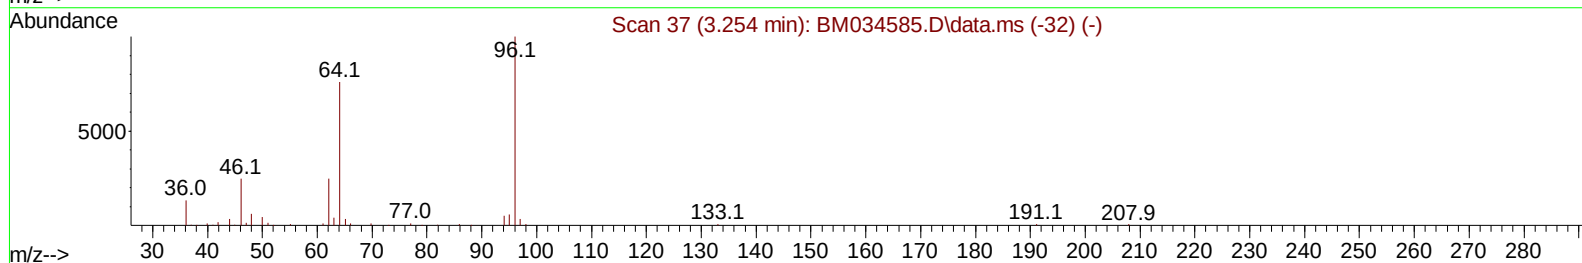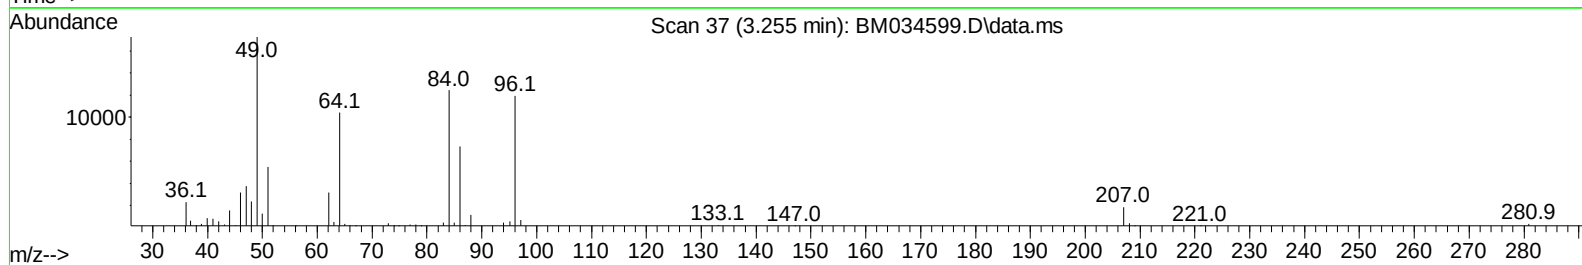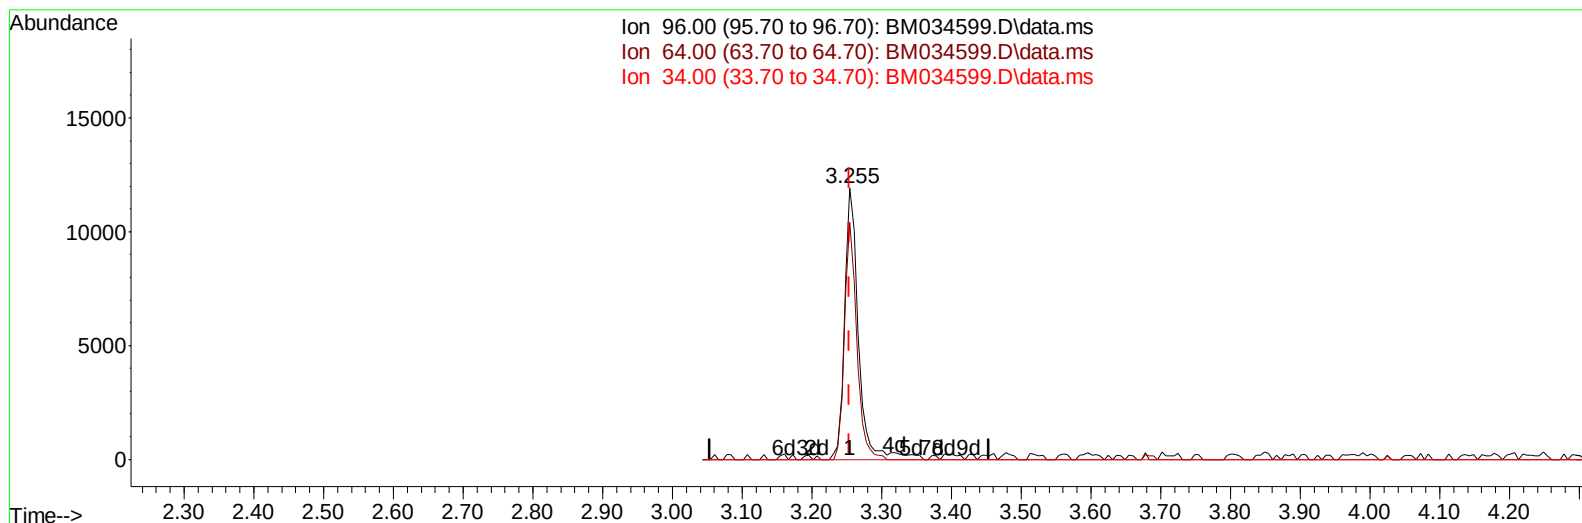

TIC: BM034599.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.255min (+ 0.001) 4.79 ng/uL m

response 15886

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	87.26#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034599.D
 Acq On : 09 Apr 2022 15:08
 Operator : CG/JU
 Sample : N2266-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

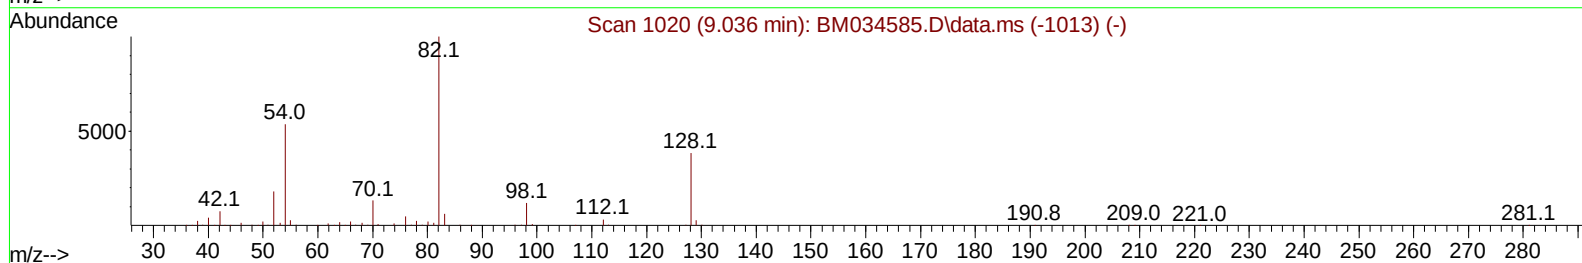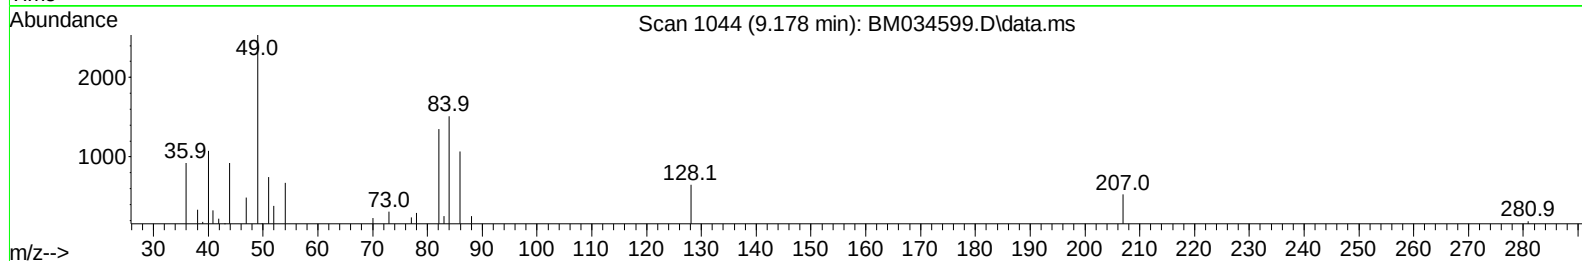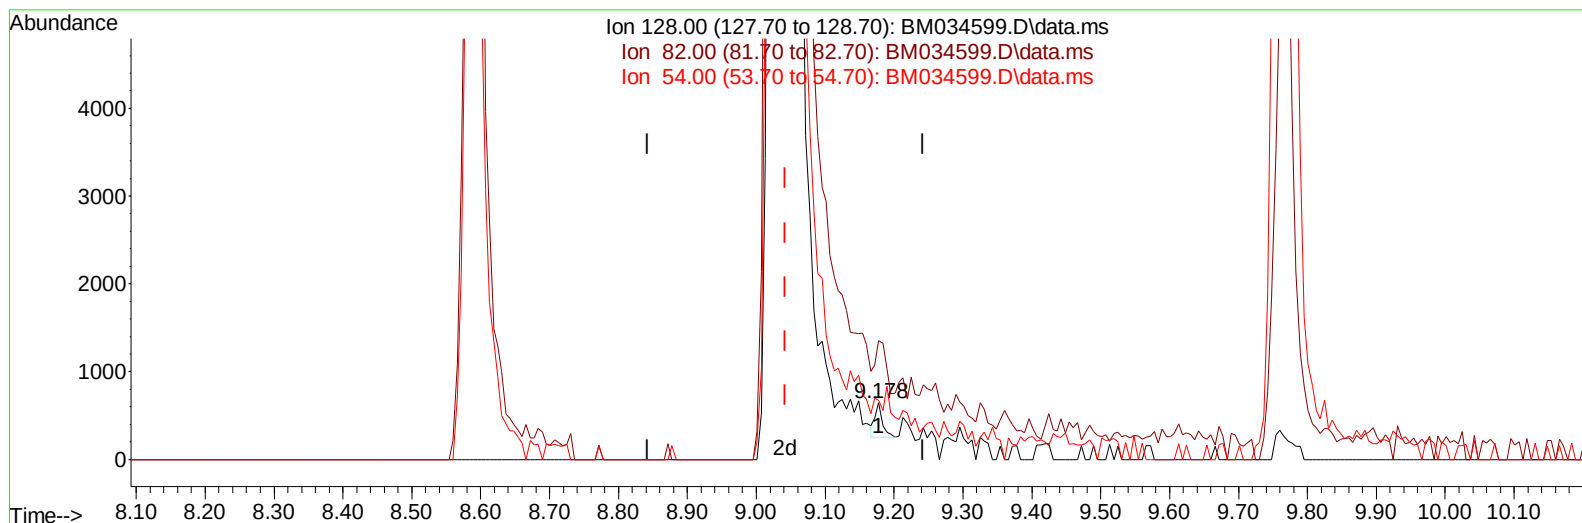

TIC: BM034599.D\data.ms

(21) Nitrobenzene-d5 (S)

9.178min (+ 0.135) 0.09 ng/ul

response 297

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	208.33
54.00	100.50	104.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

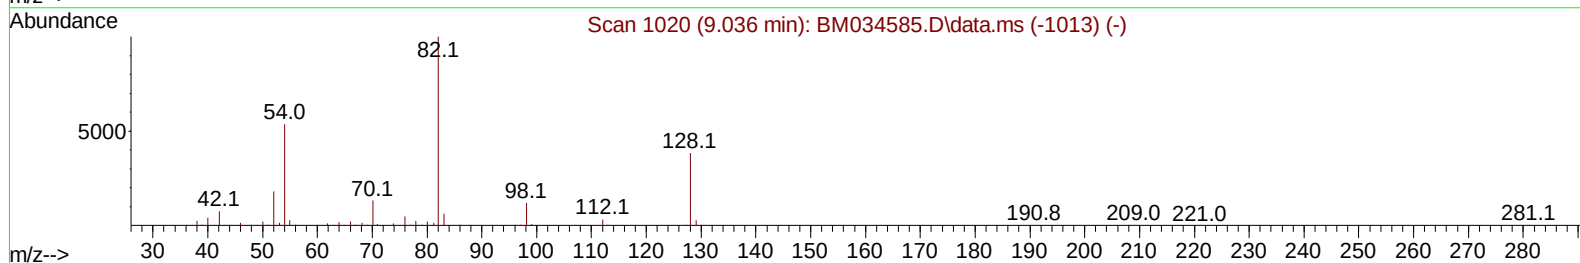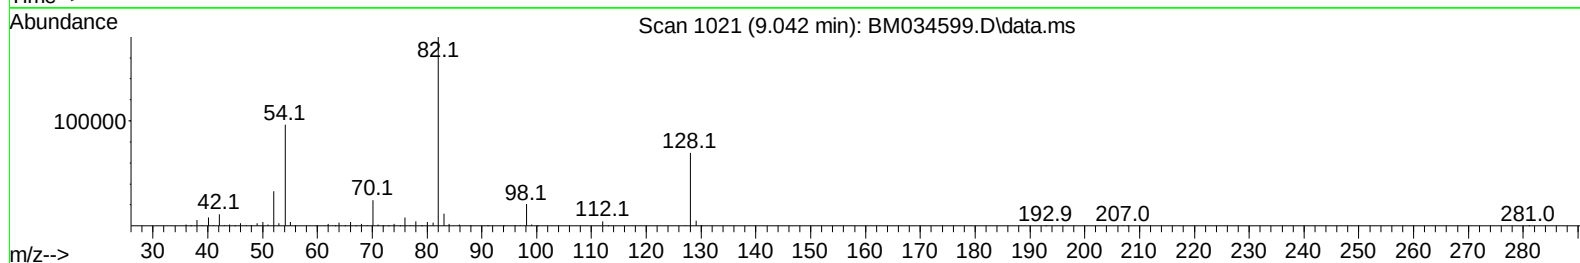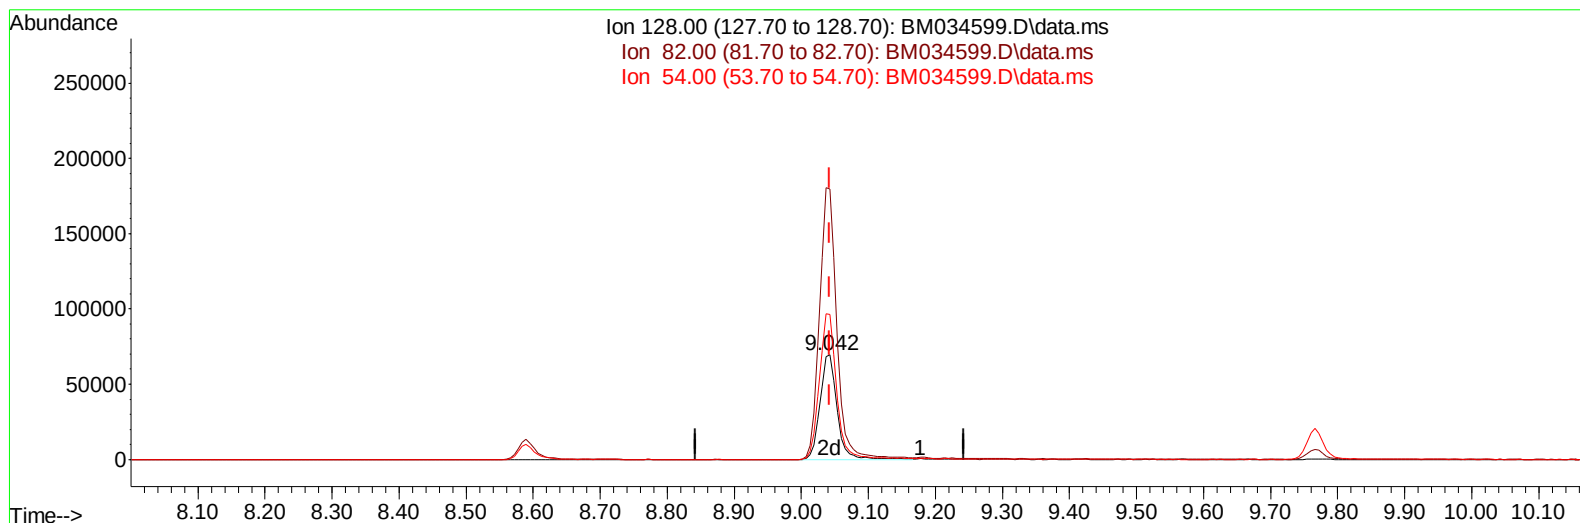

TIC: BM034599.D\data.ms

(21) Nitrobenzene-d5 (S)

9.042min (+ 0.000) 35.54 ng/ul m

response 123300

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	258.45
54.00	100.50	138.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

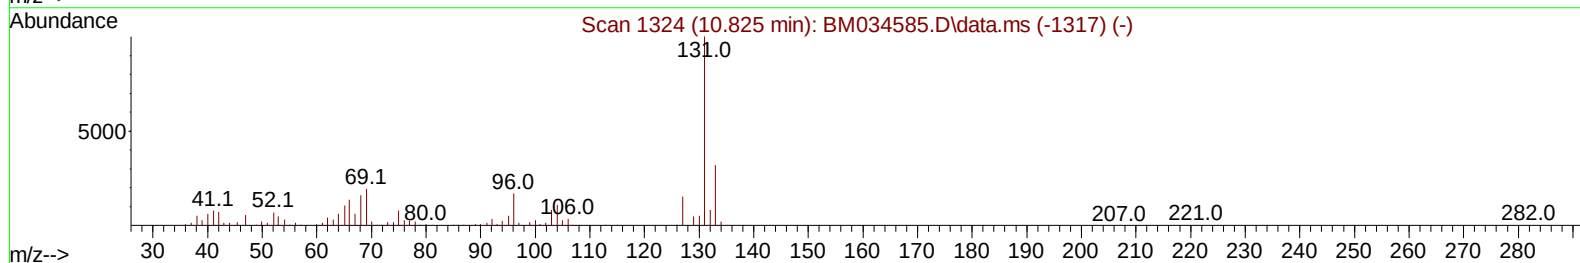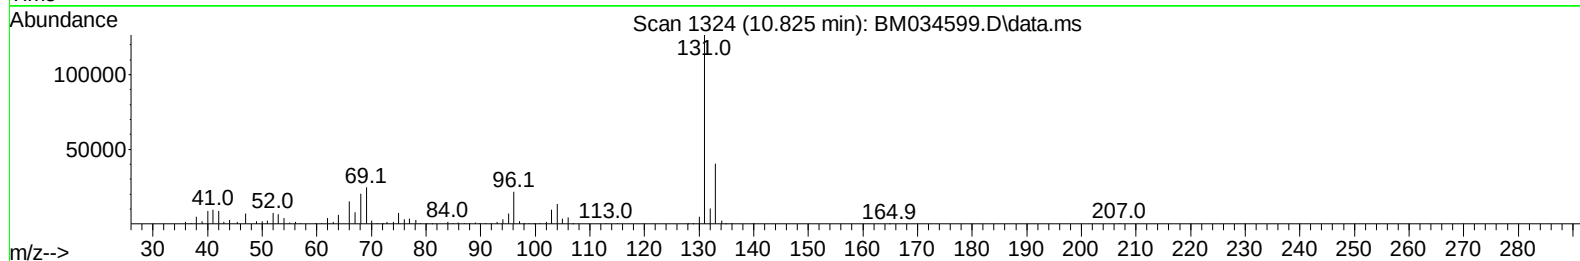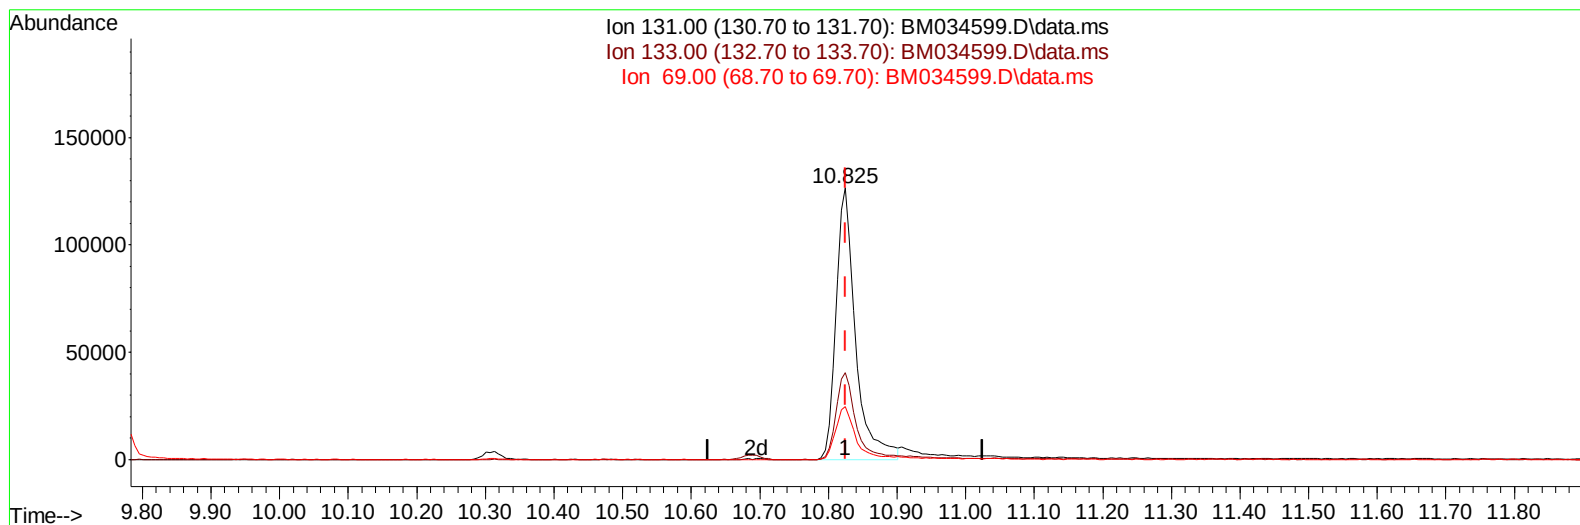

TIC: BM034599.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.825min (+ 0.000) 26.78 ng/ul

response 251299

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.03
69.00	16.80	19.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

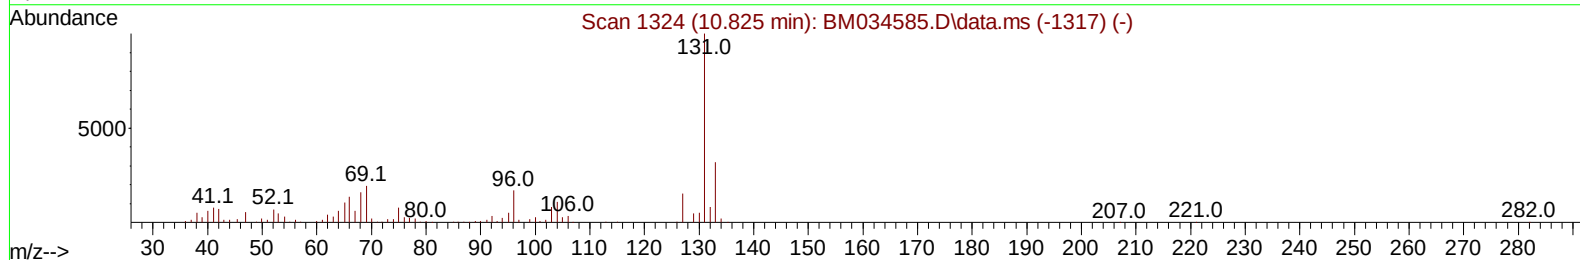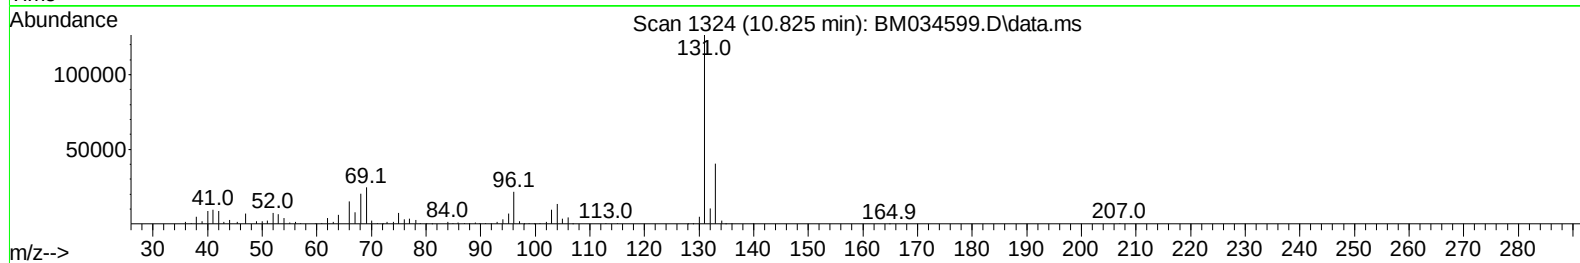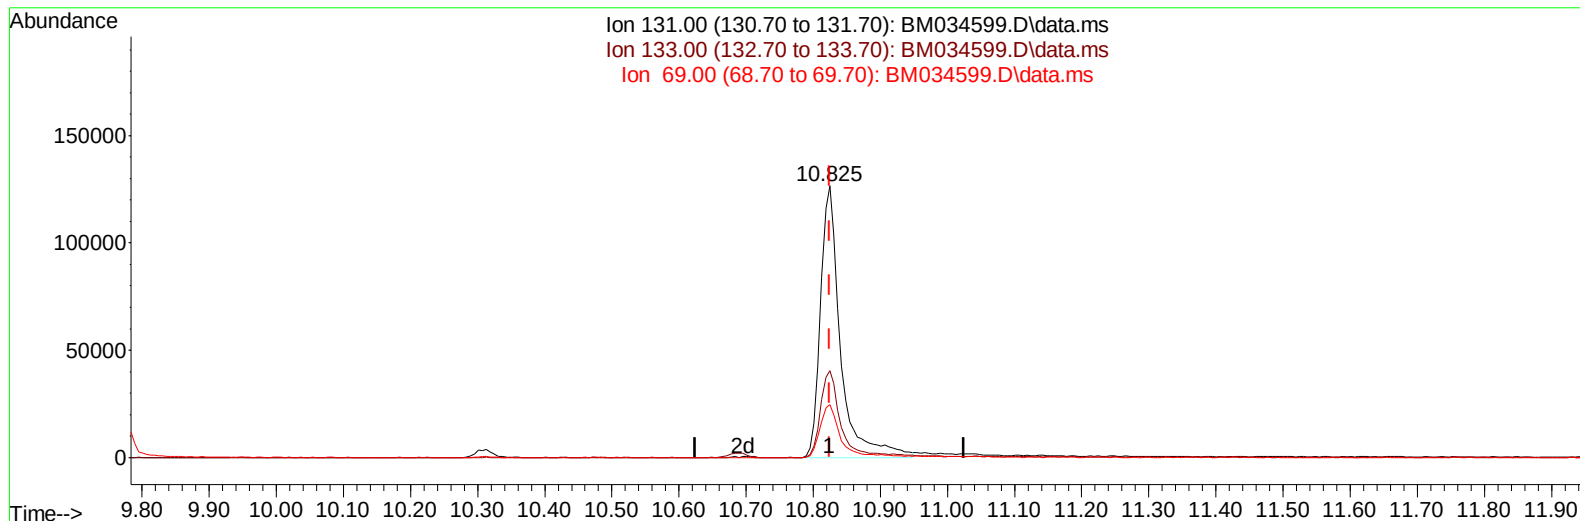

TIC: BM034599.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.825min (+ 0.000) 27.90 ng/ul m

response 261817

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.03
69.00	16.80	19.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

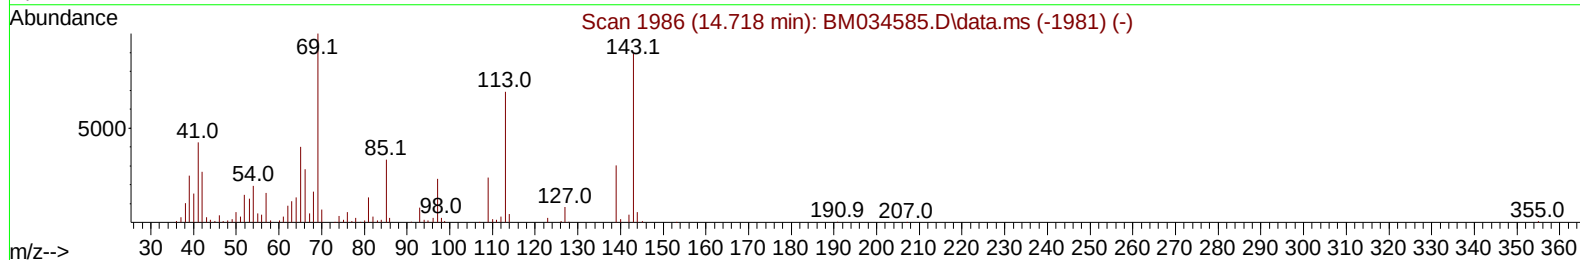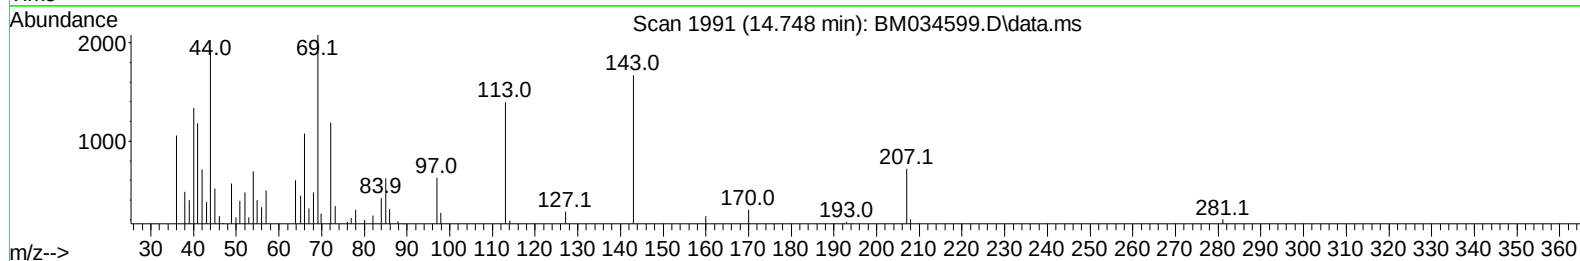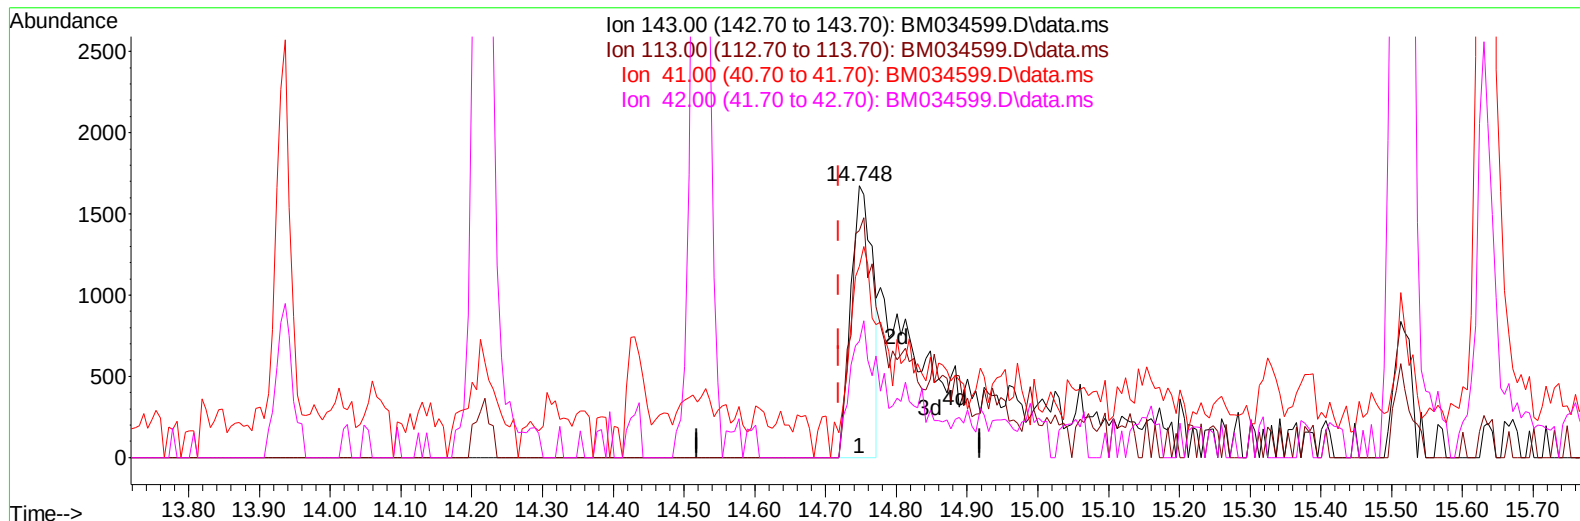

TIC: BM034599.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.748min (+ 0.029) 1.20 ng/ul

response 3579

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	83.61
41.00	31.90	70.51#
42.00	19.10	42.76#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

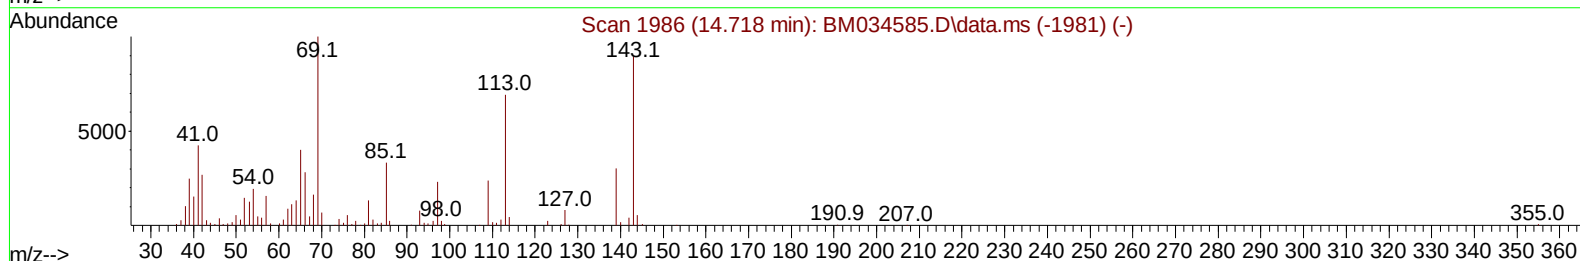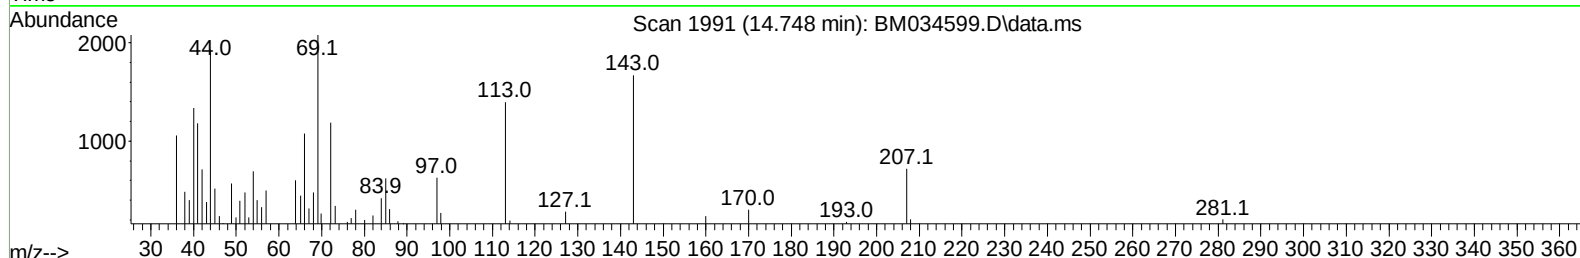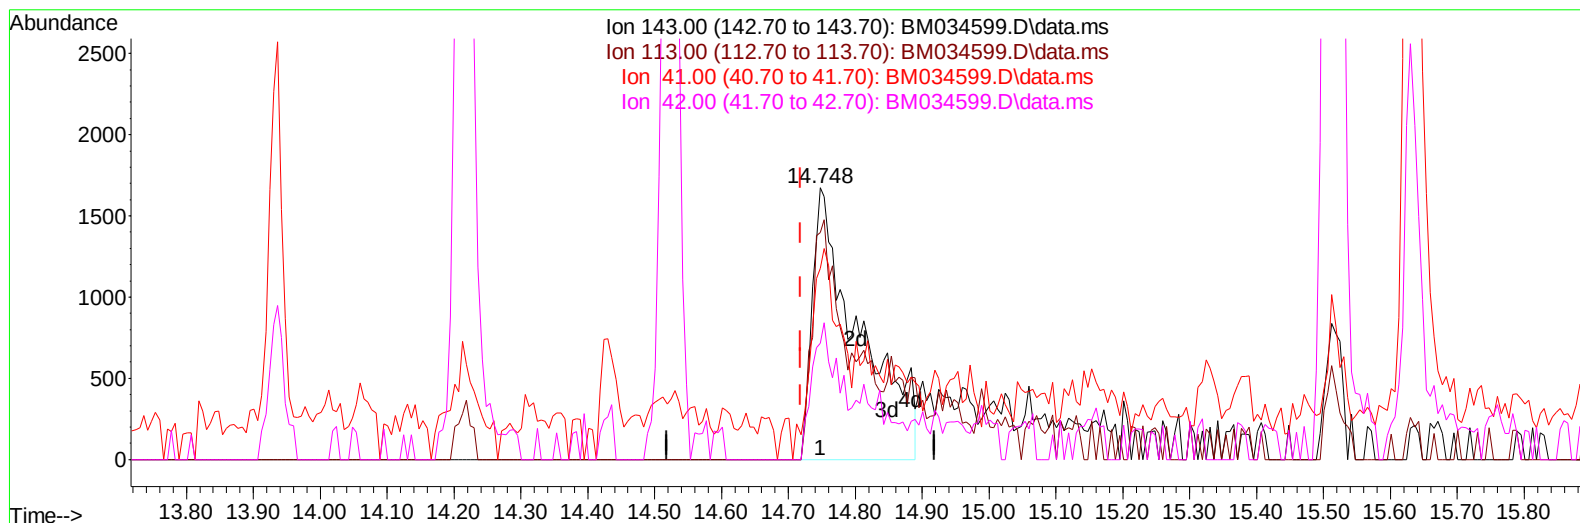

TIC: BM034599.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.748min (+ 0.029) 2.72 ng/ul m

response 8126

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	83.61
41.00	31.90	70.51#
42.00	19.10	42.76#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034599.D
 Acq On : 09 Apr 2022 15:08
 Operator : CG/JU
 Sample : N2266-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ24

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 01:00:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	118286	20.000	ng/ul	0.00
20) Naphthalene-d8	10.683	136	472084	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.524	164	271188	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188	530513	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.442	240	531087	20.000	ng/ul	# 0.00
88) Perylene-d12	23.824	264	637995	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	15886m	4.789	ng/uL	0.00
4) Pyridine-d5	3.684	84	84470	10.552	ng/ul	0.00
7) Phenol-d5	7.043	99	54617	5.548	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	223035	33.997	ng/ul	0.00
11) 2-Chlorophenol-d4	7.407	132	181872	23.897	ng/ul	0.00
15) 4-Methylphenol-d8	8.589	113	107781	14.015	ng/ul	0.00
21) Nitrobenzene-d5	9.042	128	123300m	35.538	ng/ul	0.00
24) 2-Nitrophenol-d4	9.766	143	113966	31.550	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	178679	26.269	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131	261817m	27.901	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	754404	38.499	ng/ul	0.00
49) Acenaphthylene-d8	14.219	160	893035	35.458	ng/ul	0.00
54) 4-Nitrophenol-d4	14.748	143	8126m	2.720	ng/ul	0.03
60) Fluorene-d10	15.513	176	663461	39.180	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	97893	30.226	ng/ul	0.00
73) Anthracene-d10	17.365	188	1025997	40.564	ng/ul	0.00
81) Pyrene-d10	19.653	212	1267137	43.715	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.671	264	1253341	39.054	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:00:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

