

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034598.D
 Acq On : 09 Apr 2022 14:32
 Operator : CG/JU
 Sample : N2266-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 11 01:00:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 08 14:30:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	120144	20.000	ng/u1	0.00
20) Naphthalene-d8	10.683	136	484423	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.524	164	276802	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.265	188	537575	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.442	240	515297	20.000	ng/u1	# 0.00
88) Perylene-d12	23.824	264	620163	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.254	96	13362	3.966	ng/uL	0.00
4) Pyridine-d5	3.690	84	55118	6.779	ng/u1	0.01
7) Phenol-d5	7.042	99	51992	5.199	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	238970	35.863	ng/u1	0.00
11) 2-Chlorophenol-d4	7.407	132	198075	25.624	ng/u1	0.00
15) 4-Methylphenol-d8	8.589	113	109900	14.069	ng/u1	0.00
21) Nitrobenzene-d5	9.042	128	130710	36.714	ng/u1	0.00
24) 2-Nitrophenol-d4	9.766	143	122888	33.153	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.307	165	202163m	28.965	ng/u1	0.00
31) 4-Chloroaniline-d4	10.825	131	266593m	27.686	ng/u1	0.00
46) Dimethylphthalate-d6	13.936	166	770739	38.535	ng/u1	0.00
49) Acenaphthylene-d8	14.218	160	922974	35.903	ng/u1	0.00
54) 4-Nitrophenol-d4	14.760	143	4977m	1.632	ng/u1	0.04
60) Fluorene-d10	15.513	176	673874	38.988	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.636	200	92315	28.130	ng/u1	0.00
73) Anthracene-d10	17.365	188	1091486	42.586	ng/u1	0.00
81) Pyrene-d10	19.653	212	1323912	47.073	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.671	264	1239721	39.740	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.359	149	43229	2.181	ng/u1#	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YAYW2

Quant Time: Apr 11 01:00:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 08 14:30:08 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

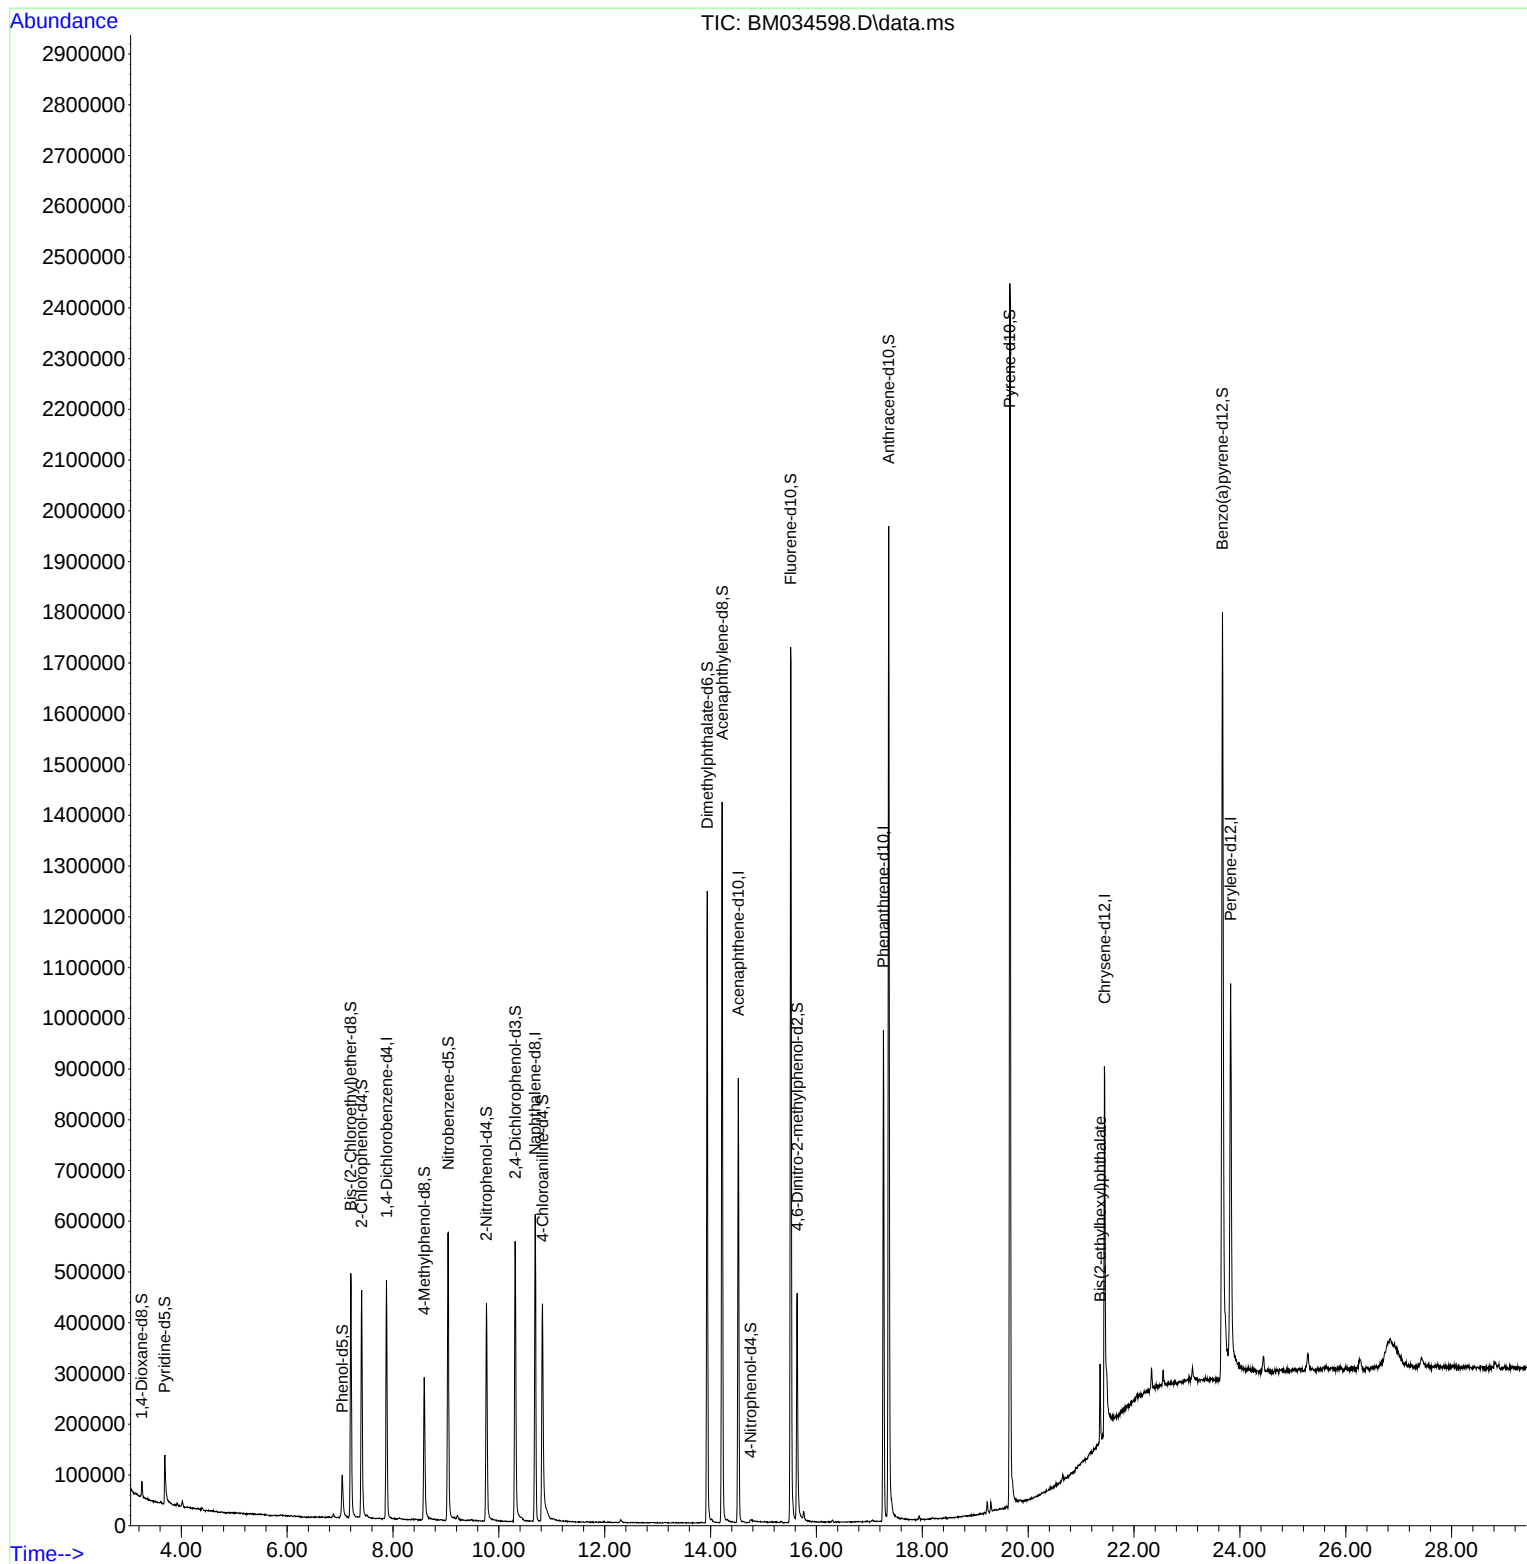

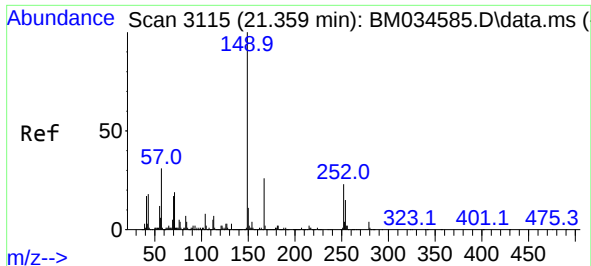

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.181 ng/ul
 RT: 21.359 min Scan# 3115
 Delta R.T. 0.000 min
 Lab File: BM034598.D
 Acq: 09 Apr 2022 14:32

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

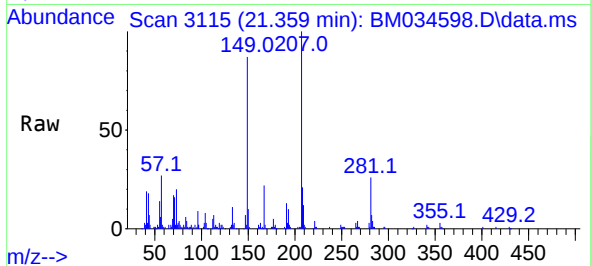

Tgt Ion:	149	Resp:	43229
Ion Ratio	Lower	Upper	
149	100		
167	25.5	22.1	33.1
279	3.8	4.2	6.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

