

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034563.D
 Acq On : 08 Apr 2022 16:06
 Operator : CG/JU
 Sample : PB143957BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK957

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	33	36	44	rVB	41669	58592	2.62%	0.254%
2	3.678	106	109	127	rBV	385653	603154	26.95%	2.613%
3	4.019	164	167	172	rVB3	8782	12585	0.56%	0.055%
4	7.037	674	680	701	rBV	395277	720972	32.22%	3.123%
5	7.202	702	708	720	rVV	361456	587156	26.24%	2.544%
6	7.407	736	743	758	rBV	450345	771682	34.48%	3.343%
7	7.878	816	823	832	rBV	354034	575953	25.74%	2.495%
8	8.590	938	944	958	rVV	476323	864451	38.63%	3.745%
9	9.037	1013	1020	1036	rBV	399978	725752	32.43%	3.144%
10	9.384	1076	1079	1080	rVB3	2867	2380	0.11%	0.010%
11	9.407	1080	1083	1084	rBV2	2312	2639	0.12%	0.011%
12	9.643	1121	1123	1128	rBV5	1553	2555	0.11%	0.011%
13	9.766	1136	1144	1162	rBV	312431	581010	25.96%	2.517%
14	10.013	1184	1186	1190	rVB5	2016	2309	0.10%	0.010%
15	10.307	1230	1236	1252	rBV	404158	790896	35.34%	3.426%
16	10.690	1293	1301	1310	rBV	462246	783828	35.02%	3.396%
17	10.825	1317	1324	1348	rBV	314730	753259	33.66%	3.263%
18	11.866	1498	1501	1503	rBV4	1853	2438	0.11%	0.011%
19	11.901	1503	1507	1509	rBV4	1982	2713	0.12%	0.012%
20	12.319	1569	1578	1584	rBV6	5218	12427	0.56%	0.054%
21	12.913	1677	1679	1686	rVB6	2111	2918	0.13%	0.013%
22	13.507	1777	1780	1786	rVB6	1389	2619	0.12%	0.011%
23	13.795	1824	1829	1831	rBV4	1442	2330	0.10%	0.010%
24	13.831	1831	1835	1837	rBV3	3100	3781	0.17%	0.016%
25	13.936	1846	1853	1864	rBV	821273	1226446	54.80%	5.313%
26	14.219	1894	1901	1916	rBV	920484	1410724	63.04%	6.111%
27	14.525	1947	1953	1962	rBV	624882	925224	41.34%	4.008%
28	14.725	1982	1987	2006	rBV	70716	270882	12.10%	1.173%
29	15.336	2088	2091	2095	rVB4	3103	4515	0.20%	0.020%
30	15.519	2115	2122	2136	rBV	1163444	1750550	78.22%	7.583%
31	15.636	2136	2142	2155	rVV	319412	551486	24.64%	2.389%
32	15.754	2159	2162	2168	rVB3	12938	19239	0.86%	0.083%
33	16.072	2211	2216	2218	rBV5	1348	2306	0.10%	0.010%
34	16.307	2253	2256	2259	rBV5	3356	3607	0.16%	0.016%
35	16.766	2330	2334	2335	rBV4	2716	3315	0.15%	0.014%
36	17.266	2413	2419	2429	rBV	692479	1013678	45.29%	4.391%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034563.D
 Acq On : 08 Apr 2022 16:06
 Operator : CG/JU
 Sample : PB143957BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK957

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	17.366	2430	2436	2454	rVB	1175236	1821028	81.37%	7.889%
38	17.777	2504	2506	2509	rBV3	1851	2345	0.10%	0.010%
39	18.083	2555	2558	2560	rBV4	2896	3983	0.18%	0.017%
40	18.783	2675	2677	2680	rBV3	3099	2268	0.10%	0.010%
41	18.871	2690	2692	2695	rBV4	2467	3112	0.14%	0.013%
42	19.230	2749	2753	2759	rVB5	13934	17387	0.78%	0.075%
43	19.301	2761	2765	2768	rBV	11169	14773	0.66%	0.064%
44	19.660	2820	2826	2845	rBV	1450542	2237981	100.00%	9.695%
45	21.448	3125	3130	3135	rBV	475167	784867	35.07%	3.400%
46	23.677	3502	3509	3526	rBV2	850776	2034042	90.89%	8.812%
47	23.824	3529	3534	3549	rVB2	480057	1111536	49.67%	4.815%


Sum of corrected areas: 23083693

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

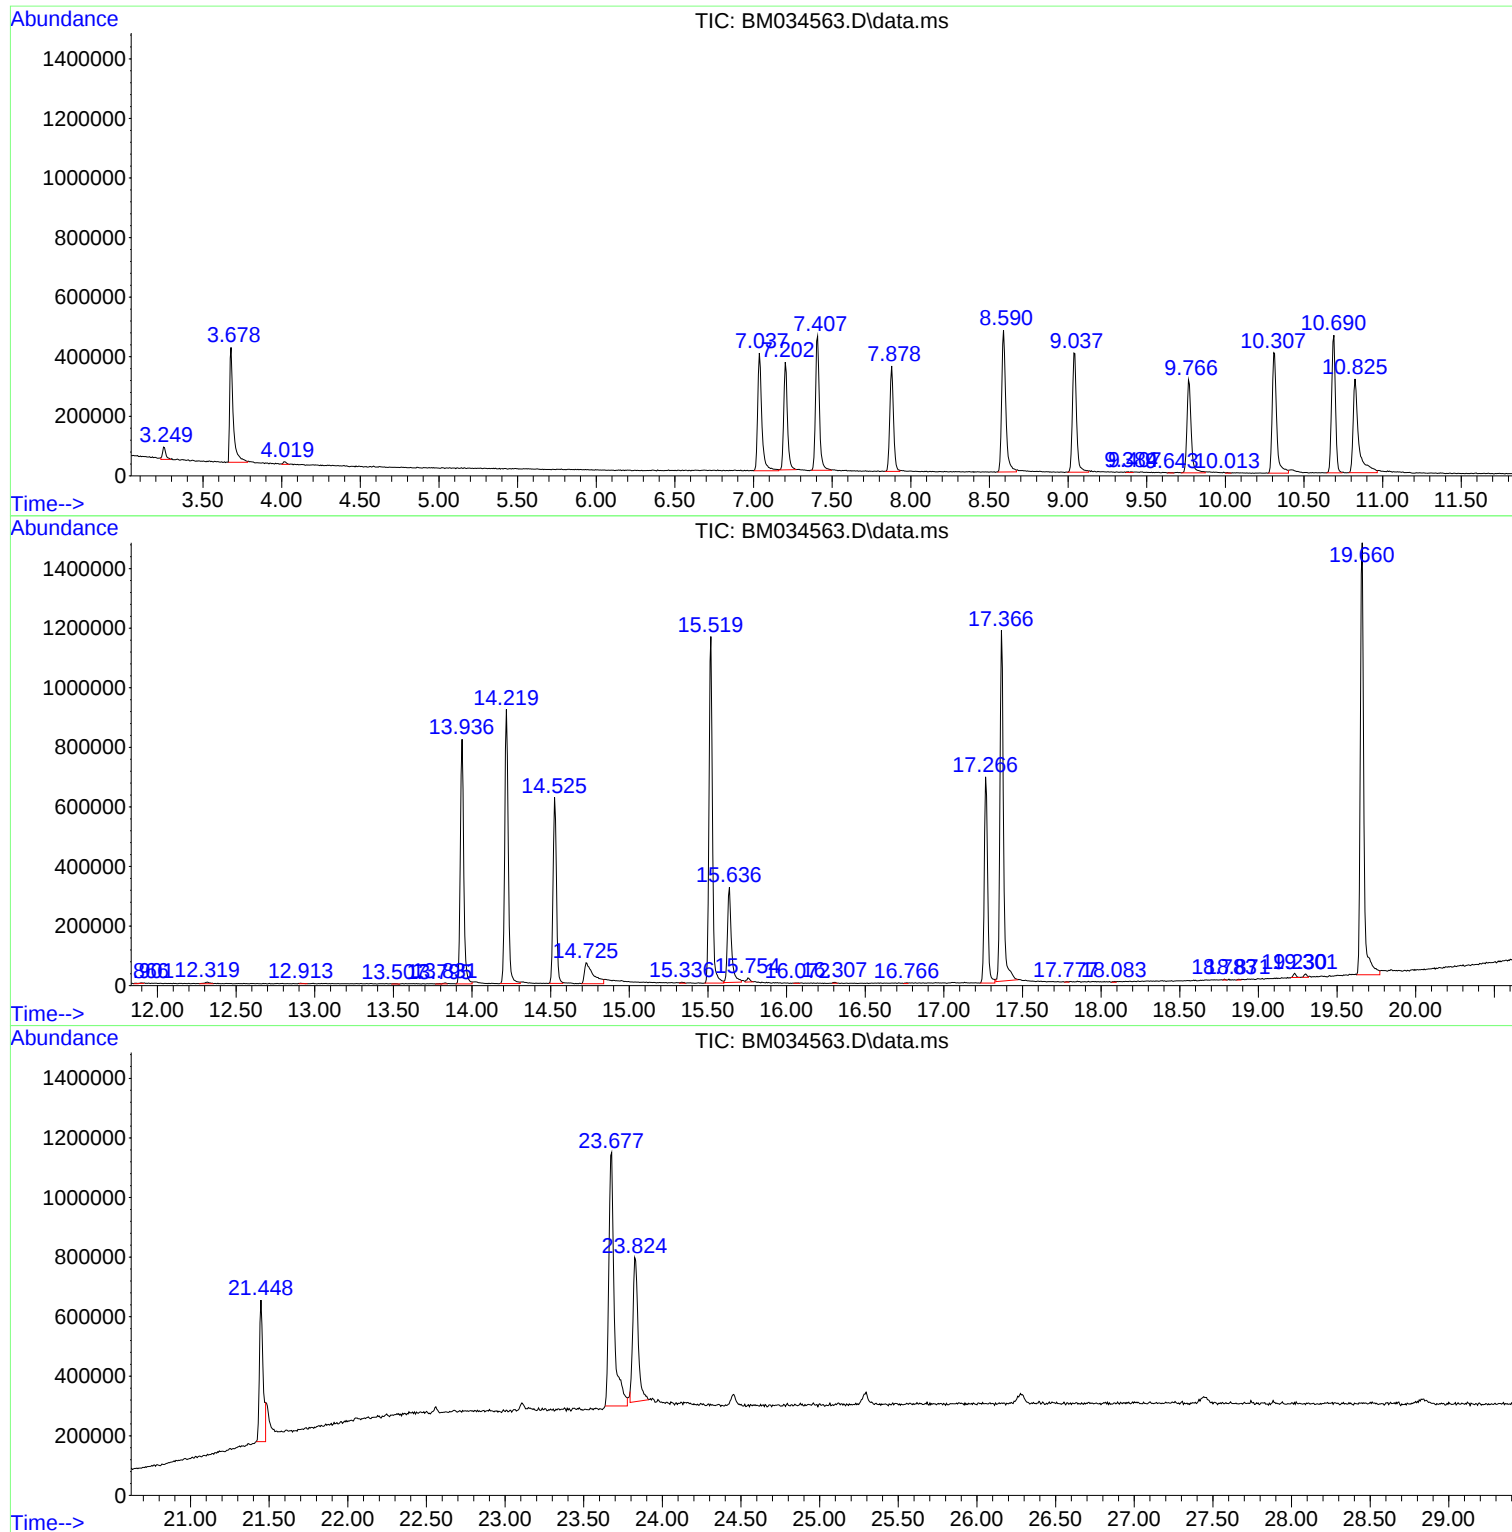

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034563.D
Acq On : 08 Apr 2022 16:06
Operator : CG/JU
Sample : PB143957BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc