

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034564.D
 Acq On : 08 Apr 2022 16:42
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	33	37	43	rVB2	29326	37030	1.62%	0.177%
2	3.684	107	110	122	rBV	94386	160247	7.01%	0.765%
3	4.019	164	167	171	rVB3	9281	11864	0.52%	0.057%
4	6.872	649	652	657	rVB6	4359	6868	0.30%	0.033%
5	7.042	674	681	690	rVV2	52488	117860	5.16%	0.563%
6	7.201	702	708	723	rBV	324216	565424	24.73%	2.699%
7	7.407	737	743	758	rBV	292483	518370	22.68%	2.475%
8	7.878	817	823	834	rBV	332052	559274	24.47%	2.670%
9	8.125	861	865	871	rVB6	3203	7124	0.31%	0.034%
10	8.495	926	928	932	rBV5	1734	2520	0.11%	0.012%
11	8.589	938	944	958	rBV	173178	348149	15.23%	1.662%
12	9.042	1014	1021	1032	rBV	375023	684494	29.94%	3.268%
13	9.207	1047	1049	1058	rVB7	4057	9988	0.44%	0.048%
14	9.483	1092	1096	1101	rVB3	11349	17719	0.78%	0.085%
15	9.766	1138	1144	1156	rBV	271725	516616	22.60%	2.466%
16	10.313	1230	1237	1252	rBV	343280	672914	29.44%	3.213%
17	10.689	1293	1301	1309	rBV	434474	756143	33.08%	3.610%
18	10.824	1317	1324	1354	rBV	214146	594759	26.02%	2.839%
19	11.907	1505	1508	1511	rVB3	1761	2310	0.10%	0.011%
20	11.989	1517	1522	1529	rVB3	12797	19577	0.86%	0.093%
21	12.319	1570	1578	1582	rVB6	2897	7601	0.33%	0.036%
22	12.907	1673	1678	1681	rBV4	2025	3300	0.14%	0.016%
23	13.513	1775	1781	1784	rBV5	2826	4193	0.18%	0.020%
24	13.830	1828	1835	1838	rBV6	2856	5278	0.23%	0.025%
25	13.936	1847	1853	1866	rBV	780007	1164573	50.94%	5.560%
26	14.018	1866	1867	1874	rVB3	6149	6866	0.30%	0.033%
27	14.218	1893	1901	1914	rBV	917357	1379447	60.34%	6.586%
28	14.524	1943	1953	1976	rBV2	648866	1092460	47.79%	5.215%
29	14.771	1991	1995	1997	rBV4	3522	5097	0.22%	0.024%
30	15.518	2115	2122	2136	rBV	1125154	1749196	76.52%	8.351%
31	15.636	2136	2142	2159	rVV	297290	544402	23.81%	2.599%
32	15.759	2159	2163	2172	rVB4	14255	31261	1.37%	0.149%
33	16.071	2212	2216	2217	rBV3	1860	2367	0.10%	0.011%
34	16.301	2249	2255	2259	rBV	12329	24174	1.06%	0.115%
35	16.342	2259	2262	2269	rVB	6257	12854	0.56%	0.061%
36	17.059	2378	2384	2386	rBV5	2269	3457	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034564.D
 Acq On : 08 Apr 2022 16:42
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	17.177	2402	2404	2408	rVB4	1834	2606	0.11%	0.012%
38	17.265	2413	2419	2428	rBV	679676	962175	42.09%	4.593%
39	17.365	2430	2436	2455	rVB2	1259772	1935416	84.66%	9.240%
40	17.948	2530	2535	2539	rBV6	4343	7495	0.33%	0.036%
41	18.112	2560	2563	2570	rBV8	3513	5221	0.23%	0.025%
42	18.189	2574	2576	2581	rVV6	1910	3376	0.15%	0.016%
43	18.289	2590	2593	2594	rBV3	2122	2411	0.11%	0.012%
44	18.783	2675	2677	2680	rBV4	2608	4042	0.18%	0.019%
45	19.230	2748	2753	2756	rBV4	14970	22426	0.98%	0.107%
46	19.300	2761	2765	2771	rVV3	12747	20377	0.89%	0.097%
47	19.659	2820	2826	2833	rBV	1592666	2285976	100.00%	10.913%
48	20.659	2993	2996	3001	rVB3	37129	44379	1.94%	0.212%
49	21.447	3125	3130	3135	rBV	486088	783486	34.27%	3.740%
50	23.671	3502	3508	3527	rBV2	956287	2145564	93.86%	10.243%
51	23.824	3528	3534	3546	rVB2	466226	1075722	47.06%	5.136%




Sum of corrected areas: 20946448

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

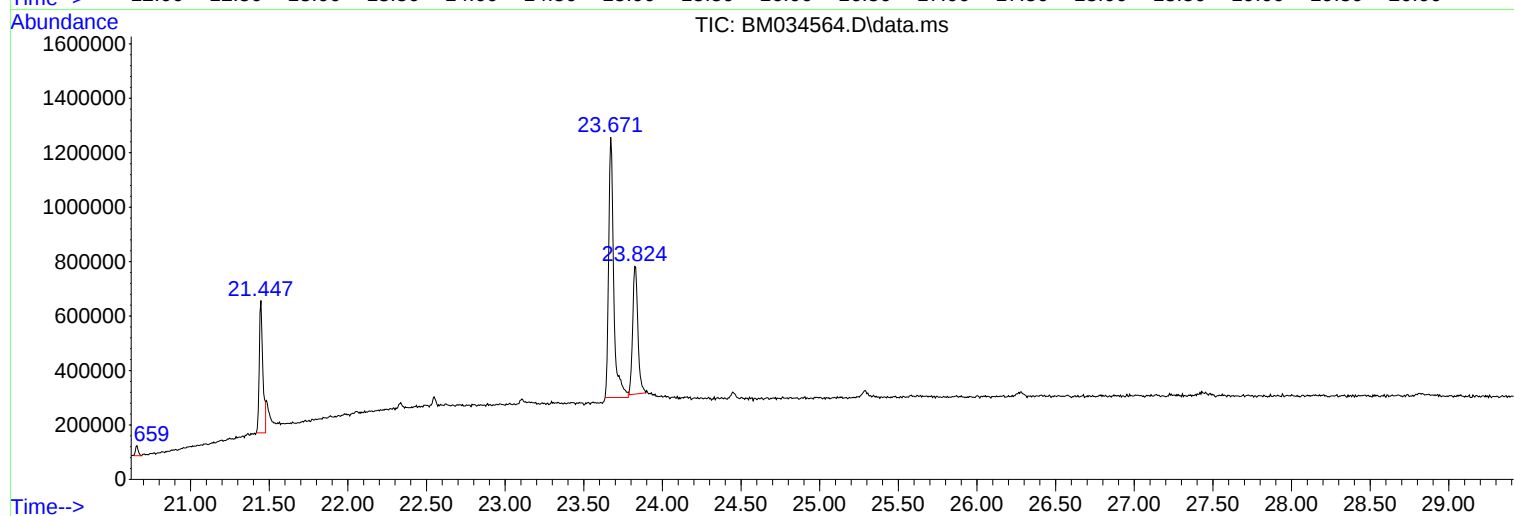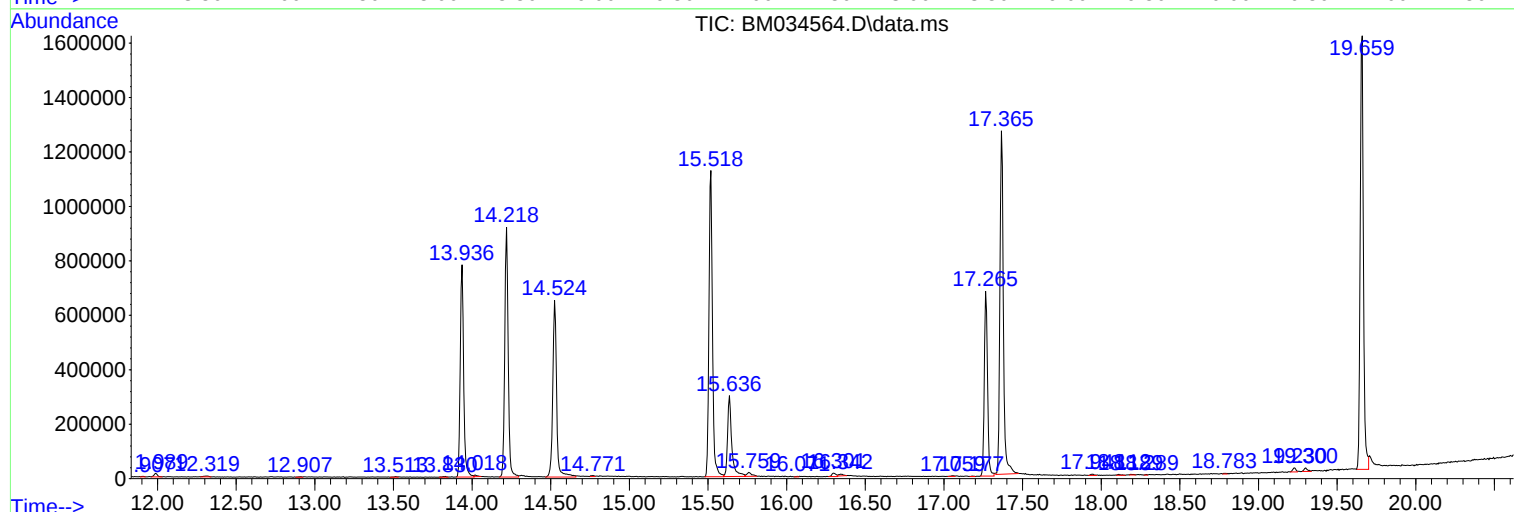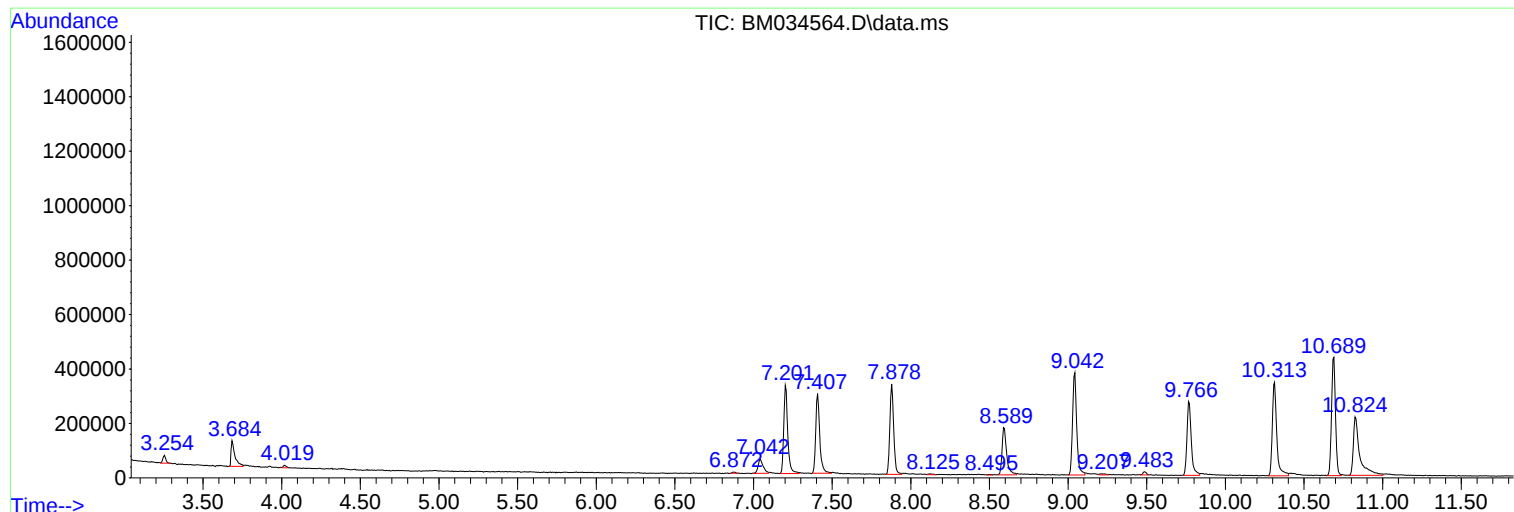

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034564.D
Acq On : 08 Apr 2022 16:42
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------