

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034566.D
 Acq On : 08 Apr 2022 17:56
 Operator : CG/JU
 Sample : N2320-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	34	37	44	rVB	29949	40178	1.46%	0.169%
2	3.690	108	111	126	rBV	69011	130009	4.74%	0.546%
3	4.019	164	167	172	rBV2	10426	11795	0.43%	0.050%
4	6.878	650	653	657	rVB5	4450	6426	0.23%	0.027%
5	7.042	674	681	690	rBV2	60525	137405	5.01%	0.577%
6	7.201	702	708	726	rBV	360604	617296	22.49%	2.594%
7	7.407	737	743	756	rBV	336544	578841	21.09%	2.433%
8	7.878	817	823	833	rBV	326305	555114	20.23%	2.333%
9	7.954	834	836	844	rVB6	5370	9018	0.33%	0.038%
10	8.119	860	864	867	rVB6	2827	3601	0.13%	0.015%
11	8.589	937	944	961	rBV	211148	413303	15.06%	1.737%
12	9.042	1013	1021	1035	rBV	432546	772459	28.15%	3.246%
13	9.213	1048	1050	1056	rVB6	4656	7831	0.29%	0.033%
14	9.483	1092	1096	1099	rBV5	4217	5887	0.21%	0.025%
15	9.766	1136	1144	1157	rBV	294243	547918	19.97%	2.303%
16	10.307	1229	1236	1252	rBV	395250	761881	27.76%	3.202%
17	10.689	1293	1301	1312	rBV	442751	754135	27.48%	3.169%
18	10.825	1317	1324	1337	rBV	270218	623342	22.71%	2.620%
19	11.989	1519	1522	1525	rBV3	3251	3210	0.12%	0.013%
20	12.313	1572	1577	1581	rBV6	5057	7962	0.29%	0.033%
21	13.507	1776	1780	1785	rBV4	1865	3360	0.12%	0.014%
22	13.936	1846	1853	1864	rBV	913640	1335252	48.66%	5.612%
23	14.218	1894	1901	1915	rBV	1065519	1576740	57.45%	6.627%
24	14.524	1943	1953	1963	rBV	621332	939762	34.24%	3.950%
25	14.618	1967	1969	1974	rVB4	2989	3736	0.14%	0.016%
26	14.771	1990	1995	1997	rBV5	4704	8270	0.30%	0.035%
27	15.330	2084	2090	2094	rBV7	3184	6520	0.24%	0.027%
28	15.518	2115	2122	2136	rBV	1315568	2002340	72.96%	8.415%
29	15.636	2136	2142	2156	rVV	281516	491907	17.92%	2.067%
30	15.759	2160	2163	2169	rVB5	12954	21629	0.79%	0.091%
31	16.301	2250	2255	2260	rBV5	7402	13667	0.50%	0.057%
32	17.059	2378	2384	2388	rBV4	3052	4973	0.18%	0.021%
33	17.265	2413	2419	2430	rBV	706183	1005329	36.63%	4.225%
34	17.365	2430	2436	2458	rVV	1527948	2306803	84.06%	9.695%
35	17.895	2523	2526	2530	rVV6	3701	5579	0.20%	0.023%
36	17.942	2530	2534	2537	rVB6	5701	7047	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034566.D
 Acq On : 08 Apr 2022 17:56
 Operator : CG/JU
 Sample : N2320-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	18.106	2559	2562	2565	rBV4	3014	4403	0.16%	0.019%
38	18.189	2571	2576	2582	rBV10	4077	9794	0.36%	0.041%
39	19.224	2748	2752	2759	rBV4	16495	26643	0.97%	0.112%
40	19.295	2760	2764	2768	rBV	13215	22003	0.80%	0.092%
41	19.659	2820	2826	2833	rBV	1951632	2721144	99.16%	11.436%
42	20.659	2991	2996	3000	rBV	348951	394911	14.39%	1.660%
43	21.447	3125	3130	3145	rBV	512830	1054494	38.42%	4.432%
44	23.671	3501	3508	3527	rBV2	1159311	2744323	100.00%	11.534%
45	23.824	3529	3534	3545	rVB2	485262	1096001	39.94%	4.606%


Sum of corrected areas: 23794241

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034566.D
Acq On : 08 Apr 2022 17:56
Operator : CG/JU
Sample : N2320-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

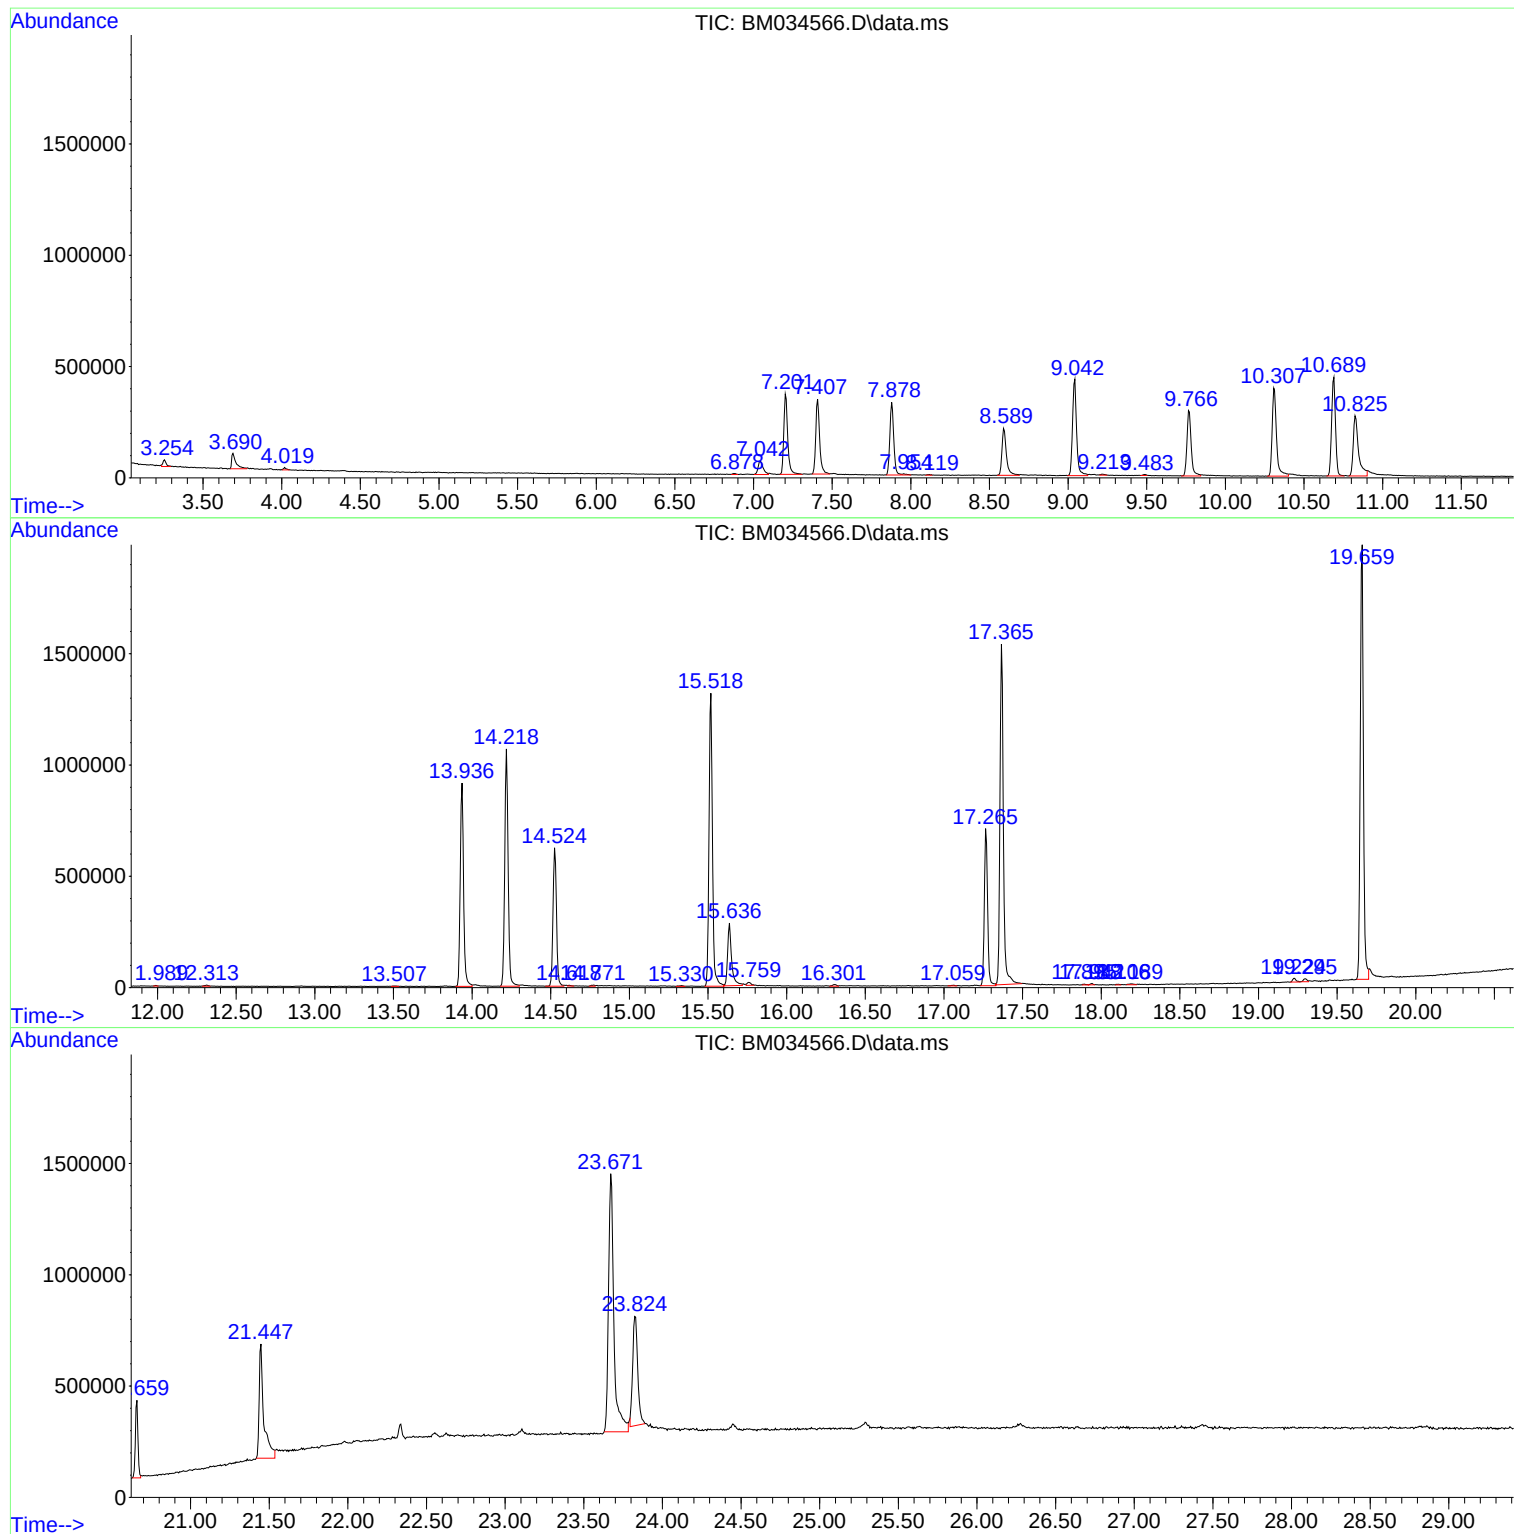

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034566.D
Acq On : 08 Apr 2022 17:56
Operator : CG/JU
Sample : N2320-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.659	7.49 ng/ul	394911	Chrysene-d12	21.447

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Diisooctyl adipate	370	C22H42O4	001330-86-5	91
3			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
5			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	83

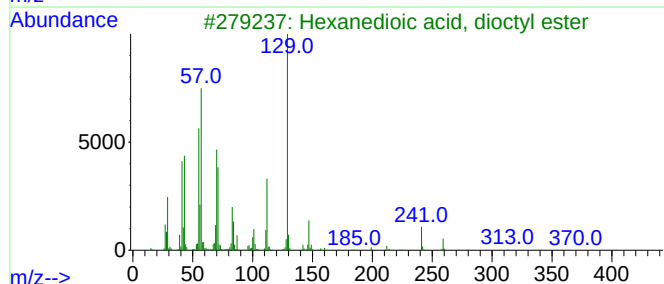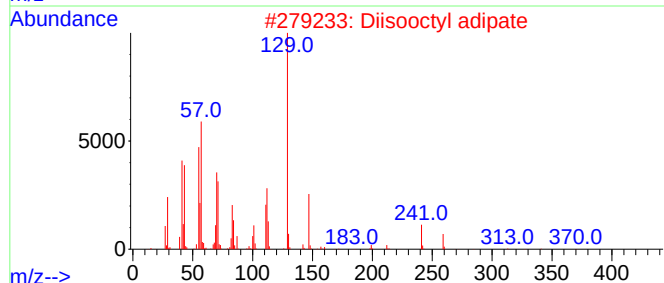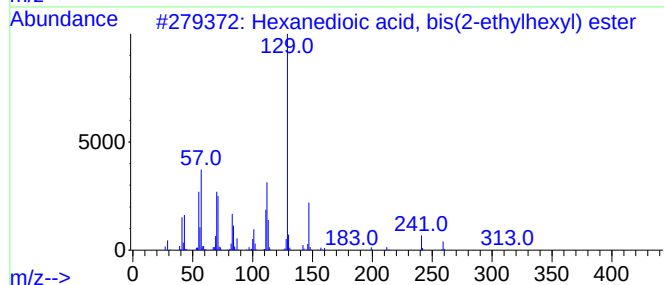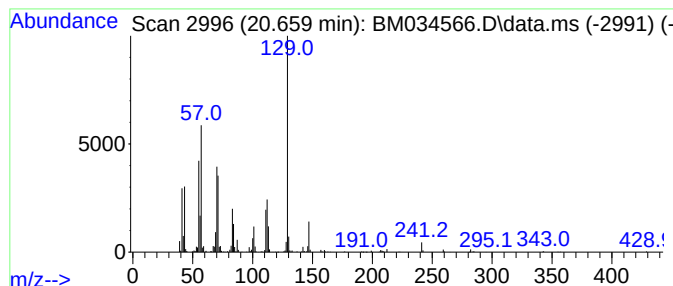

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034566.D
Acq On : 08 Apr 2022 17:56
Operator : CG/JU
Sample : N2320-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.659	7.5	ng/u1	394911	5	21.447	1054490	20.0