

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034572.D
 Acq On : 08 Apr 2022 22:11
 Operator : CG/JU
 Sample : PB143966BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK966

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	34	37	44	rVB	45758	58771	1.96%	0.200%
2	3.678	105	109	128	rBV	480351	743177	24.78%	2.529%
3	7.036	674	680	700	rBV	493339	857531	28.59%	2.918%
4	7.201	702	708	722	rVV	437130	711173	23.71%	2.420%
5	7.407	736	743	757	rBV	538280	924476	30.82%	3.146%
6	7.878	817	823	835	rBV	373949	614271	20.48%	2.090%
7	8.589	937	944	964	rBV	598129	1076529	35.89%	3.664%
8	9.042	1013	1021	1037	rBV	502676	905095	30.18%	3.080%
9	9.766	1136	1144	1162	rBV	411001	729878	24.34%	2.484%
10	10.307	1229	1236	1253	rBV	533234	1002931	33.44%	3.413%
11	10.689	1294	1301	1317	rBV	491757	853439	28.46%	2.904%
12	10.824	1317	1324	1352	rBV	427996	987412	32.92%	3.360%
13	12.307	1572	1576	1584	rBV6	5819	13332	0.44%	0.045%
14	13.824	1831	1834	1839	rBV5	3108	3456	0.12%	0.012%
15	13.936	1846	1853	1865	rBV	1071686	1614328	53.83%	5.494%
16	14.018	1865	1867	1873	rVB5	5646	8642	0.29%	0.029%
17	14.218	1894	1901	1916	rBV	1222349	1816670	60.57%	6.182%
18	14.318	1916	1918	1922	rVB3	3705	4809	0.16%	0.016%
19	14.524	1946	1953	1963	rBV	738871	1056632	35.23%	3.596%
20	14.724	1981	1987	2001	rBV	146348	399846	13.33%	1.361%
21	14.948	2023	2025	2031	rVB7	5137	6966	0.23%	0.024%
22	15.330	2088	2090	2094	rBV5	3657	4021	0.13%	0.014%
23	15.512	2115	2121	2136	rBV	1492903	2282385	76.10%	7.767%
24	15.636	2136	2142	2156	rVV	476350	793229	26.45%	2.699%
25	15.759	2158	2163	2168	rVB3	16658	27435	0.91%	0.093%
26	16.301	2252	2255	2261	rVB5	4733	7022	0.23%	0.024%
27	17.053	2380	2383	2387	rBV6	2130	3020	0.10%	0.010%
28	17.265	2413	2419	2428	rBV	812894	1177957	39.28%	4.009%
29	17.365	2430	2436	2461	rVB	1656384	2516656	83.91%	8.565%
30	18.706	2662	2664	2668	rBV6	2001	3075	0.10%	0.010%
31	19.230	2749	2753	2757	rBV3	19030	22366	0.75%	0.076%
32	19.300	2761	2765	2769	rBV	15249	20798	0.69%	0.071%
33	19.659	2819	2826	2842	rBV	2036265	2999173	100.00%	10.207%
34	21.447	3125	3130	3134	rBV	556797	906691	30.23%	3.086%
35	23.671	3501	3508	3527	rBV	1259492	2903989	96.83%	9.883%
36	23.824	3528	3534	3547	rVB	585393	1327515	44.26%	4.518%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034572.D
Acq On : 08 Apr 2022 22:11
Operator : CG/JU
Sample : PB143966BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK966

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION




Sum of corrected areas: 29384696

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034572.D
Acq On : 08 Apr 2022 22:11
Operator : CG/JU
Sample : PB143966BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK966

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

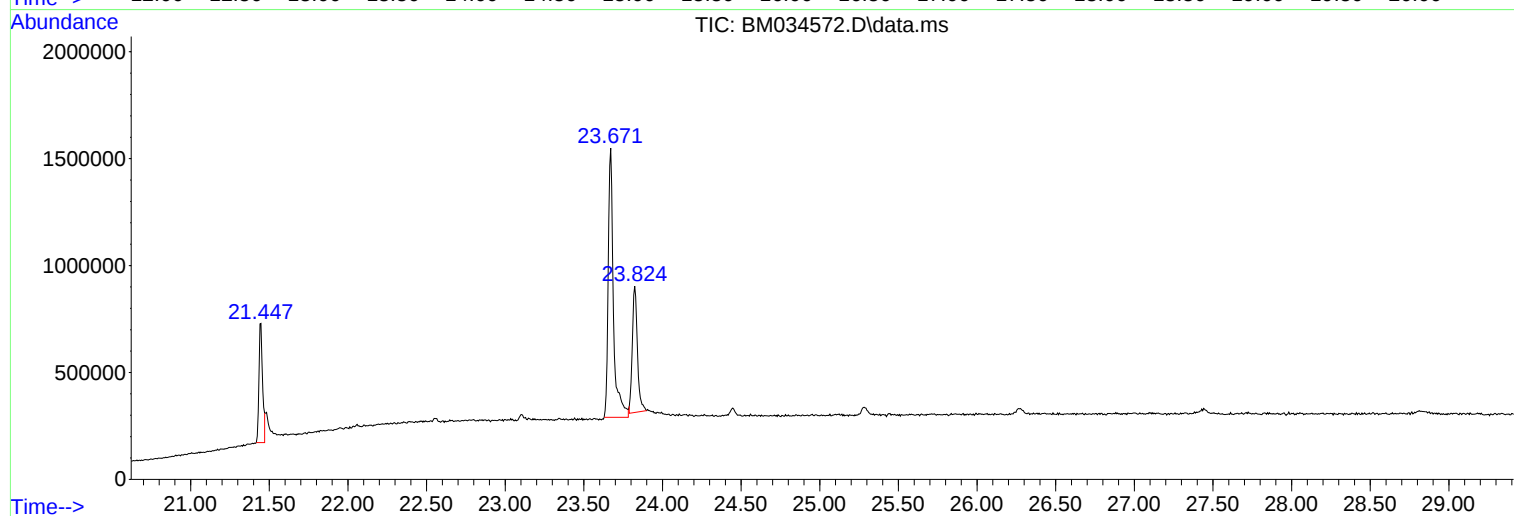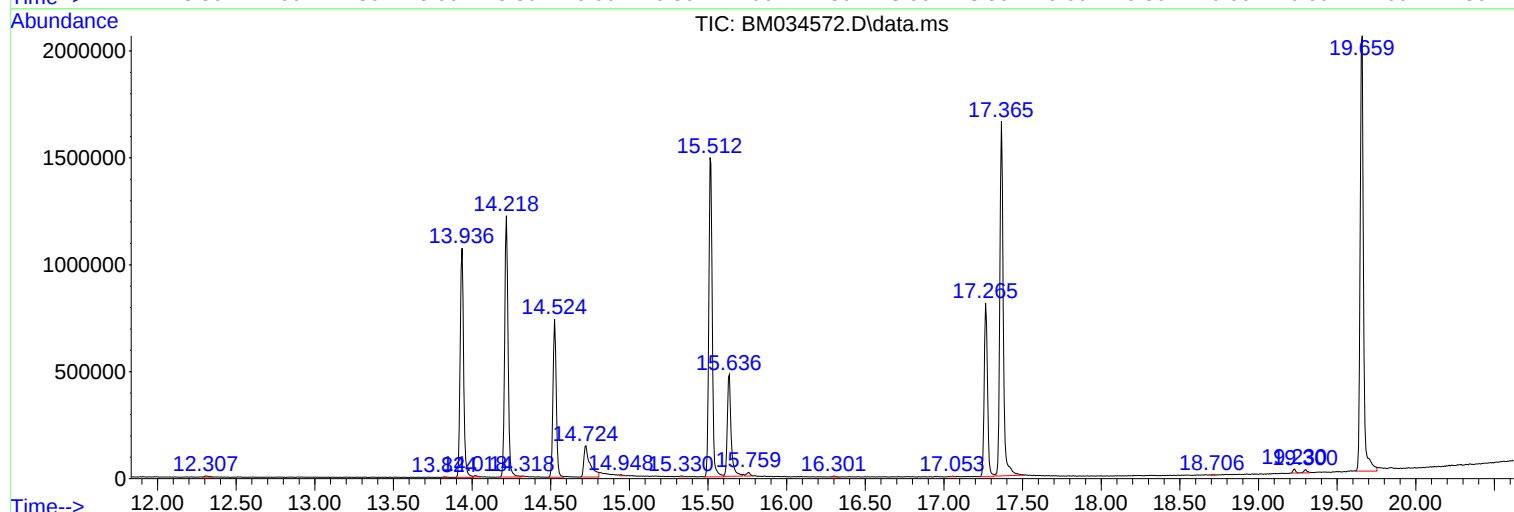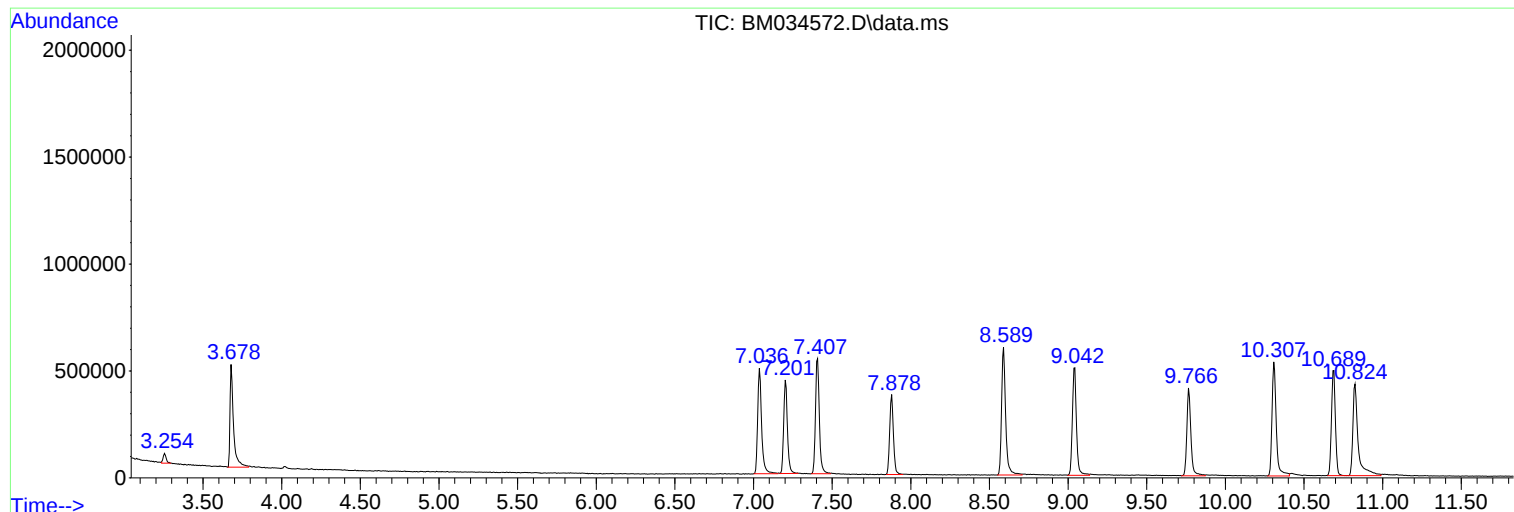

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034572.D
Acq On : 08 Apr 2022 22:11
Operator : CG/JU
Sample : PB143966BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK966

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034572.D
Acq On : 08 Apr 2022 22:11
Operator : CG/JU
Sample : PB143966BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK966

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------