

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034577.D
 Acq On : 09 Apr 2022 01:13
 Operator : CG/JU
 Sample : N2319-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	28	32	35	rBV	86011	116325	3.21%	0.368%
2	3.684	107	110	133	rVB	128433	229615	6.34%	0.727%
3	4.019	165	167	171	rVB2	11071	11522	0.32%	0.036%
4	4.560	254	259	266	rVB	42166	61172	1.69%	0.194%
5	5.907	486	488	493	rVB5	5089	6731	0.19%	0.021%
6	6.878	648	653	658	rVB3	9086	15604	0.43%	0.049%
7	7.042	675	681	690	rBV	80817	162936	4.50%	0.516%
8	7.201	702	708	718	rBV	485339	794716	21.94%	2.517%
9	7.407	736	743	756	rBV	441356	767707	21.20%	2.432%
10	7.878	816	823	832	rBV	407651	668863	18.47%	2.118%
11	7.948	833	835	840	rVB5	5381	8088	0.22%	0.026%
12	8.119	861	864	873	rVB9	5004	9385	0.26%	0.030%
13	8.589	938	944	956	rBV	282170	509781	14.08%	1.615%
14	9.036	1013	1020	1040	rBV	554833	1000813	27.63%	3.170%
15	9.483	1092	1096	1102	rVB2	14298	23687	0.65%	0.075%
16	9.766	1136	1144	1159	rBV	424400	769920	21.26%	2.439%
17	10.307	1227	1236	1253	rBV	558343	1022688	28.24%	3.239%
18	10.683	1293	1300	1313	rVB	536610	933875	25.78%	2.958%
19	10.825	1317	1324	1348	rBV	389058	905333	25.00%	2.867%
20	11.736	1473	1479	1482	rBV6	1673	3975	0.11%	0.013%
21	12.130	1540	1546	1551	rBV6	6083	9654	0.27%	0.031%
22	12.295	1570	1574	1579	rBV5	5153	10503	0.29%	0.033%
23	13.024	1691	1698	1701	rBV7	2657	4589	0.13%	0.015%
24	13.077	1704	1707	1712	rVV4	2808	3816	0.11%	0.012%
25	13.142	1714	1718	1722	rVB5	3430	4651	0.13%	0.015%
26	13.360	1751	1755	1760	rBV2	14393	21605	0.60%	0.068%
27	13.501	1774	1779	1782	rBV5	4095	6366	0.18%	0.020%
28	13.936	1846	1853	1863	rBV	1167802	1745271	48.19%	5.528%
29	14.013	1865	1866	1871	rVV3	9728	13363	0.37%	0.042%
30	14.054	1871	1873	1879	rVB6	3765	5952	0.16%	0.019%
31	14.218	1893	1901	1913	rBV	1353909	2025654	55.93%	6.416%
32	14.389	1924	1930	1934	rBV	32823	49980	1.38%	0.158%
33	14.430	1934	1937	1943	rVB3	13981	21100	0.58%	0.067%
34	14.524	1945	1953	1964	rBV	792900	1172603	32.38%	3.714%
35	14.760	1986	1993	1998	rBV8	9640	23375	0.65%	0.074%
36	15.048	2040	2042	2046	rVV5	5368	7544	0.21%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034577.D
 Acq On : 09 Apr 2022 01:13
 Operator : CG/JU
 Sample : N2319-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	15.336	2084	2091	2095	rBV7	5970	11905	0.33%	0.038%
38	15.377	2095	2098	2102	rVB	24690	29078	0.80%	0.092%
39	15.512	2115	2121	2134	rBV	1715653	2637621	72.83%	8.354%
40	15.630	2136	2141	2157	rVB	531830	829728	22.91%	2.628%
41	15.760	2159	2163	2166	rBV2	18590	24519	0.68%	0.078%
42	15.877	2181	2183	2190	rVB7	4430	6720	0.19%	0.021%
43	15.936	2190	2193	2198	rVB6	4331	6864	0.19%	0.022%
44	16.001	2201	2204	2206	rBV4	5159	6020	0.17%	0.019%
45	16.242	2240	2245	2248	rBV	44188	66500	1.84%	0.211%
46	16.301	2252	2255	2259	rVV4	10183	15662	0.43%	0.050%
47	16.342	2259	2262	2269	rVB6	15977	26348	0.73%	0.083%
48	16.589	2301	2304	2305	rBV2	5335	4879	0.13%	0.015%
49	16.701	2319	2323	2325	rBV5	3797	6260	0.17%	0.020%
50	16.818	2337	2343	2346	rBV6	10034	17772	0.49%	0.056%
51	16.848	2346	2348	2350	rVV3	4113	4094	0.11%	0.013%
52	16.948	2363	2365	2370	rVB6	6714	7705	0.21%	0.024%
53	17.036	2376	2380	2384	rBV	47461	69250	1.91%	0.219%
54	17.083	2386	2388	2392	rVB2	17239	20607	0.57%	0.065%
55	17.265	2413	2419	2429	rBV	898966	1310175	36.17%	4.150%
56	17.365	2430	2436	2451	rVV	2001393	2926635	80.81%	9.270%
57	17.771	2502	2505	2510	rVB	46843	57855	1.60%	0.183%
58	18.165	2568	2572	2574	rBV3	49318	68004	1.88%	0.215%
59	18.465	2619	2623	2628	rBV	36379	46279	1.28%	0.147%
60	19.095	2727	2730	2736	rVB3	23989	28507	0.79%	0.090%
61	19.224	2748	2752	2760	rBV5	28862	51968	1.43%	0.165%
62	19.295	2761	2764	2769	rVV	19594	26845	0.74%	0.085%
63	19.442	2787	2789	2794	rBV6	11830	17246	0.48%	0.055%
64	19.653	2819	2825	2832	rBV	2582007	3621795	100.00%	11.471%
65	19.895	2864	2866	2870	rVB3	16584	13977	0.39%	0.044%
66	21.153	3077	3080	3089	rBV	118445	167215	4.62%	0.530%
67	21.441	3124	3129	3146	rBV	741135	1428766	39.45%	4.525%
68	23.665	3501	3507	3526	rBV2	1505675	3410953	94.18%	10.804%
69	23.824	3528	3534	3546	rVB2	664512	1456098	40.20%	4.612%




Sum of corrected areas: 31572612

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034577.D
Acq On : 09 Apr 2022 01:13
Operator : CG/JU
Sample : N2319-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

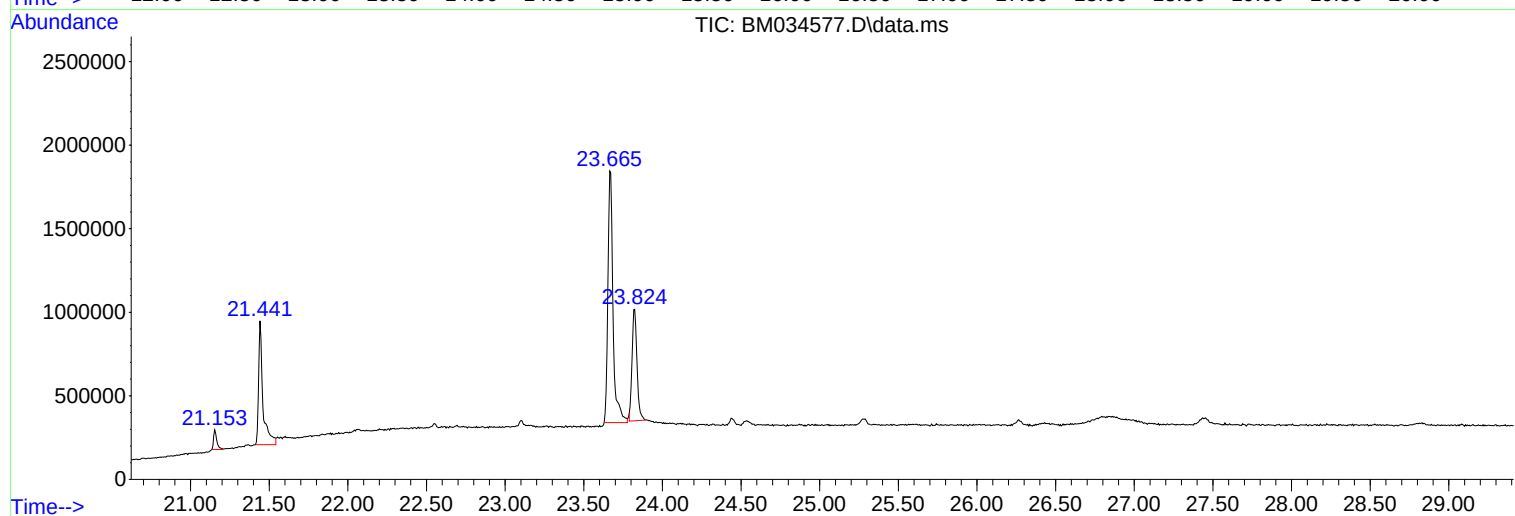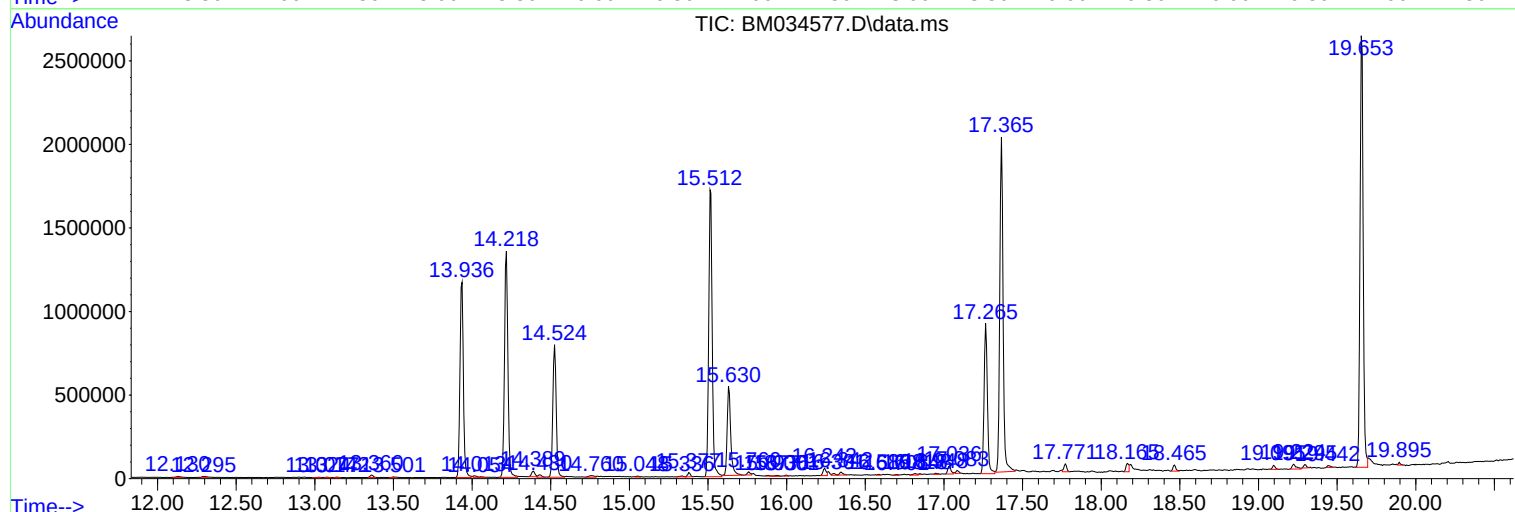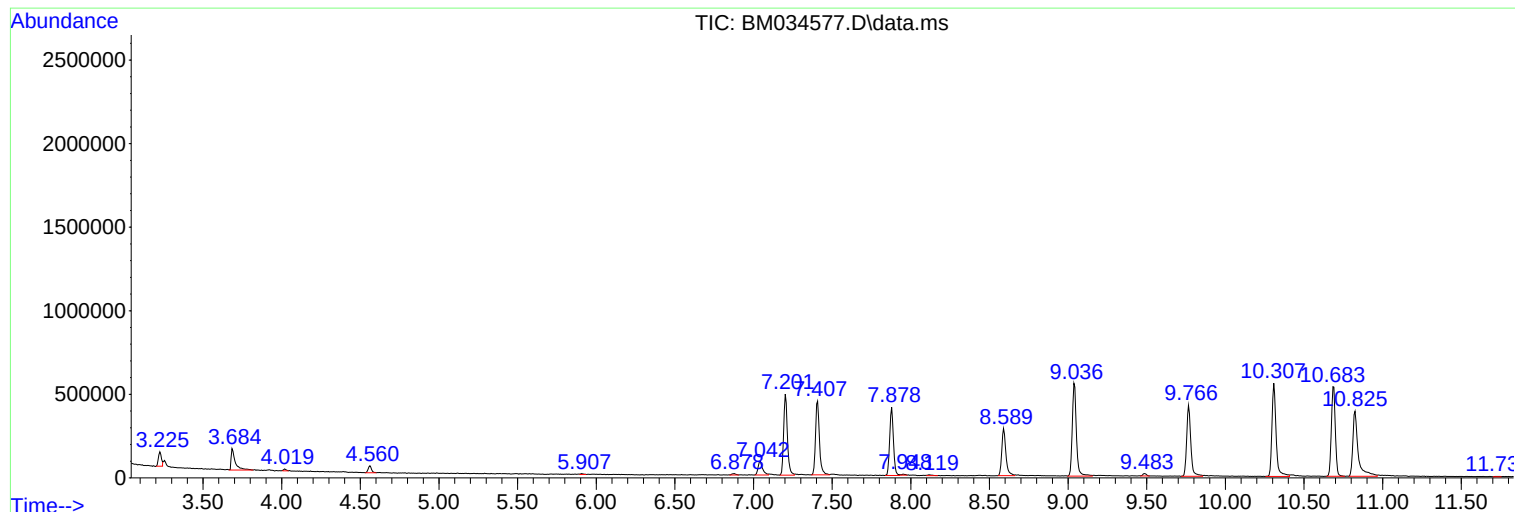

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034577.D
Acq On : 09 Apr 2022 01:13
Operator : CG/JU
Sample : N2319-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.153	2.34 ng/ul	167215	Chrysene-d12	21.442

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	94
2	1-Heneicosanol			312	C21H44O	015594-90-8	94
3	Heptadecafluorononanoic acid, tr...			646	C22H27F17O2	1000356-02-9	94
4	Heptafluorobutyric acid, pentade...			424	C19H31F7O2	959261-23-5	93
5	1-Heneicosyl formate			340	C22H44O2	077899-03-7	91

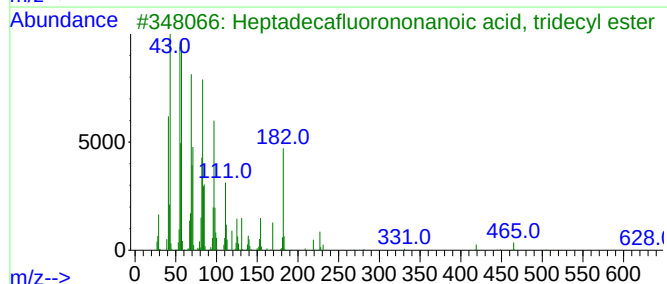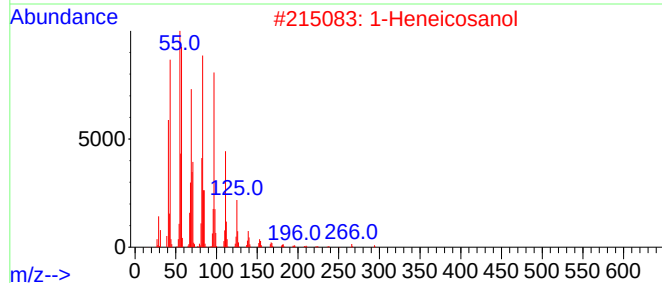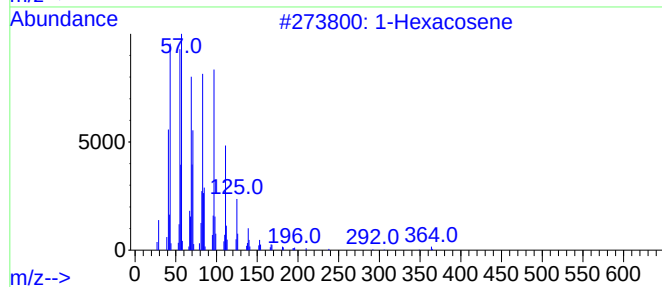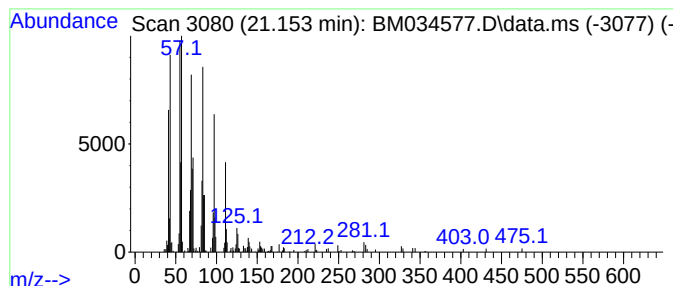

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034577.D
Acq On : 09 Apr 2022 01:13
Operator : CG/JU
Sample : N2319-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.153	2.3	ng/u1	167215	5	21.442	1428770	20.0