

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034578.D
 Acq On : 09 Apr 2022 01:49
 Operator : CG/JU
 Sample : N2319-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	29	32	34	rBV3	23996	30090	0.89%	0.097%
2	3.255	35	37	43	rVB	37990	44978	1.33%	0.146%
3	3.684	107	110	122	rBV	115754	191269	5.66%	0.619%
4	4.560	255	259	266	rVB	25383	38681	1.14%	0.125%
5	5.901	485	487	495	rVB6	4998	9691	0.29%	0.031%
6	6.878	648	653	658	rBV3	10477	16665	0.49%	0.054%
7	7.043	675	681	690	rBV	103280	205499	6.08%	0.665%
8	7.201	702	708	721	rBV	498635	807544	23.88%	2.614%
9	7.407	737	743	756	rBV	476273	816323	24.14%	2.642%
10	7.878	817	823	832	rBV	416337	685503	20.27%	2.219%
11	7.954	833	836	842	rVB6	6590	9653	0.29%	0.031%
12	8.113	860	863	869	rVB7	4930	6831	0.20%	0.022%
13	8.425	912	916	921	rBV7	4120	6754	0.20%	0.022%
14	8.590	937	944	962	rBV	327411	590004	17.45%	1.910%
15	9.037	1013	1020	1033	rBV	576936	1001717	29.63%	3.243%
16	9.178	1040	1044	1048	rVB6	3773	6342	0.19%	0.021%
17	9.484	1092	1096	1101	rVB2	11969	19146	0.57%	0.062%
18	9.766	1136	1144	1156	rBV	446653	782139	23.13%	2.532%
19	10.307	1228	1236	1252	rBV	584755	1058243	31.30%	3.425%
20	10.683	1293	1300	1310	rBV	567581	959510	28.38%	3.106%
21	10.825	1316	1324	1346	rBV	448413	999746	29.57%	3.236%
22	12.136	1542	1547	1551	rVB4	4846	7665	0.23%	0.025%
23	12.295	1569	1574	1576	rBV4	5750	9704	0.29%	0.031%
24	13.077	1703	1707	1711	rBV4	2786	3560	0.11%	0.012%
25	13.142	1714	1718	1722	rVV4	3723	4392	0.13%	0.014%
26	13.360	1748	1755	1762	rVB3	10990	19213	0.57%	0.062%
27	13.936	1847	1853	1864	rBV	1218690	1807753	53.47%	5.852%
28	14.019	1864	1867	1873	rVB4	6957	11757	0.35%	0.038%
29	14.219	1892	1901	1915	rBV	1383626	2074343	61.35%	6.715%
30	14.319	1916	1918	1923	rVB5	3995	6550	0.19%	0.021%
31	14.524	1947	1953	1966	rBV	783698	1162117	34.37%	3.762%
32	14.754	1985	1992	1999	rBV8	11936	37300	1.10%	0.121%
33	15.330	2086	2090	2097	rBV4	7118	13862	0.41%	0.045%
34	15.518	2115	2122	2136	rBV	1749254	2687550	79.49%	8.699%
35	15.636	2136	2142	2159	rVV	522161	889208	26.30%	2.878%
36	15.760	2159	2163	2177	rVB2	22565	46641	1.38%	0.151%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034578.D
 Acq On : 09 Apr 2022 01:49
 Operator : CG/JU
 Sample : N2319-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	16.077	2214	2217	2223	rVB7	2337	4247	0.13%	0.014%
38	16.301	2251	2255	2261	rVB7	5405	10141	0.30%	0.033%
39	16.418	2266	2275	2276	rBV7	2044	4262	0.13%	0.014%
40	16.777	2331	2336	2341	rBV7	1758	3545	0.10%	0.011%
41	17.030	2374	2379	2381	rBV6	2915	4522	0.13%	0.015%
42	17.054	2381	2383	2387	rVV4	2394	3750	0.11%	0.012%
43	17.265	2413	2419	2427	rBV	868236	1251201	37.01%	4.050%
44	17.365	2430	2436	2455	rVV	1914743	2907538	85.99%	9.412%
45	17.948	2528	2535	2540	rBV3	17964	28081	0.83%	0.091%
46	18.165	2568	2572	2582	rBV6	21367	47939	1.42%	0.155%
47	18.236	2582	2584	2588	rVV5	4466	6330	0.19%	0.020%
48	18.459	2620	2622	2626	rBV5	2580	3917	0.12%	0.013%
49	18.595	2642	2645	2649	rBV5	11046	11530	0.34%	0.037%
50	19.224	2748	2752	2759	rVB2	23877	32194	0.95%	0.104%
51	19.295	2760	2764	2769	rBV2	16349	28818	0.85%	0.093%
52	19.448	2788	2790	2797	rBV8	5881	10435	0.31%	0.034%
53	19.653	2819	2825	2832	rBV	2400526	3381074	100.00%	10.944%
54	21.153	3077	3080	3088	rBV4	71928	112959	3.34%	0.366%
55	21.442	3124	3129	3143	rBV	679913	1278752	37.82%	4.139%
56	23.671	3500	3508	3524	rBV2	1366508	3303359	97.70%	10.693%
57	23.818	3528	3533	3549	rVB2	623298	1390703	41.13%	4.502%




Sum of corrected areas: 30893240

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034578.D
Acq On : 09 Apr 2022 01:49
Operator : CG/JU
Sample : N2319-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

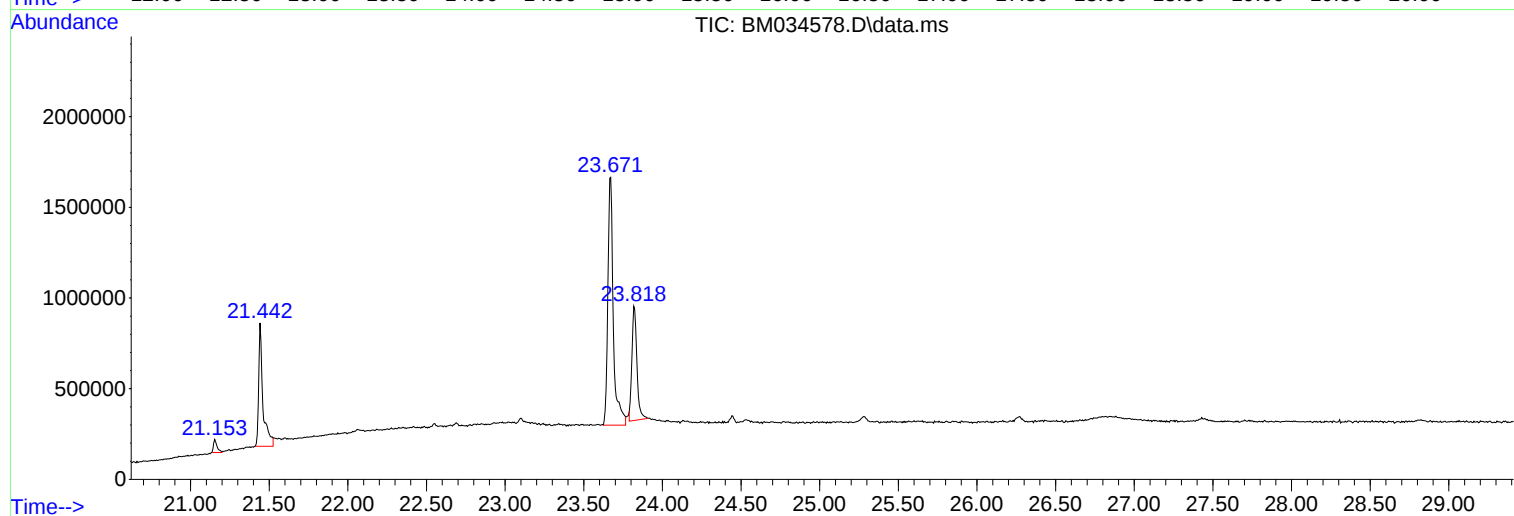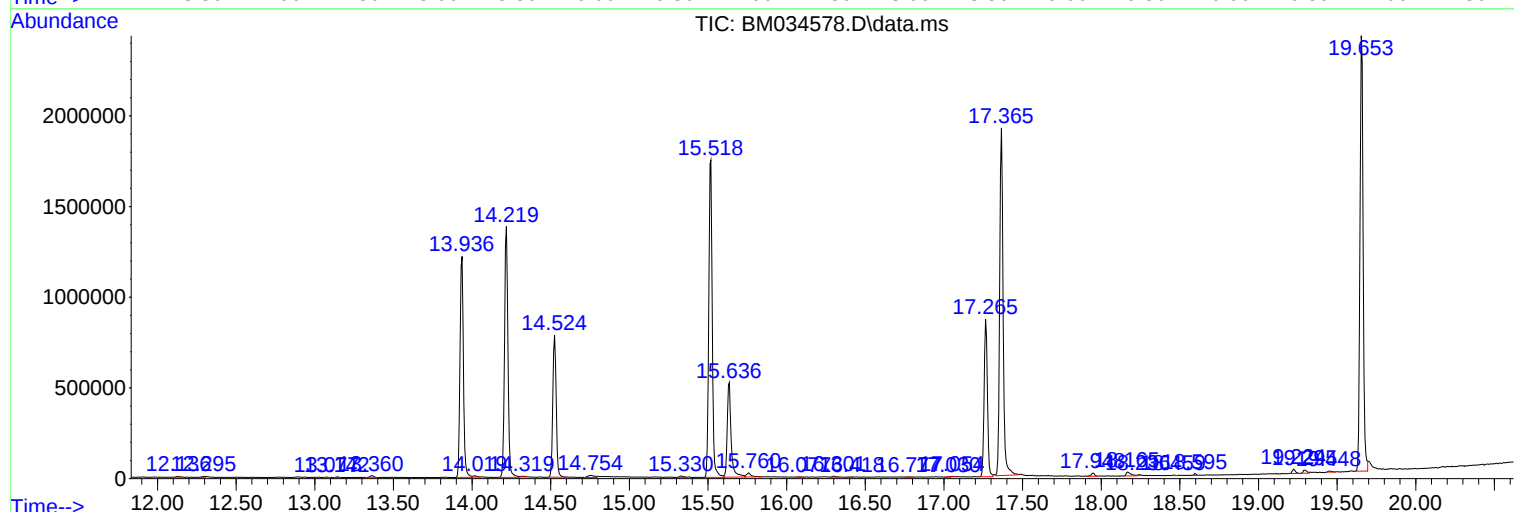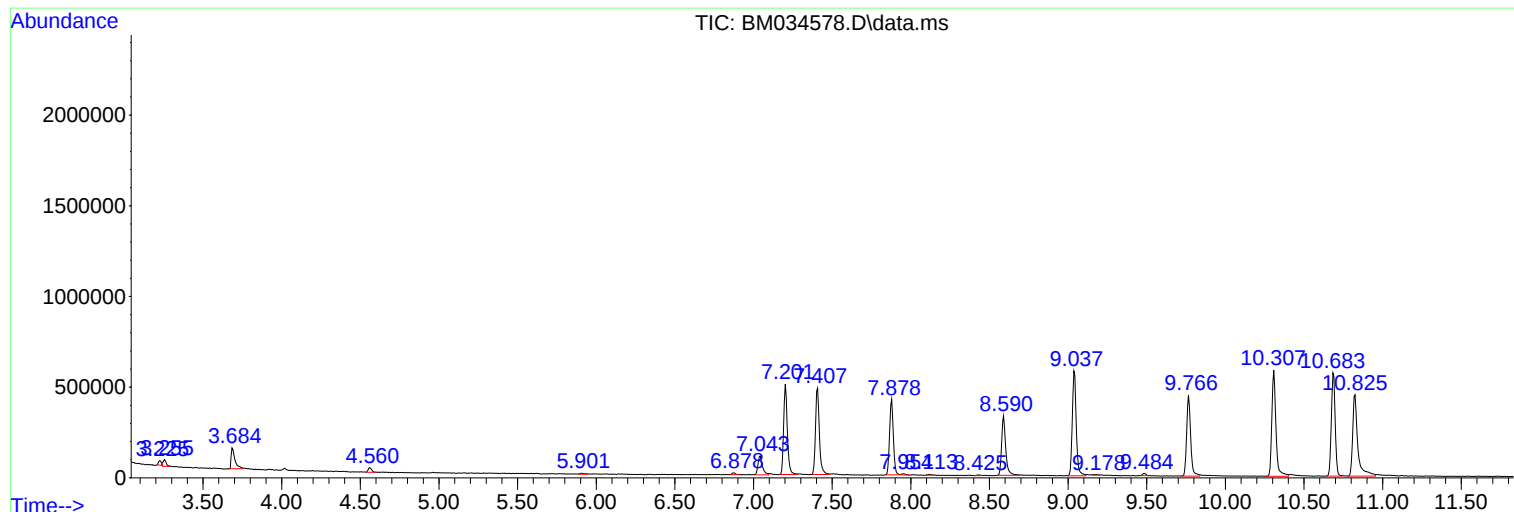

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034578.D
Acq On : 09 Apr 2022 01:49
Operator : CG/JU
Sample : N2319-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034578.D
Acq On : 09 Apr 2022 01:49
Operator : CG/JU
Sample : N2319-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------