

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034581.D
 Acq On : 09 Apr 2022 03:38
 Operator : CG/JU
 Sample : N2319-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.255	34	37	42	rVB	35119	43945	1.27%	0.138%
2	3.684	108	110	126	rBV	96407	167813	4.86%	0.526%
3	4.019	164	167	173	rVB2	13465	18282	0.53%	0.057%
4	4.560	254	259	266	rBV2	45911	67378	1.95%	0.211%
5	6.872	649	652	659	rVB4	8344	12047	0.35%	0.038%
6	7.037	675	680	696	rVB	87396	177419	5.13%	0.557%
7	7.201	702	708	722	rBV	503130	825706	23.89%	2.590%
8	7.401	736	742	757	rBV	452110	791068	22.89%	2.481%
9	7.878	816	823	832	rBV	508728	849421	24.58%	2.665%
10	7.948	834	835	844	rVB9	8227	11034	0.32%	0.035%
11	8.590	937	944	962	rBV	298804	557058	16.12%	1.747%
12	9.037	1012	1020	1032	rBV	576700	1011361	29.26%	3.173%
13	9.213	1045	1050	1059	rVB9	10387	19507	0.56%	0.061%
14	9.484	1092	1096	1101	rVB	14338	20799	0.60%	0.065%
15	9.766	1136	1144	1160	rBV	440080	798059	23.09%	2.503%
16	10.307	1229	1236	1251	rBV	568169	1037830	30.03%	3.256%
17	10.684	1293	1300	1315	rVB	694952	1184427	34.27%	3.715%
18	10.825	1315	1324	1348	rBV	380781	901465	26.08%	2.828%
19	11.983	1518	1521	1525	rVB5	3147	4535	0.13%	0.014%
20	12.136	1538	1547	1553	rBV7	5641	10701	0.31%	0.034%
21	12.295	1570	1574	1581	rVV5	6607	13979	0.40%	0.044%
22	12.807	1656	1661	1664	rVB6	2584	4229	0.12%	0.013%
23	13.030	1691	1699	1700	rBV6	2374	3884	0.11%	0.012%
24	13.360	1751	1755	1761	rBV3	10661	15808	0.46%	0.050%
25	13.501	1775	1779	1780	rBV4	3466	4056	0.12%	0.013%
26	13.936	1846	1853	1862	rBV	1166487	1754571	50.77%	5.504%
27	14.019	1865	1867	1873	rVV2	9162	14216	0.41%	0.045%
28	14.219	1894	1901	1914	rBV	1365397	2091027	60.50%	6.559%
29	14.389	1926	1930	1936	rBV2	13817	21229	0.61%	0.067%
30	14.524	1946	1953	1966	rBV	982611	1439167	41.64%	4.514%
31	14.748	1986	1991	1996	rBV7	8758	19833	0.57%	0.062%
32	14.889	2012	2015	2021	rVB7	2785	4622	0.13%	0.014%
33	15.513	2115	2121	2135	rBV	1747237	2637106	76.30%	8.272%
34	15.630	2135	2141	2157	rVV	500374	830848	24.04%	2.606%
35	15.760	2159	2163	2166	rVB2	14419	20956	0.61%	0.066%
36	16.077	2212	2217	2220	rBV6	2832	4100	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034581.D
 Acq On : 09 Apr 2022 03:38
 Operator : CG/JU
 Sample : N2319-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	16.307	2252	2256	2258	rVB5	4331	6035	0.17%	0.019%
38	16.642	2311	2313	2317	rVB5	2886	3627	0.10%	0.011%
39	16.948	2362	2365	2368	rVV5	4010	4905	0.14%	0.015%
40	17.048	2375	2382	2383	rBV7	5677	8935	0.26%	0.028%
41	17.083	2386	2388	2393	rVB5	3594	5122	0.15%	0.016%
42	17.265	2413	2419	2428	rBV	1089323	1557274	45.06%	4.885%
43	17.365	2430	2436	2456	rVB	1933112	2882753	83.41%	9.043%
44	17.842	2514	2517	2522	rBV6	3390	5447	0.16%	0.017%
45	17.942	2532	2534	2537	rVB4	3114	3677	0.11%	0.012%
46	18.107	2560	2562	2566	rVB4	2782	3888	0.11%	0.012%
47	18.171	2569	2573	2574	rBV3	22322	30434	0.88%	0.095%
48	18.189	2574	2576	2582	rVB3	23377	30404	0.88%	0.095%
49	18.595	2642	2645	2650	rVB4	13045	14446	0.42%	0.045%
50	19.224	2748	2752	2756	rBV3	24304	37419	1.08%	0.117%
51	19.295	2760	2764	2768	rBV	20382	31733	0.92%	0.100%
52	19.448	2787	2790	2792	rBV3	8811	10351	0.30%	0.032%
53	19.589	2810	2814	2819	rVB8	9668	16184	0.47%	0.051%
54	19.654	2819	2825	2841	rBV	2418351	3456094	100.00%	10.841%
55	21.153	3077	3080	3087	rBV3	70293	108295	3.13%	0.340%
56	21.442	3124	3129	3145	rBV	862854	1612353	46.65%	5.058%
57	23.665	3500	3507	3524	rBV	1305100	3043168	88.05%	9.546%
58	23.818	3527	3533	3545	rVB2	739219	1616836	46.78%	5.072%




Sum of corrected areas: 31878866

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034581.D
Acq On : 09 Apr 2022 03:38
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

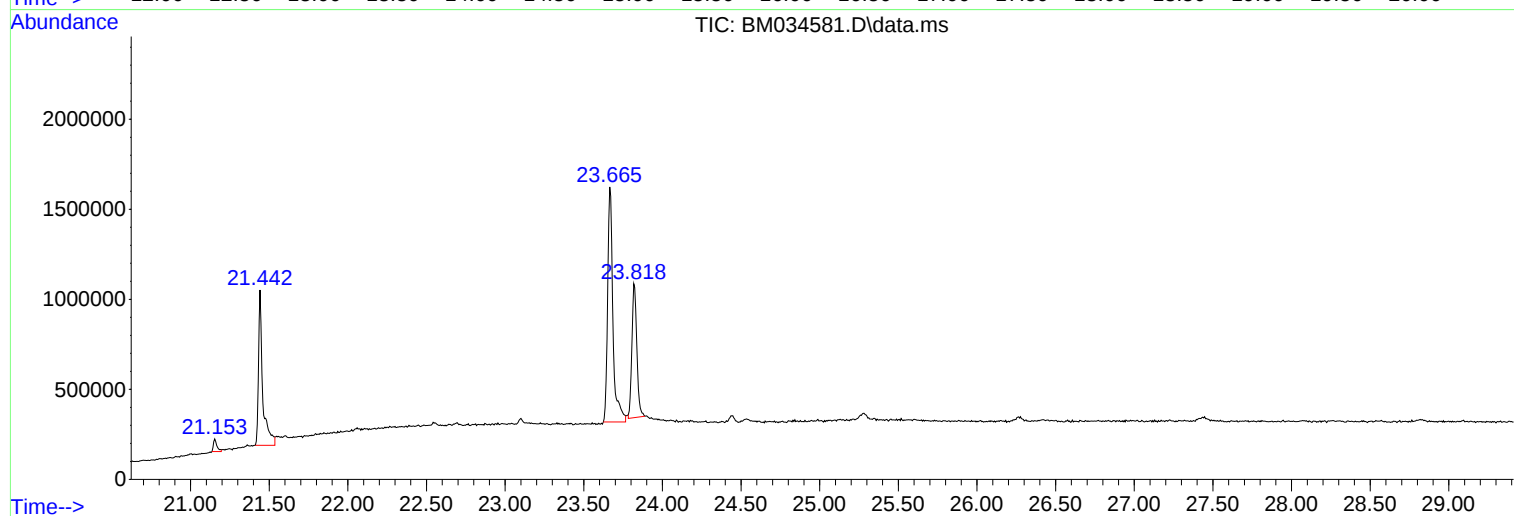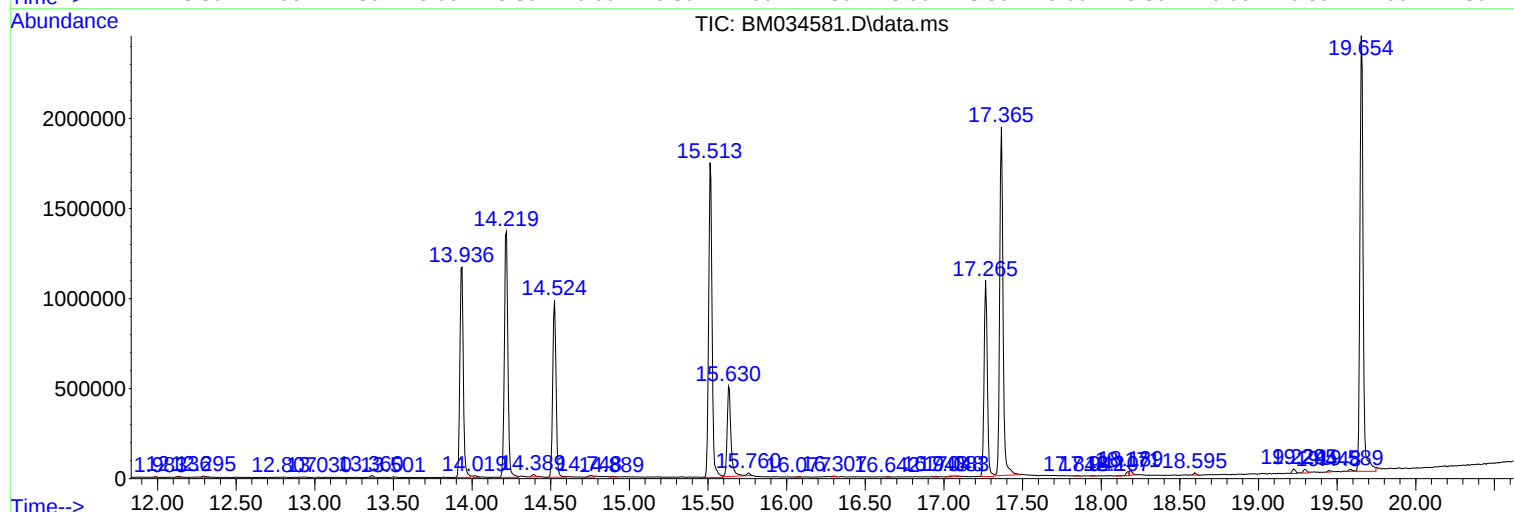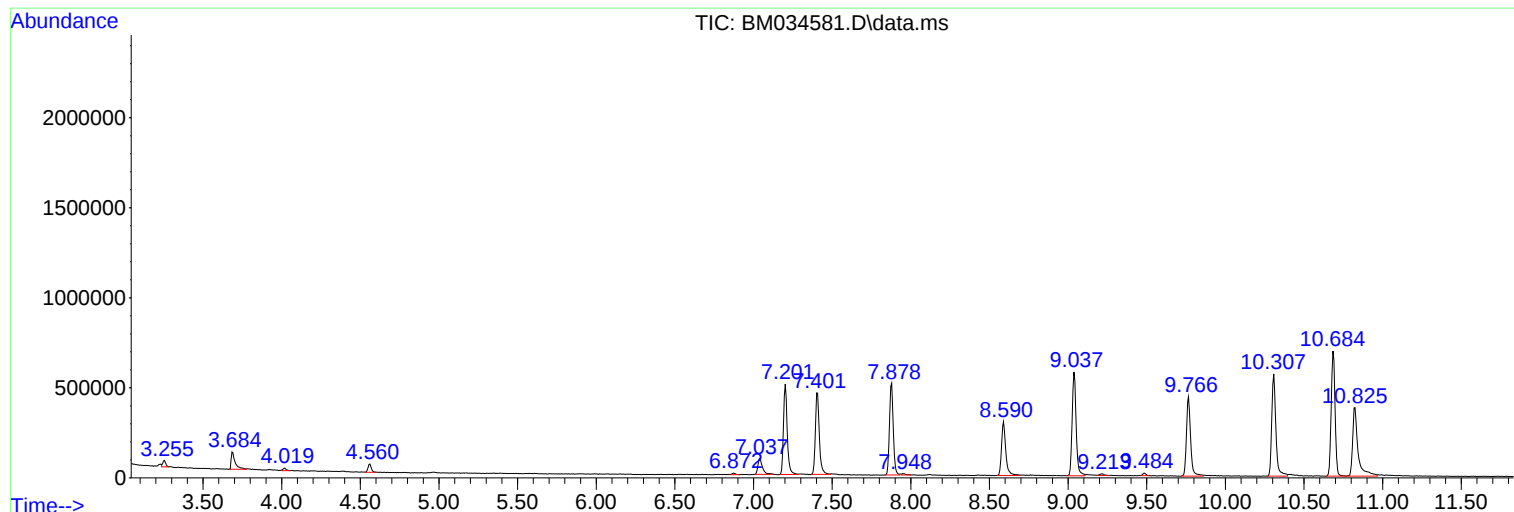

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034581.D
Acq On : 09 Apr 2022 03:38
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034581.D
Acq On : 09 Apr 2022 03:38
Operator : CG/JU
Sample : N2319-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
