

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034582.D
 Acq On : 09 Apr 2022 04:14
 Operator : CG/JU
 Sample : N2319-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	27	32	42	rVB2	209366	330269	10.07%	1.037%
2	3.684	107	110	120	rBV	118888	184823	5.64%	0.580%
3	4.019	164	167	171	rVB3	11418	14097	0.43%	0.044%
4	4.560	254	259	266	rVB	86500	130004	3.96%	0.408%
5	6.872	648	652	655	rBV3	7629	11803	0.36%	0.037%
6	7.037	675	680	690	rBV	95860	194801	5.94%	0.612%
7	7.201	702	708	720	rBV	535985	871854	26.59%	2.737%
8	7.401	736	742	757	rBV	497994	869225	26.50%	2.729%
9	7.878	816	823	832	rBV	478383	782749	23.87%	2.458%
10	7.948	832	835	842	rVB4	10937	19037	0.58%	0.060%
11	8.119	861	864	870	rVB7	4451	7642	0.23%	0.024%
12	8.590	934	944	958	rBV	322646	589816	17.99%	1.852%
13	9.037	1013	1020	1039	rBV	615514	1073573	32.74%	3.371%
14	9.219	1047	1051	1057	rVB8	6011	10251	0.31%	0.032%
15	9.484	1089	1096	1102	rVB3	9391	17357	0.53%	0.054%
16	9.766	1137	1144	1160	rBV	471152	836937	25.52%	2.628%
17	10.307	1229	1236	1253	rBV	594510	1085227	33.09%	3.407%
18	10.419	1253	1255	1268	rVB10	8699	21276	0.65%	0.067%
19	10.684	1293	1300	1316	rBV	615124	1058949	32.29%	3.325%
20	10.825	1316	1324	1346	rBV	419832	950980	29.00%	2.986%
21	11.025	1356	1358	1365	rVB6	4359	5888	0.18%	0.018%
22	12.136	1537	1547	1554	rBV8	4939	13597	0.41%	0.043%
23	12.295	1568	1574	1588	rVB4	6782	18952	0.58%	0.060%
24	12.801	1656	1660	1664	rVB6	3031	3649	0.11%	0.011%
25	13.360	1751	1755	1759	rBV3	7954	11217	0.34%	0.035%
26	13.819	1827	1833	1835	rBV5	2898	4653	0.14%	0.015%
27	13.930	1846	1852	1865	rBV	1230654	1807361	55.11%	5.674%
28	14.019	1865	1867	1874	rVB5	6326	9819	0.30%	0.031%
29	14.219	1893	1901	1914	rBV	1395432	2116762	64.55%	6.646%
30	14.389	1926	1930	1936	rBV6	16655	27809	0.85%	0.087%
31	14.524	1946	1953	1965	rBV	832966	1239649	37.80%	3.892%
32	14.754	1987	1992	1998	rBV6	8799	24169	0.74%	0.076%
33	15.330	2085	2090	2096	rBV5	4452	9265	0.28%	0.029%
34	15.513	2115	2121	2135	rBV	1792708	2666316	81.30%	8.371%
35	15.630	2136	2141	2158	rVV	510383	835372	25.47%	2.623%
36	15.760	2158	2163	2169	rVB	18860	33447	1.02%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034582.D
 Acq On : 09 Apr 2022 04:14
 Operator : CG/JU
 Sample : N2319-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	16.301	2251	2255	2259	rVB6	6081	8255	0.25%	0.026%
38	16.342	2259	2262	2263	rBV3	3440	3371	0.10%	0.011%
39	16.948	2362	2365	2369	rVB6	2930	4515	0.14%	0.014%
40	17.042	2377	2381	2382	rBV4	5976	7384	0.23%	0.023%
41	17.265	2413	2419	2430	rBV	932184	1325554	40.42%	4.162%
42	17.365	2430	2436	2452	rVV	1896421	2825051	86.14%	8.869%
43	17.642	2479	2483	2485	rBV4	3097	3965	0.12%	0.012%
44	17.842	2516	2517	2522	rVB5	3936	4877	0.15%	0.015%
45	18.165	2567	2572	2580	rBV4	60673	124753	3.80%	0.392%
46	18.242	2582	2585	2591	rVB7	7459	12965	0.40%	0.041%
47	18.589	2641	2644	2648	rBV6	4528	6880	0.21%	0.022%
48	19.230	2748	2753	2758	rBV2	22465	37717	1.15%	0.118%
49	19.295	2761	2764	2769	rVV2	17170	24797	0.76%	0.078%
50	19.448	2788	2790	2796	rVB7	9027	10122	0.31%	0.032%
51	19.654	2819	2825	2832	rBV	2396271	3279488	100.00%	10.296%
52	21.153	3076	3080	3091	rBV	226286	362836	11.06%	1.139%
53	21.442	3124	3129	3147	rBV	727231	1411360	43.04%	4.431%
54	23.665	3501	3507	3523	rBV2	1428505	3067618	93.54%	9.631%
55	23.818	3528	3533	3546	rVB2	677664	1441267	43.95%	4.525%




Sum of corrected areas: 31851370

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034582.D
Acq On : 09 Apr 2022 04:14
Operator : CG/JU
Sample : N2319-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

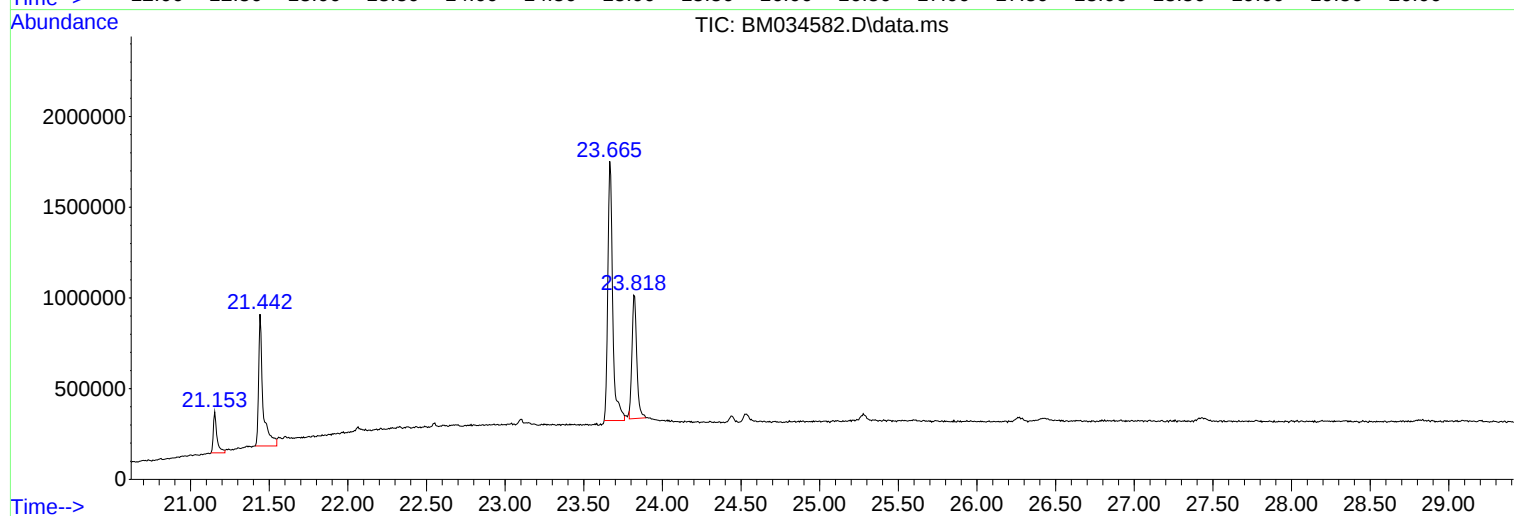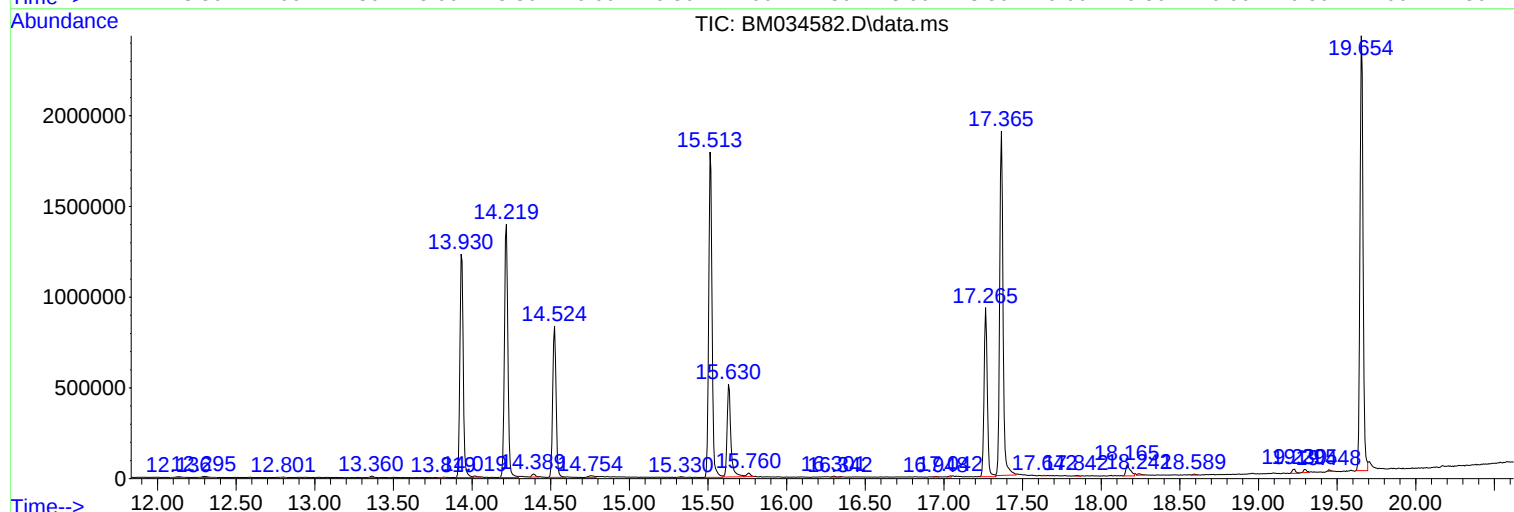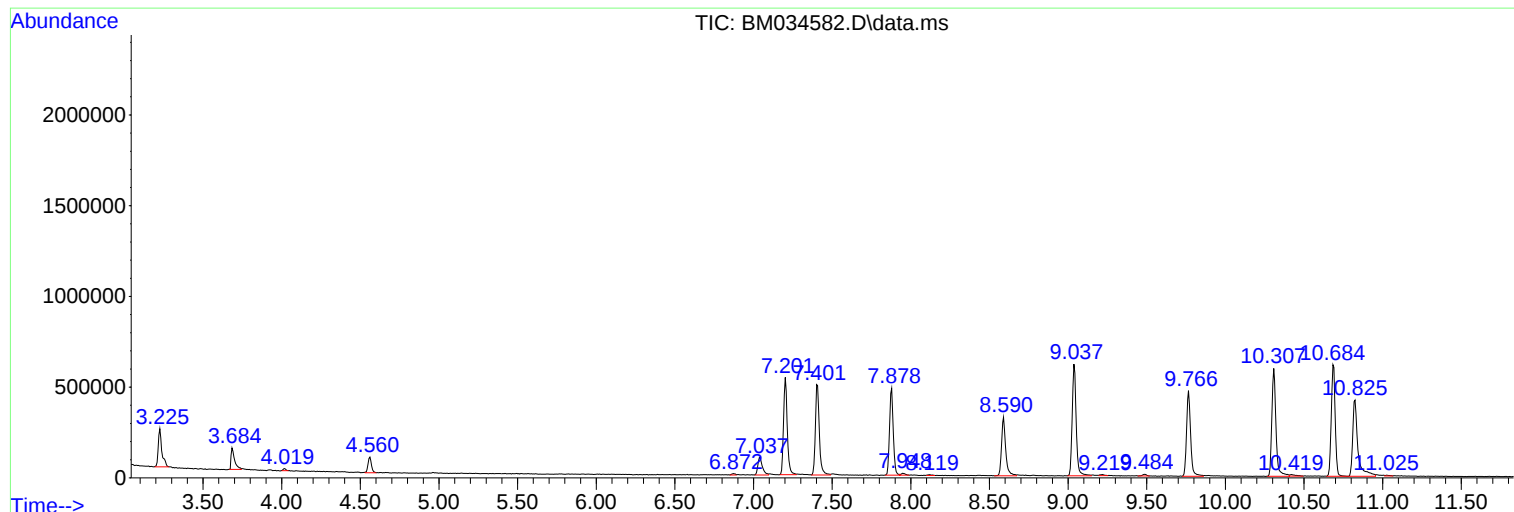

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034582.D
Acq On : 09 Apr 2022 04:14
Operator : CG/JU
Sample : N2319-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.154	5.14 ng/ul	362836	Chrysene-d12	21.442

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-			280	C20H40	074685-30-6	99
2	1-Octadecanol			270	C18H38O	000112-92-5	95
3	Bromoacetic acid, octadecyl ester			390	C20H39BrO2	018992-03-5	94
4	Trichloroacetic acid, hexadecyl ...			386	C18H33Cl3O2	074339-54-1	94
5	1-Nonadecene			266	C19H38	018435-45-5	94

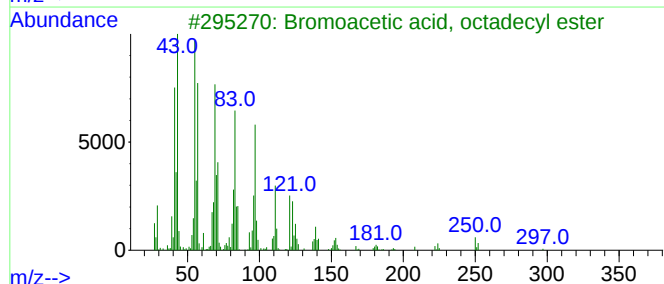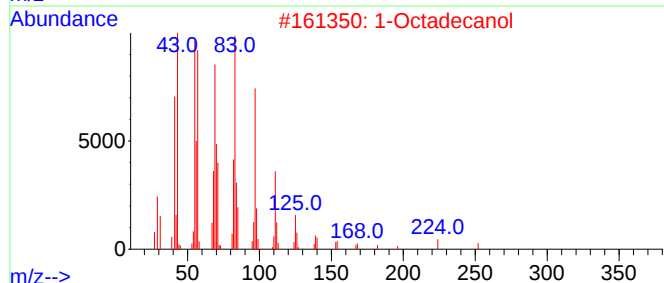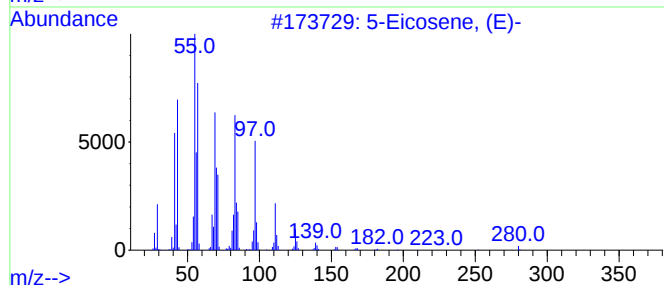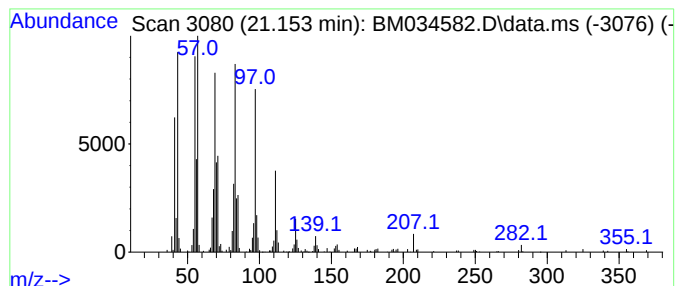

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034582.D
Acq On : 09 Apr 2022 04:14
Operator : CG/JU
Sample : N2319-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.154	5.1	ng/u1	362836	5	21.442	1411360	20.0