

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034586.D
 Acq On : 09 Apr 2022 07:16
 Operator : CG/JU
 Sample : PB143976BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.255	33	37	43	rVB	56384	73870	2.64%	0.238%
2	3.678	105	109	124	rBV	538931	838194	29.97%	2.703%
3	4.019	163	167	172	rVB	20342	31314	1.12%	0.101%
4	6.396	570	571	575	rBV3	2623	3793	0.14%	0.012%
5	7.037	674	680	693	rBV	568736	988703	35.36%	3.188%
6	7.201	702	708	721	rBV	516743	825645	29.53%	2.662%
7	7.401	736	742	760	rBV	639257	1091899	39.05%	3.521%
8	7.878	816	823	832	rVV	453596	743044	26.57%	2.396%
9	8.542	932	936	937	rBV3	1870	2922	0.10%	0.009%
10	8.590	937	944	966	rVV	683289	1236690	44.22%	3.988%
11	9.037	1013	1020	1037	rBV	594423	1024886	36.65%	3.305%
12	9.766	1137	1144	1161	rBV	463889	818567	29.27%	2.639%
13	10.307	1229	1236	1252	rBV	617096	1136291	40.63%	3.664%
14	10.684	1292	1300	1312	rBV	589858	1001049	35.80%	3.228%
15	10.819	1316	1323	1348	rBV	480421	1109981	39.69%	3.579%
16	11.313	1404	1407	1414	rBV8	1534	3139	0.11%	0.010%
17	12.313	1568	1577	1585	rBV3	7924	18625	0.67%	0.060%
18	13.930	1846	1852	1865	rBV	1083916	1654110	59.15%	5.333%
19	14.019	1865	1867	1871	rVB4	4135	6065	0.22%	0.020%
20	14.219	1893	1901	1915	rBV	1285120	1961946	70.16%	6.326%
21	14.524	1946	1953	1962	rBV	805958	1183725	42.33%	3.817%
22	14.719	1979	1986	2012	rBV	141644	464111	16.60%	1.496%
23	14.942	2022	2024	2027	rVB4	3380	3724	0.13%	0.012%
24	15.513	2115	2121	2136	rBV	1634328	2388071	85.40%	7.700%
25	15.630	2136	2141	2154	rVV	470436	736296	26.33%	2.374%
26	15.754	2159	2162	2167	rVB	16972	23974	0.86%	0.077%
27	16.295	2250	2254	2255	rBV4	4640	4525	0.16%	0.015%
28	16.565	2293	2300	2301	rBV5	1425	3050	0.11%	0.010%
29	17.054	2379	2383	2387	rBV5	3560	6030	0.22%	0.019%
30	17.265	2412	2419	2428	rBV	903472	1268888	45.38%	4.091%
31	17.365	2430	2436	2452	rVV	1596400	2441945	87.33%	7.874%
32	17.507	2458	2460	2465	rVB5	3348	3770	0.13%	0.012%
33	17.601	2475	2476	2482	rVB6	2655	4248	0.15%	0.014%
34	19.224	2748	2752	2757	rBV3	20622	26804	0.96%	0.086%
35	19.295	2760	2764	2768	rBV2	14874	22322	0.80%	0.072%
36	19.654	2819	2825	2832	rBV	1981017	2796379	100.00%	9.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034586.D
Acq On : 09 Apr 2022 07:16
Operator : CG/JU
Sample : PB143976BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION

37	21.442	3124	3129	3135	rBV	618584	1047290	37.45%	3.377%
38	23.671	3501	3508	3526	rBV2	1137313	2689346	96.17%	8.671%
39	23.824	3528	3534	3544	rVB2	615915	1328573	47.51%	4.284%




Sum of corrected areas: 31013804

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034586.D
Acq On : 09 Apr 2022 07:16
Operator : CG/JU
Sample : PB143976BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

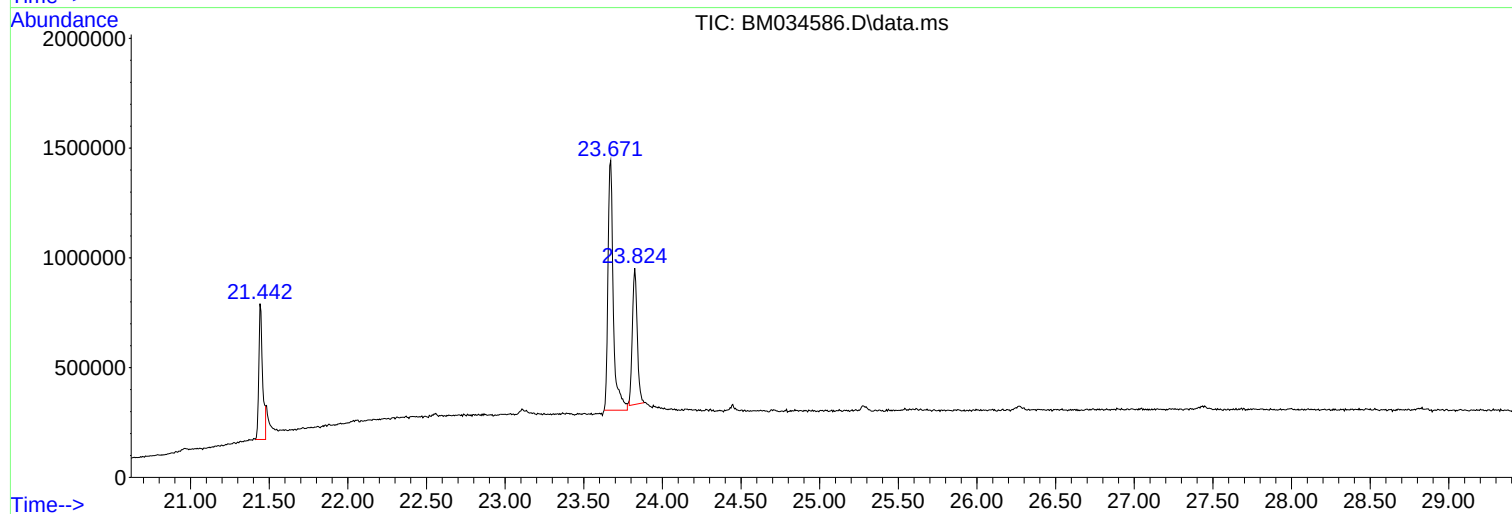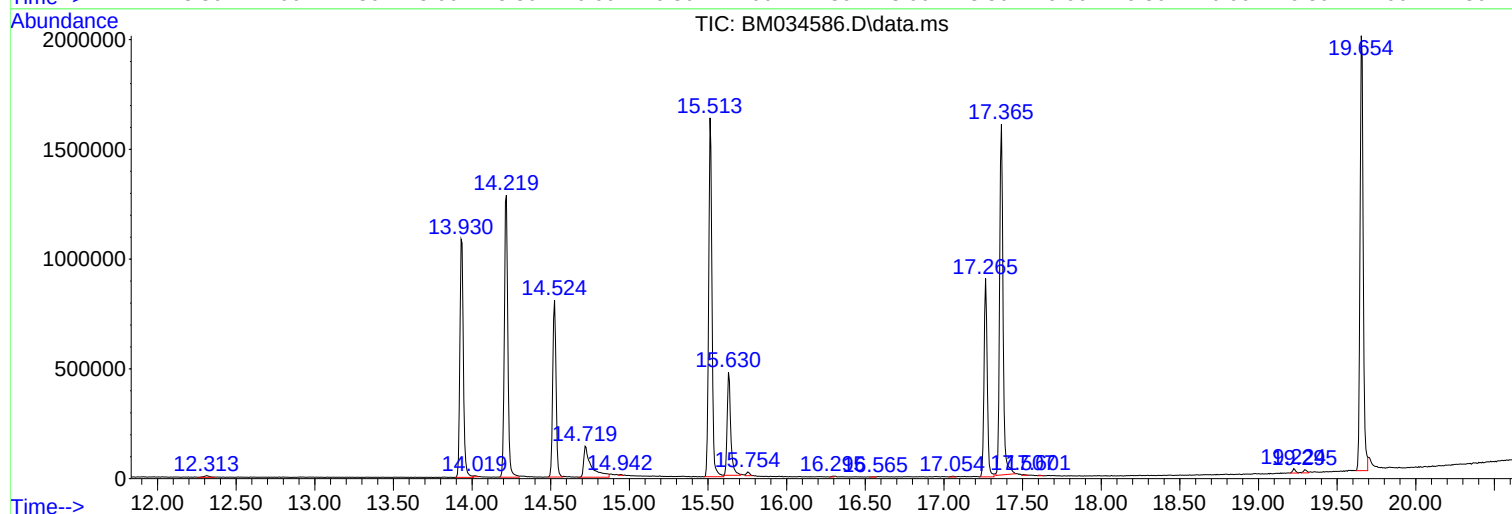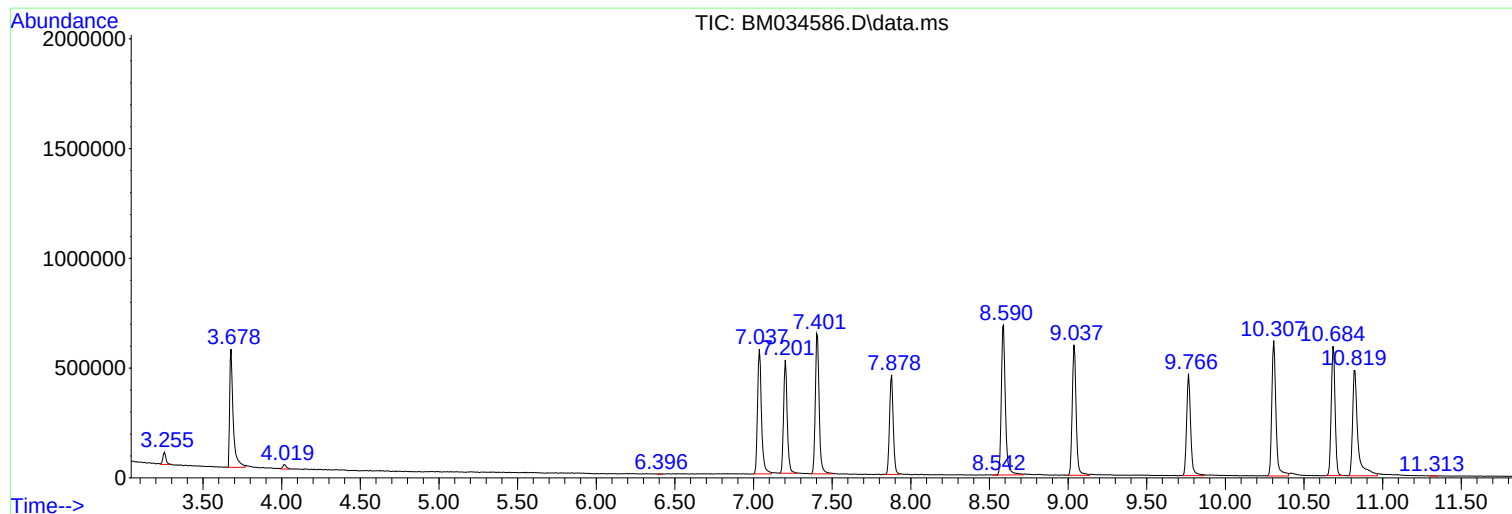

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034586.D
Acq On : 09 Apr 2022 07:16
Operator : CG/JU
Sample : PB143976BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034586.D
Acq On : 09 Apr 2022 07:16
Operator : CG/JU
Sample : PB143976BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc