

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034588.D
 Acq On : 09 Apr 2022 08:29
 Operator : CG/JU
 Sample : PB143975BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	33	36	47	rVB	50490	80394	2.97%	0.282%
2	3.678	105	109	124	rBV	498663	793630	29.34%	2.786%
3	4.013	163	166	173	rVB2	20563	29985	1.11%	0.105%
4	7.037	674	680	694	rBV	546622	928927	34.35%	3.261%
5	7.201	702	708	722	rBV	477730	768862	28.43%	2.699%
6	7.401	736	742	759	rBV	594613	1013347	37.47%	3.558%
7	7.878	816	823	832	rBV	378859	625150	23.11%	2.195%
8	8.590	937	944	961	rBV	647383	1154542	42.69%	4.053%
9	9.037	1014	1020	1033	rBV	549433	952834	35.23%	3.345%
10	9.766	1137	1144	1160	rBV	429768	758218	28.03%	2.662%
11	10.307	1229	1236	1252	rBV	582155	1054177	38.98%	3.701%
12	10.684	1293	1300	1313	rVB	509736	861012	31.84%	3.023%
13	10.825	1316	1324	1346	rBV	452254	1034070	38.23%	3.630%
14	11.948	1512	1515	1518	rBV5	1823	2769	0.10%	0.010%
15	12.313	1569	1577	1584	rBV5	6190	13531	0.50%	0.048%
16	13.936	1846	1853	1865	rBV	1019691	1567742	57.97%	5.504%
17	14.048	1871	1872	1879	rVB6	2871	2811	0.10%	0.010%
18	14.219	1894	1901	1915	rBV	1223866	1864606	68.94%	6.546%
19	14.524	1946	1953	1964	rBV	689415	1027615	38.00%	3.608%
20	14.724	1979	1987	2005	rBV	114334	377338	13.95%	1.325%
21	15.336	2089	2091	2096	rVV5	3288	4686	0.17%	0.016%
22	15.460	2110	2112	2115	rBV3	2760	2982	0.11%	0.010%
23	15.513	2115	2121	2136	rBV	1492635	2270823	83.96%	7.972%
24	15.630	2136	2141	2159	rVV	420032	698123	25.81%	2.451%
25	15.754	2159	2162	2166	rVB2	13731	17920	0.66%	0.063%
26	16.201	2236	2238	2242	rVB4	2204	2714	0.10%	0.010%
27	16.307	2251	2256	2260	rBB7	4196	5542	0.20%	0.019%
28	17.054	2379	2383	2386	rBV5	3053	4104	0.15%	0.014%
29	17.265	2413	2419	2428	rBV	748826	1075974	39.78%	3.778%
30	17.365	2430	2436	2459	rVB	1512879	2332071	86.23%	8.188%
31	19.224	2749	2752	2758	rVB4	16918	22899	0.85%	0.080%
32	19.295	2761	2764	2768	rVB2	12029	18130	0.67%	0.064%
33	19.654	2819	2825	2844	rBV	1850579	2704570	100.00%	9.495%
34	21.448	3125	3130	3134	rBV	455653	770404	28.49%	2.705%
35	23.671	3501	3508	3525	rBV	1070591	2496314	92.30%	8.764%
36	23.824	3528	3534	3547	rVB2	519988	1144395	42.31%	4.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034588.D
Acq On : 09 Apr 2022 08:29
Operator : CG/JU
Sample : PB143975BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION


Sum of corrected areas: 28483211

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034588.D
Acq On : 09 Apr 2022 08:29
Operator : CG/JU
Sample : PB143975BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

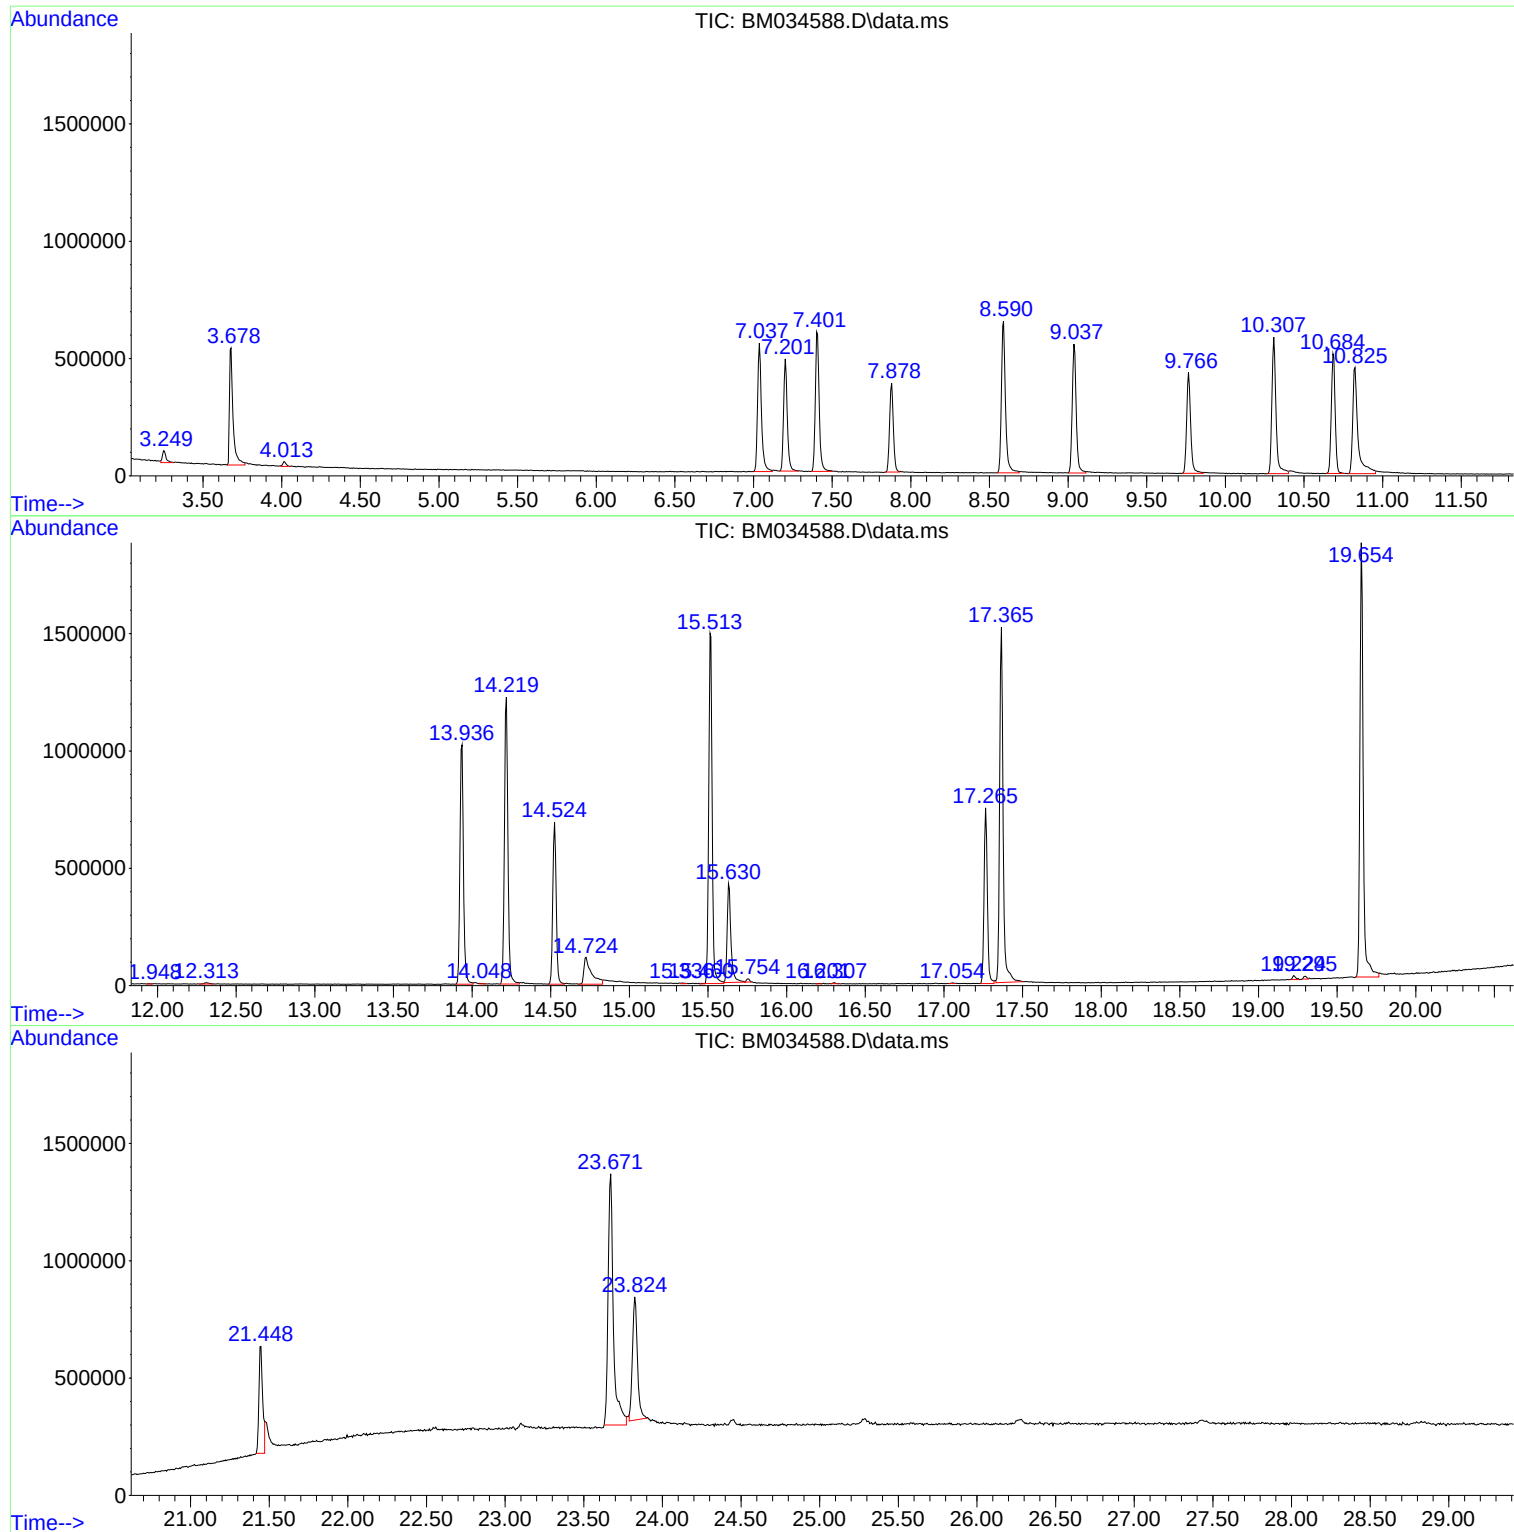

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034588.D
Acq On : 09 Apr 2022 08:29
Operator : CG/JU
Sample : PB143975BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034588.D
Acq On : 09 Apr 2022 08:29
Operator : CG/JU
Sample : PB143975BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------