

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034589.D
 Acq On : 09 Apr 2022 09:05
 Operator : CG/JU
 Sample : PB143959BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	33	37	42	rVB	46139	59916	2.26%	0.214%
2	3.678	105	109	129	rBV	483704	744891	28.08%	2.660%
3	4.019	163	167	171	rBV3	12667	16549	0.62%	0.059%
4	4.590	262	264	266	rBV2	4048	3560	0.13%	0.013%
5	5.731	456	458	461	rBV3	3424	2805	0.11%	0.010%
6	7.037	674	680	692	rBV	516231	886948	33.44%	3.167%
7	7.201	702	708	726	rVB	459902	745004	28.09%	2.660%
8	7.401	736	742	757	rBV	563762	975113	36.76%	3.482%
9	7.878	816	823	836	rBV	431004	709469	26.75%	2.533%
10	8.589	936	944	956	rBV	623121	1092790	41.20%	3.902%
11	9.036	1013	1020	1037	rBV	520417	919556	34.67%	3.283%
12	9.766	1137	1144	1164	rBV	402468	730150	27.53%	2.607%
13	10.307	1229	1236	1254	rBV	549404	1020255	38.46%	3.643%
14	10.466	1261	1263	1266	rVB4	3808	3631	0.14%	0.013%
15	10.683	1293	1300	1311	rBV	555324	954522	35.99%	3.408%
16	10.825	1316	1324	1337	rBV	420554	905413	34.13%	3.233%
17	12.313	1570	1577	1581	rBV3	5316	10701	0.40%	0.038%
18	13.495	1773	1778	1784	rBV7	1727	3275	0.12%	0.012%
19	13.936	1846	1853	1865	rBV	964351	1469429	55.40%	5.247%
20	14.218	1893	1901	1912	rBV	1143293	1740339	65.61%	6.214%
21	14.324	1917	1919	1922	rVV4	5263	7419	0.28%	0.026%
22	14.371	1926	1927	1932	rVB4	2303	3376	0.13%	0.012%
23	14.524	1946	1953	1966	rBV	769565	1126458	42.47%	4.022%
24	14.648	1972	1974	1980	rVB5	1517	2693	0.10%	0.010%
25	14.724	1980	1987	2008	rBV2	107916	371956	14.02%	1.328%
26	15.324	2087	2089	2093	rVB4	3925	4475	0.17%	0.016%
27	15.512	2115	2121	2136	rVV	1417163	2141517	80.74%	7.646%
28	15.630	2136	2141	2158	rVV	396420	685766	25.85%	2.449%
29	15.754	2158	2162	2170	rVB2	16725	29838	1.12%	0.107%
30	16.301	2251	2255	2259	rBV5	5239	7110	0.27%	0.025%
31	17.065	2379	2385	2389	rBV5	3293	5397	0.20%	0.019%
32	17.265	2413	2419	2430	rBV	813744	1192210	44.95%	4.257%
33	17.365	2430	2436	2457	rVB	1452930	2221675	83.76%	7.933%
34	18.206	2577	2579	2583	rBV4	2096	3147	0.12%	0.011%
35	18.248	2583	2586	2589	rBV3	2465	3593	0.14%	0.013%
36	19.224	2749	2752	2758	rVB4	16058	23601	0.89%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION

37	19.295	2761	2764	2770	rVB2	12284	17603	0.66%	0.063%
38	19.653	2819	2825	2847	rBV	1759234	2652494	100.00%	9.471%
39	21.442	3125	3129	3134	rBV	554589	886750	33.43%	3.166%
40	23.671	3501	3508	3515	rBV	1088563	2265694	85.42%	8.090%
41	23.824	3528	3534	3550	rVB2	602873	1360026	51.27%	4.856%


Sum of corrected areas: 28007114

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

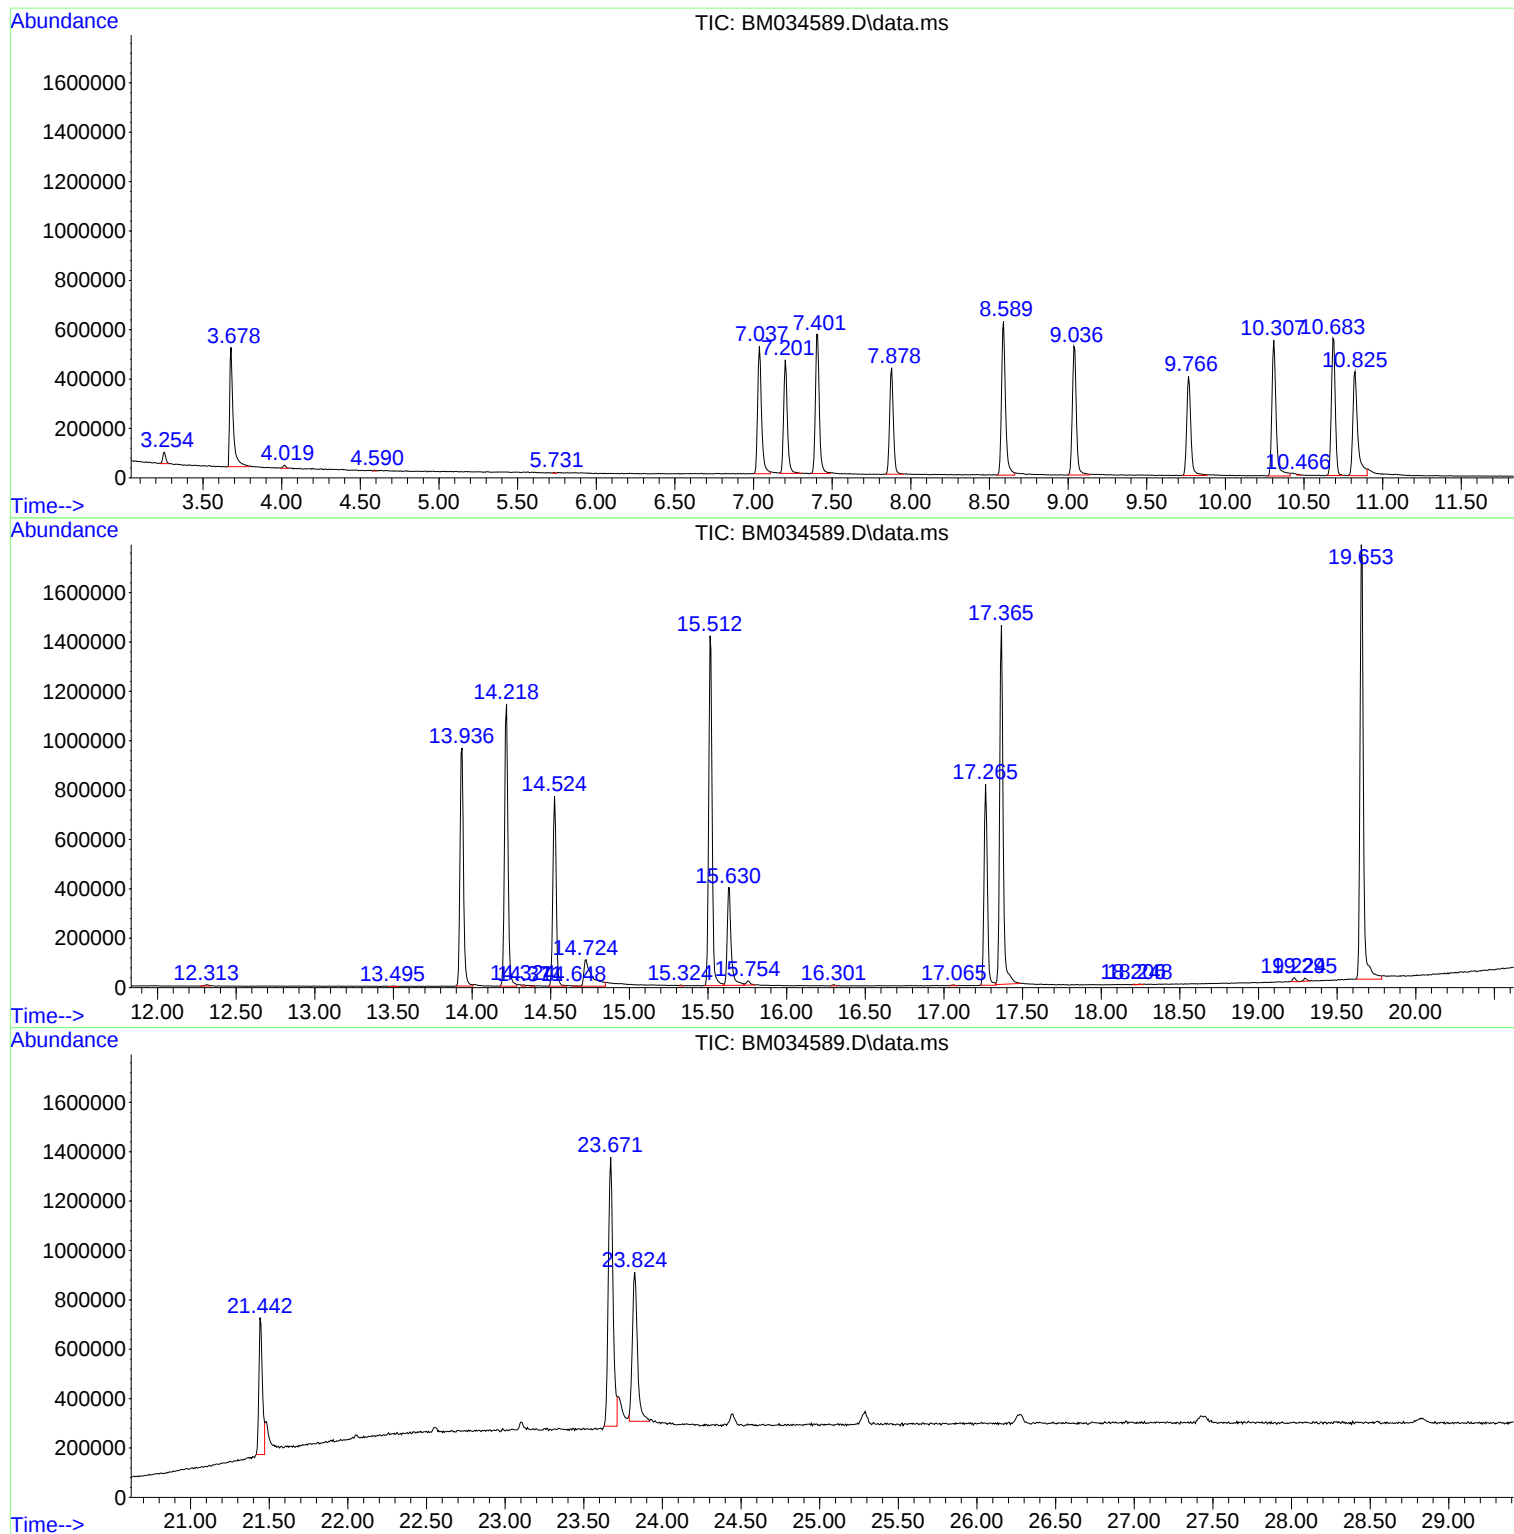

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034589.D
Acq On : 09 Apr 2022 09:05
Operator : CG/JU
Sample : PB143959BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------