

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034593.D
 Acq On : 09 Apr 2022 11:30
 Operator : CG/JU
 Sample : N2319-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	27	32	44	rVB2	193859	302231	10.39%	1.196%
2	3.684	107	110	126	rBV	93647	164616	5.66%	0.651%
3	4.014	164	166	170	rVB2	10092	11415	0.39%	0.045%
4	4.561	254	259	266	rVB	50844	71497	2.46%	0.283%
5	6.878	648	653	659	rVB2	8495	13606	0.47%	0.054%
6	7.043	673	681	690	rBV	64833	134763	4.63%	0.533%
7	7.202	702	708	723	rBV	399931	658207	22.62%	2.604%
8	7.407	737	743	757	rBV	352266	637772	21.92%	2.523%
9	7.878	816	823	833	rBV	376537	633158	21.76%	2.505%
10	8.119	860	864	869	rVB6	4428	7164	0.25%	0.028%
11	8.590	938	944	963	rBV	227736	431179	14.82%	1.706%
12	9.037	1012	1020	1035	rBV	459355	827833	28.45%	3.275%
13	9.219	1048	1051	1055	rVB6	3792	5346	0.18%	0.021%
14	9.484	1092	1096	1102	rVB2	11840	17567	0.60%	0.069%
15	9.766	1137	1144	1159	rBV	345438	630163	21.66%	2.493%
16	10.307	1229	1236	1253	rBV	433292	806866	27.73%	3.192%
17	10.684	1293	1300	1312	rBV	505782	861730	29.61%	3.409%
18	10.825	1317	1324	1347	rBV	302858	725916	24.95%	2.871%
19	11.119	1369	1374	1377	rBV6	1737	3104	0.11%	0.012%
20	12.137	1543	1547	1553	rVB6	3786	6210	0.21%	0.025%
21	12.313	1570	1577	1586	rBV5	5356	12002	0.41%	0.047%
22	12.772	1649	1655	1657	rBV5	2486	4311	0.15%	0.017%
23	13.078	1702	1707	1711	rBV4	2012	3236	0.11%	0.013%
24	13.366	1751	1756	1761	rVB3	6798	10442	0.36%	0.041%
25	13.707	1809	1814	1819	rBV7	1692	3649	0.13%	0.014%
26	13.931	1846	1852	1865	rBV	859233	1332148	45.78%	5.269%
27	14.219	1893	1901	1915	rBV	1094689	1629698	56.01%	6.446%
28	14.395	1926	1931	1936	rBV6	11113	19113	0.66%	0.076%
29	14.525	1946	1953	1965	rBV	700674	1021468	35.10%	4.041%
30	14.760	1987	1993	1996	rBV5	6804	13741	0.47%	0.054%
31	14.883	2011	2014	2017	rVB4	2800	3069	0.11%	0.012%
32	15.272	2076	2080	2085	rVB5	3089	3960	0.14%	0.016%
33	15.513	2115	2121	2136	rBV	1360899	2086593	71.71%	8.254%
34	15.630	2136	2141	2160	rVV	374098	663678	22.81%	2.625%
35	15.760	2160	2163	2167	rVB3	12841	18122	0.62%	0.072%
36	16.301	2253	2255	2260	rVB6	4379	5506	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034593.D
 Acq On : 09 Apr 2022 11:30
 Operator : CG/JU
 Sample : N2319-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	16.342	2260	2262	2265	rBV3	3634	4119	0.14%	0.016%
38	16.777	2331	2336	2339	rVB5	2307	3073	0.11%	0.012%
39	16.813	2339	2342	2347	rBV6	1519	3438	0.12%	0.014%
40	17.036	2376	2380	2382	rBV4	5323	7695	0.26%	0.030%
41	17.266	2413	2419	2429	rBV	761430	1087901	37.39%	4.303%
42	17.366	2429	2436	2460	rVB	1504619	2342435	80.50%	9.266%
43	17.624	2478	2480	2487	rVB7	5350	8993	0.31%	0.036%
44	18.189	2569	2576	2581	rBV6	18466	44687	1.54%	0.177%
45	19.224	2748	2752	2757	rBV2	19108	25657	0.88%	0.101%
46	19.295	2760	2764	2768	rBV3	15253	21290	0.73%	0.084%
47	19.654	2819	2825	2832	rBV	1989362	2761294	94.90%	10.923%
48	21.160	3078	3081	3089	rVB6	36281	51932	1.78%	0.205%
49	21.442	3125	3129	3135	rBV	561796	913759	31.40%	3.614%
50	23.671	3501	3508	3525	rBV2	1288795	2909835	100.00%	11.510%
51	23.824	3528	3534	3547	rVB2	605679	1313305	45.13%	5.195%


Sum of corrected areas: 25280492

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034593.D
Acq On : 09 Apr 2022 11:30
Operator : CG/JU
Sample : N2319-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

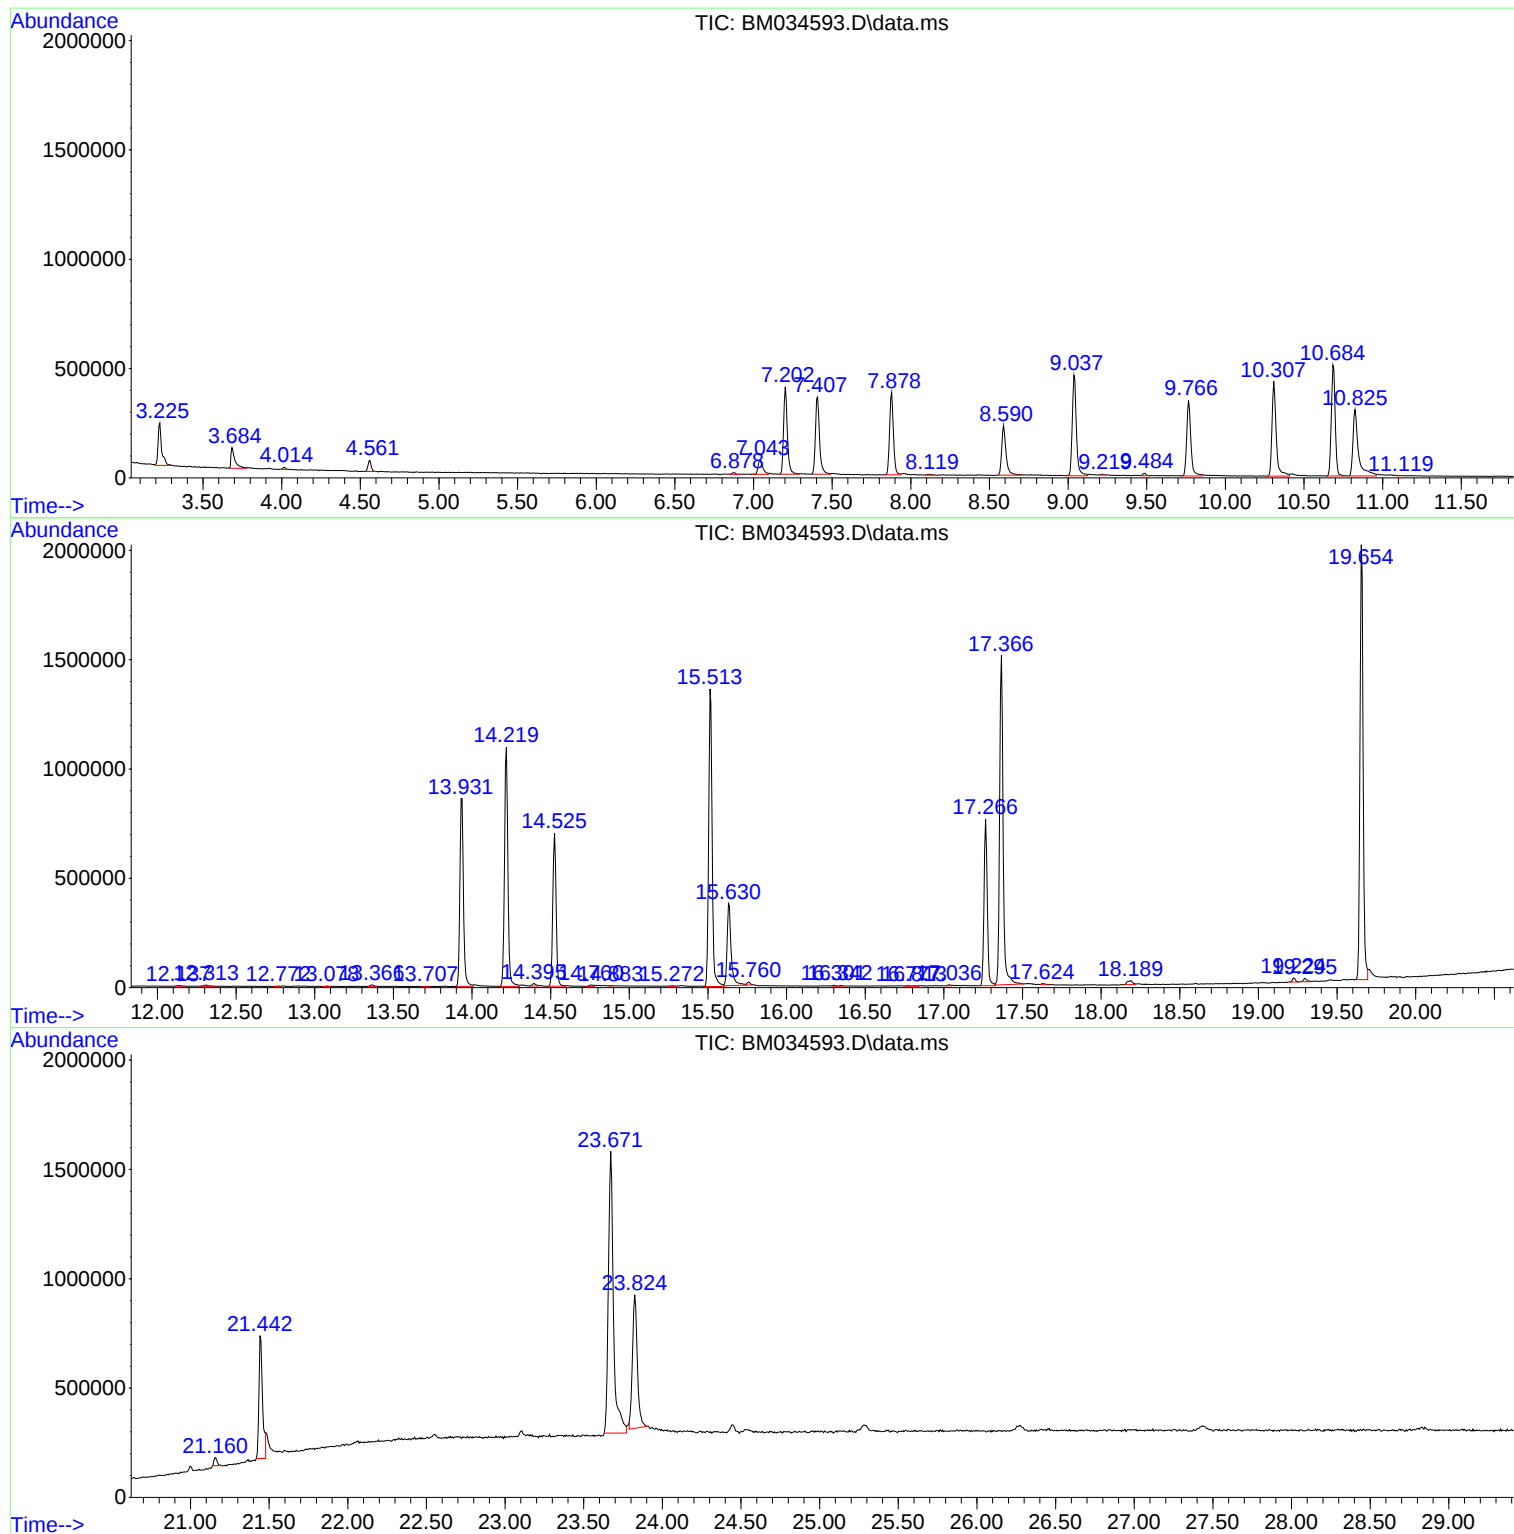

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034593.D
Acq On : 09 Apr 2022 11:30
Operator : CG/JU
Sample : N2319-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034593.D
Acq On : 09 Apr 2022 11:30
Operator : CG/JU
Sample : N2319-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------