

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034597.D
 Acq On : 09 Apr 2022 13:56
 Operator : CG/JU
 Sample : N2319-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	28	32	35	rBV	100291	127290	4.34%	0.467%
2	3.684	107	110	133	rVB	123264	223668	7.62%	0.820%
3	4.560	254	259	265	rVB	101988	144352	4.92%	0.529%
4	6.872	649	652	656	rVB4	5389	8405	0.29%	0.031%
5	7.042	675	681	690	rBV	93608	183235	6.24%	0.672%
6	7.201	702	708	723	rBV	471870	778981	26.53%	2.855%
7	7.407	736	743	756	rBV	445396	778886	26.53%	2.855%
8	7.878	816	823	835	rBV	421596	706430	24.06%	2.589%
9	8.589	936	944	956	rBV	302013	548237	18.67%	2.010%
10	9.042	1013	1021	1034	rBV	526618	956314	32.57%	3.505%
11	9.407	1079	1083	1086	rBV5	3556	3775	0.13%	0.014%
12	9.766	1137	1144	1158	rBV	418571	728688	24.82%	2.671%
13	10.307	1229	1236	1252	rBV	528695	970726	33.07%	3.558%
14	10.454	1259	1261	1265	rVB4	3229	3415	0.12%	0.013%
15	10.683	1294	1300	1315	rVB	534950	922787	31.43%	3.382%
16	10.825	1317	1324	1336	rBV	382951	803718	27.38%	2.946%
17	12.071	1531	1536	1539	rBV5	1735	3092	0.11%	0.011%
18	12.307	1568	1576	1585	rBV6	6301	16862	0.57%	0.062%
19	13.824	1830	1834	1837	rVB4	1938	3222	0.11%	0.012%
20	13.936	1846	1853	1864	rBV	1043914	1546740	52.69%	5.669%
21	14.013	1864	1866	1873	rVB5	5913	11078	0.38%	0.041%
22	14.218	1894	1901	1914	rBV	1240217	1842497	62.76%	6.754%
23	14.318	1916	1918	1923	rVB5	4095	5951	0.20%	0.022%
24	14.524	1947	1953	1964	rBV	735638	1070558	36.47%	3.924%
25	14.754	1987	1992	1994	rBV5	8103	13585	0.46%	0.050%
26	15.330	2088	2090	2093	rBV3	2557	3219	0.11%	0.012%
27	15.518	2115	2122	2135	rBV	1515929	2347056	79.95%	8.603%
28	15.636	2135	2142	2156	rVV	428969	731848	24.93%	2.683%
29	15.759	2159	2163	2173	rVB3	17335	37880	1.29%	0.139%
30	16.301	2252	2255	2261	rVB7	5634	7796	0.27%	0.029%
31	16.954	2361	2366	2370	rVB7	2040	3538	0.12%	0.013%
32	17.054	2380	2383	2386	rVB4	2823	3439	0.12%	0.013%
33	17.265	2413	2419	2429	rBV	768267	1123605	38.27%	4.118%
34	17.365	2429	2436	2455	rVV2	1663167	2507454	85.41%	9.191%
35	18.189	2572	2576	2584	rBV5	15222	27104	0.92%	0.099%
36	19.112	2731	2733	2737	rBV5	3088	3979	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034597.D
Acq On : 09 Apr 2022 13:56
Operator : CG/JU
Sample : N2319-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2K4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION

37	19.224	2748	2752	2757	rBV3	19883	29544	1.01%	0.108%
38	19.295	2760	2764	2768	rBV2	17837	26198	0.89%	0.096%
39	19.653	2819	2825	2833	rBV	2037787	2935739	100.00%	10.761%
40	21.447	3125	3130	3134	rBV	574561	905189	30.83%	3.318%
41	23.671	3501	3508	3516	rBV2	1349082	2856103	97.29%	10.469%
42	23.824	3528	3534	3547	rVB2	608089	1329760	45.30%	4.874%


Sum of corrected areas: 27281943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034597.D
Acq On : 09 Apr 2022 13:56
Operator : CG/JU
Sample : N2319-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2K4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

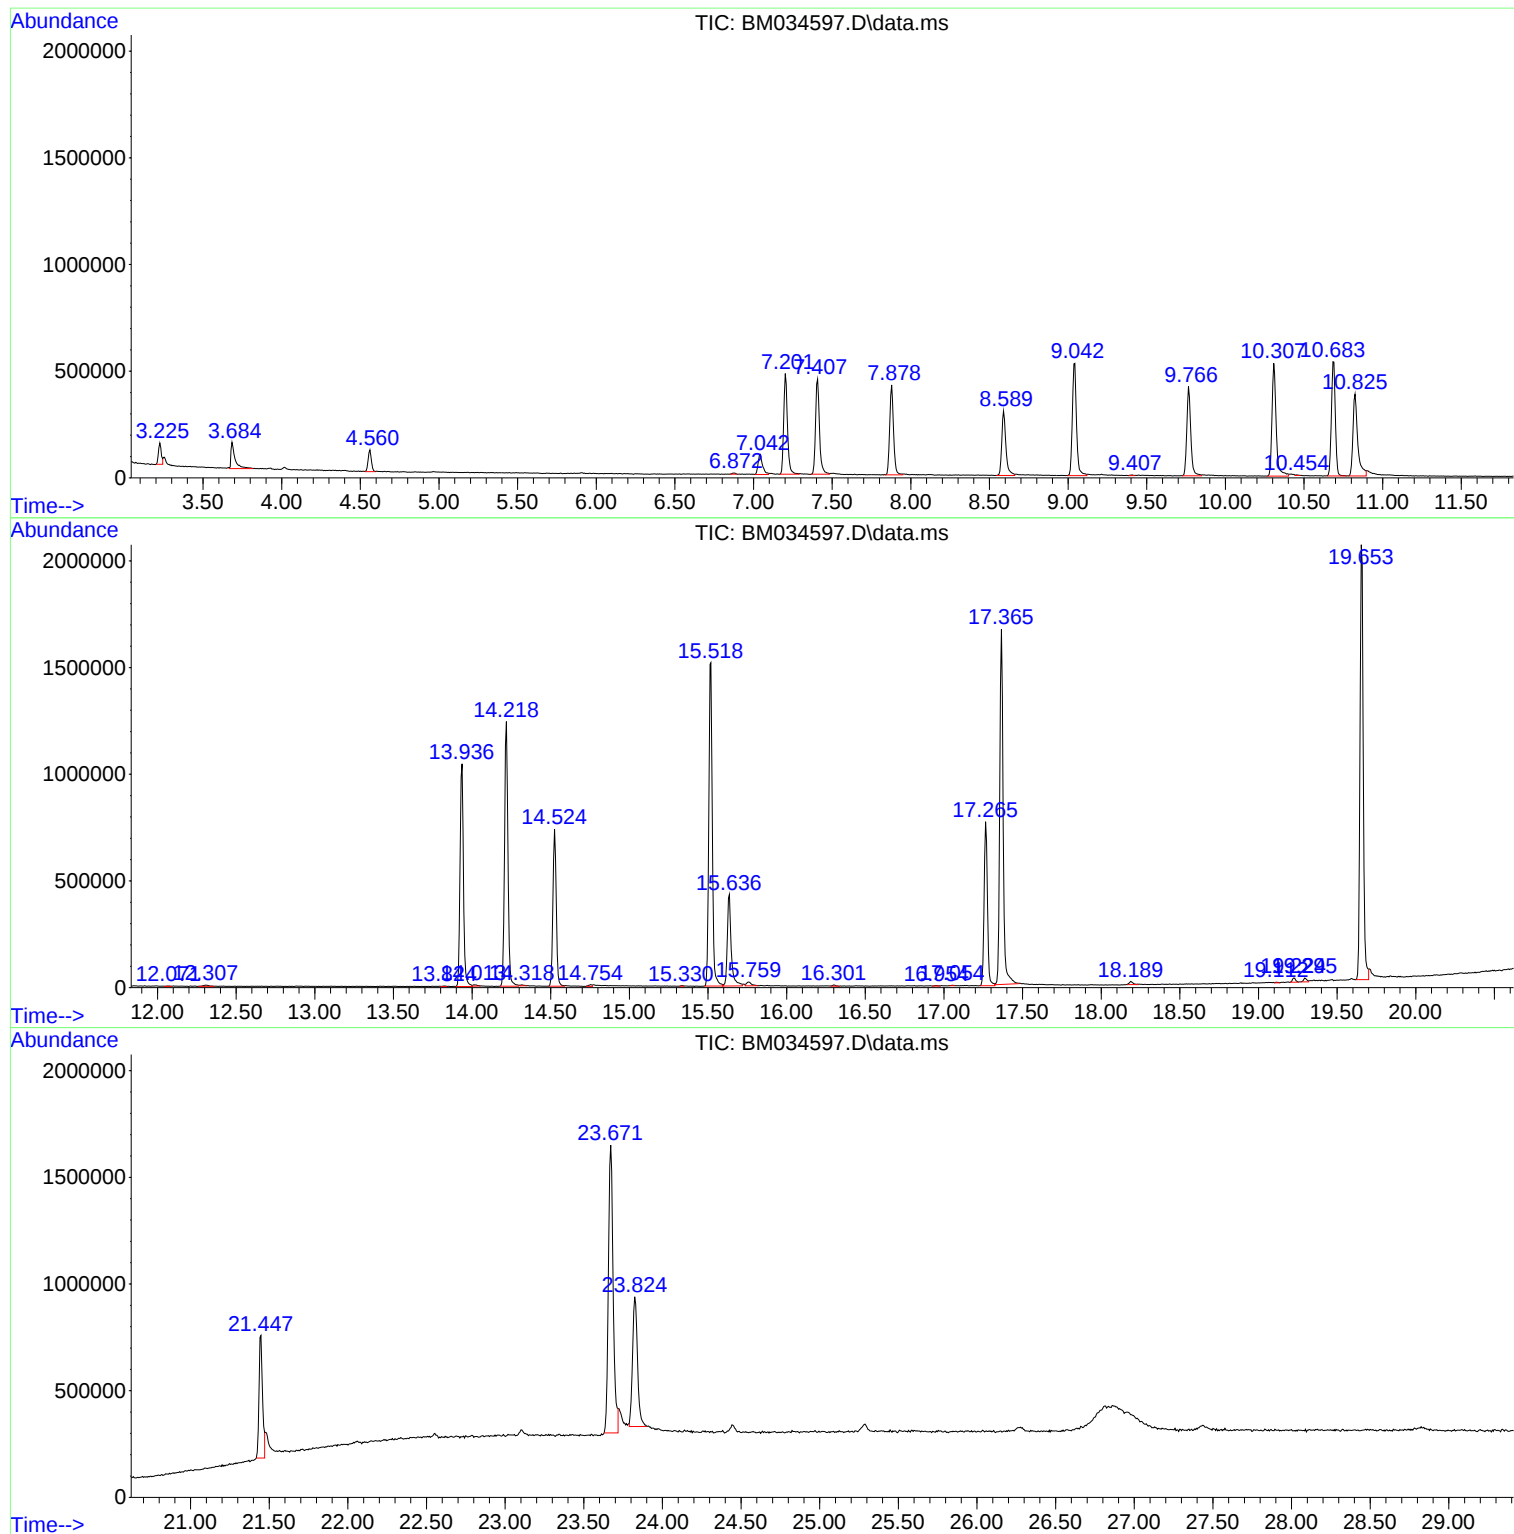

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034597.D
Acq On : 09 Apr 2022 13:56
Operator : CG/JU
Sample : N2319-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2K4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034597.D
Acq On : 09 Apr 2022 13:56
Operator : CG/JU
Sample : N2319-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2K4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc