

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034598.D
 Acq On : 09 Apr 2022 14:32
 Operator : CG/JU
 Sample : N2266-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.254	34	37	42	rVB	32497	38024	1.07%	0.122%
2	3.690	108	111	120	rBV	95918	157311	4.44%	0.506%
3	6.872	649	652	656	rVB3	5715	7710	0.22%	0.025%
4	7.042	672	681	692	rBV	84821	179430	5.06%	0.577%
5	7.201	702	708	725	rVB	480252	807462	22.79%	2.598%
6	7.407	737	743	755	rBV	447390	757916	21.39%	2.438%
7	7.878	816	823	833	rBV	469806	757729	21.39%	2.438%
8	8.589	938	944	958	rBV	279382	502880	14.19%	1.618%
9	9.042	1012	1021	1035	rBV	567877	1020983	28.82%	3.285%
10	9.219	1046	1051	1056	rVB5	8097	14266	0.40%	0.046%
11	9.766	1138	1144	1160	rBV	428650	751562	21.21%	2.418%
12	10.307	1230	1236	1254	rBV	552120	1009012	28.48%	3.246%
13	10.689	1293	1301	1311	rBV	605454	1037126	29.27%	3.337%
14	10.825	1317	1324	1351	rBV	428335	948832	26.78%	3.053%
15	12.301	1569	1575	1584	rVB7	5978	13964	0.39%	0.045%
16	13.936	1846	1853	1864	rBV	1245149	1767459	49.89%	5.686%
17	14.019	1866	1867	1879	rVB5	6565	10676	0.30%	0.034%
18	14.218	1894	1901	1915	rBV	1419508	2067118	58.34%	6.650%
19	14.524	1945	1953	1964	rBV	876249	1273611	35.95%	4.097%
20	14.766	1987	1994	1996	rBV5	5869	12002	0.34%	0.039%
21	15.330	2086	2090	2095	rVB6	2926	4350	0.12%	0.014%
22	15.513	2115	2121	2136	rBV	1724708	2606372	73.56%	8.385%
23	15.636	2136	2142	2158	rVV	448624	740559	20.90%	2.382%
24	15.754	2159	2162	2168	rVB3	16305	26418	0.75%	0.085%
25	16.301	2250	2255	2260	rVB8	5151	10130	0.29%	0.033%
26	17.048	2377	2382	2383	rBV5	2907	4105	0.12%	0.013%
27	17.265	2413	2419	2429	rBV	968302	1381989	39.01%	4.446%
28	17.365	2430	2436	2455	rVV	1954254	2942313	83.05%	9.466%
29	17.942	2530	2534	2539	rVB6	8531	13620	0.38%	0.044%
30	18.189	2571	2576	2577	rBV5	3337	4694	0.13%	0.015%
31	19.224	2748	2752	2759	rBV3	22482	35753	1.01%	0.115%
32	19.295	2759	2764	2769	rBV3	21752	33836	0.96%	0.109%
33	19.653	2819	2825	2844	rBV	2413180	3543020	100.00%	11.398%
34	21.359	3112	3115	3120	rBV	152326	165348	4.67%	0.532%
35	21.442	3124	3129	3145	rBV	730252	1458860	41.18%	4.693%
36	23.671	3501	3508	3525	rBV	1500944	3402990	96.05%	10.948%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION

37	23.824	3528	3534	3546	rVB2	738283	1574197	44.43%	5.064%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 31083627

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

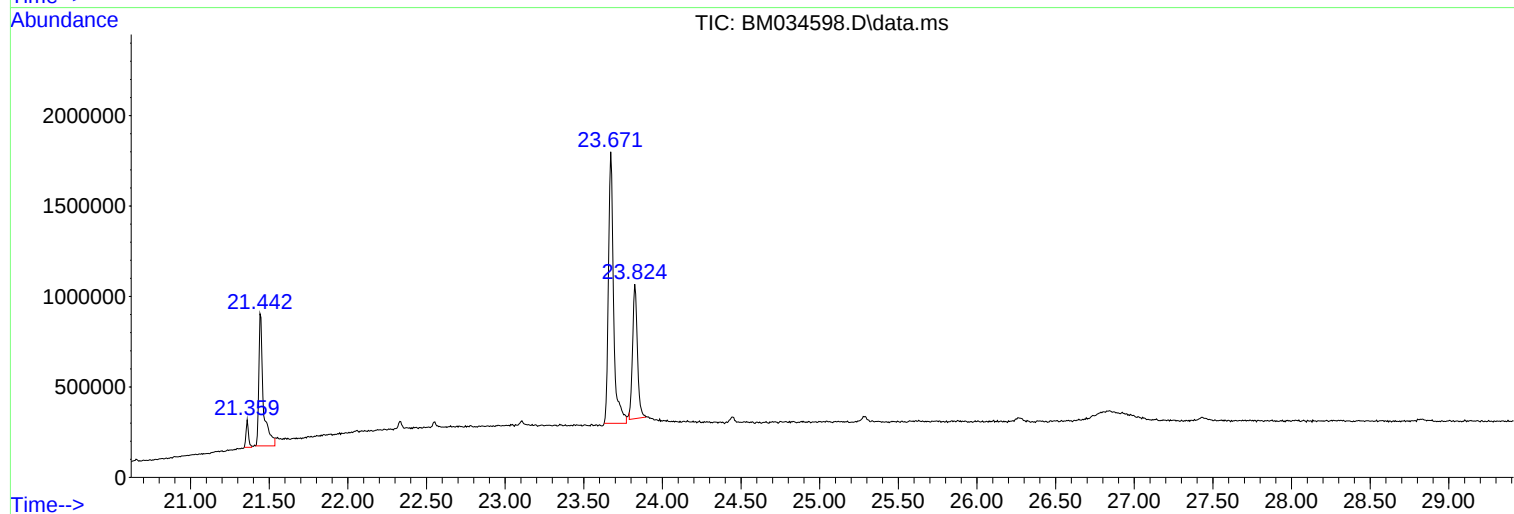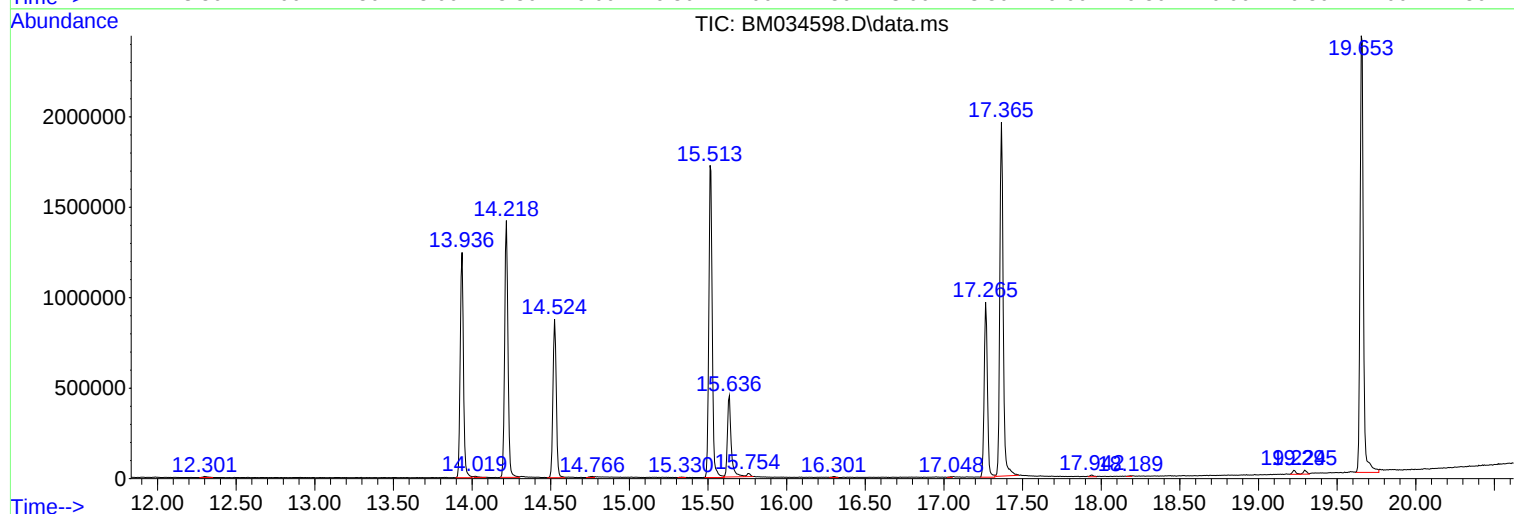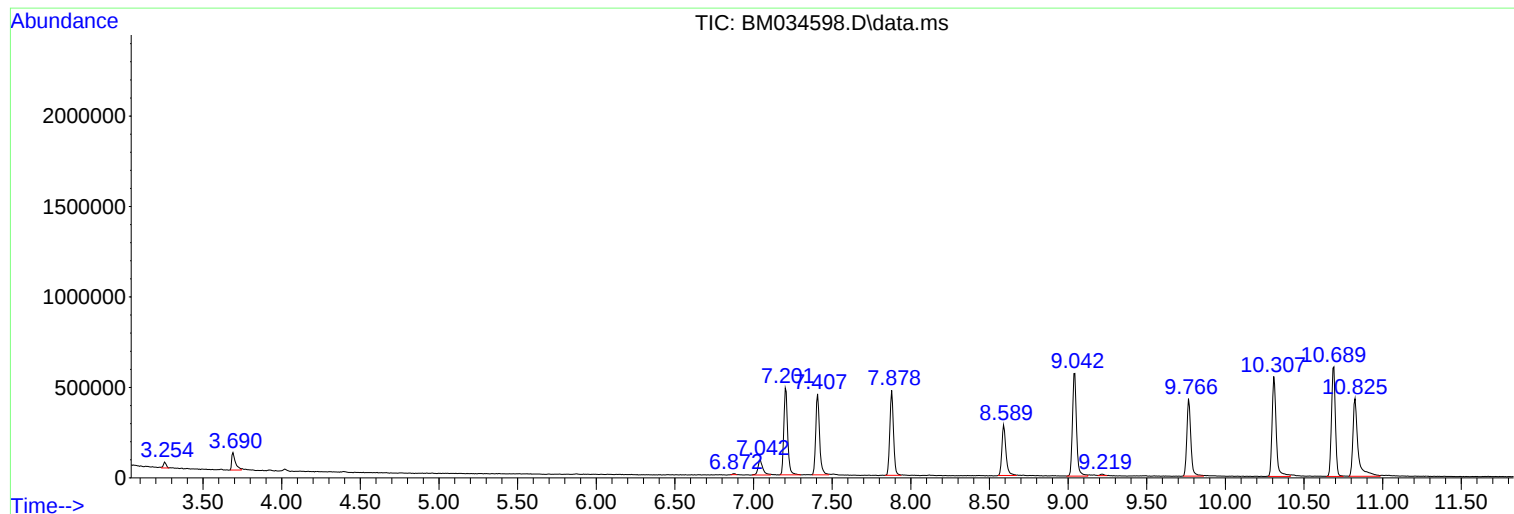

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034598.D
Acq On : 09 Apr 2022 14:32
Operator : CG/JU
Sample : N2266-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------