

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034599.D
 Acq On : 09 Apr 2022 15:08
 Operator : CG/JU
 Sample : N2266-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.255	34	37	44	rVB	38004	46694	1.39%	0.149%
2	3.684	107	110	129	rBV	153997	247432	7.38%	0.790%
3	4.019	164	167	171	rVB3	11745	15038	0.45%	0.048%
4	6.878	648	653	658	rVB2	9955	14663	0.44%	0.047%
5	7.043	675	681	689	rBV	84078	170481	5.09%	0.544%
6	7.201	702	708	722	rBV	471449	776017	23.15%	2.477%
7	7.407	737	743	758	rBV	414602	705183	21.04%	2.251%
8	7.878	816	823	831	rBV	459789	739752	22.07%	2.361%
9	7.954	832	836	844	rVB7	7216	15812	0.47%	0.050%
10	8.119	860	864	869	rBV6	6639	12848	0.38%	0.041%
11	8.431	915	917	920	rBV4	3971	4652	0.14%	0.015%
12	8.589	936	944	957	rBV	282049	505028	15.07%	1.612%
13	8.984	1007	1011	1013	rBV4	2444	3391	0.10%	0.011%
14	9.037	1013	1020	1038	rVV	532114	958663	28.60%	3.060%
15	9.484	1091	1096	1104	rVB	15250	27624	0.82%	0.088%
16	9.766	1137	1144	1161	rBV	388547	693639	20.69%	2.214%
17	10.307	1229	1236	1254	rBV	500168	921973	27.51%	2.943%
18	10.478	1259	1265	1275	rBV3	32790	88196	2.63%	0.282%
19	10.683	1294	1300	1313	rVB	595225	1010155	30.14%	3.224%
20	10.825	1317	1324	1346	rBV	432030	920407	27.46%	2.938%
21	11.989	1515	1522	1527	rBV2	18056	28784	0.86%	0.092%
22	12.130	1543	1546	1553	rVB6	4150	6855	0.20%	0.022%
23	12.289	1567	1573	1580	rBV6	7456	15325	0.46%	0.049%
24	12.942	1679	1684	1686	rVB6	3033	4183	0.12%	0.013%
25	13.142	1714	1718	1721	rBV6	3001	3987	0.12%	0.013%
26	13.360	1750	1755	1760	rVB2	14886	20930	0.62%	0.067%
27	13.936	1846	1853	1864	rBV	1192031	1742042	51.97%	5.561%
28	14.019	1864	1867	1870	rVB5	3792	5876	0.18%	0.019%
29	14.219	1894	1901	1913	rBV	1371677	2004342	59.80%	6.398%
30	14.319	1914	1918	1924	rVB6	5780	10210	0.30%	0.033%
31	14.430	1933	1937	1940	rVB4	6101	7812	0.23%	0.025%
32	14.524	1946	1953	1965	rBV	841787	1229820	36.69%	3.926%
33	14.748	1986	1991	2001	rBV10	19036	55833	1.67%	0.178%
34	15.071	2039	2046	2051	rBV2	26173	51113	1.52%	0.163%
35	15.148	2056	2059	2064	rVB7	6927	11106	0.33%	0.035%
36	15.318	2079	2088	2095	rBV3	18295	48347	1.44%	0.154%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
 Data File : BM034599.D
 Acq On : 09 Apr 2022 15:08
 Operator : CG/JU
 Sample : N2266-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	15.513	2115	2121	2135	rBV	1712644	2580374	76.99%	8.236%
38	15.630	2135	2141	2154	rVV	486175	754235	22.50%	2.407%
39	15.760	2159	2163	2171	rVB	17133	30364	0.91%	0.097%
40	16.301	2252	2255	2257	rBV4	5884	7361	0.22%	0.023%
41	16.665	2314	2317	2322	rBV5	3826	7490	0.22%	0.024%
42	17.265	2413	2419	2429	rBV	950260	1364444	40.71%	4.355%
43	17.365	2430	2436	2458	rVV	1884320	2797657	83.47%	8.930%
44	18.165	2568	2572	2578	rBV4	44522	72958	2.18%	0.233%
45	19.224	2749	2752	2759	rVB3	30685	40883	1.22%	0.130%
46	19.301	2761	2765	2771	rVV2	23125	36589	1.09%	0.117%
47	19.377	2775	2778	2782	rVV3	27220	29947	0.89%	0.096%
48	19.442	2786	2789	2798	rVB6	25773	38912	1.16%	0.124%
49	19.589	2812	2814	2819	rBV6	8937	10358	0.31%	0.033%
50	19.659	2820	2826	2833	rBV	2377792	3351745	100.00%	10.699%
51	21.159	3077	3081	3089	rBV4	75100	131836	3.93%	0.421%
52	21.442	3124	3129	3143	rBV	843261	1487044	44.37%	4.747%
53	22.618	3325	3329	3335	rBV	427322	604946	18.05%	1.931%
54	23.671	3501	3508	3515	rBV2	1542516	3210629	95.79%	10.248%
55	23.824	3528	3534	3545	rVB2	781275	1646686	49.13%	5.256%




Sum of corrected areas: 31328671

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

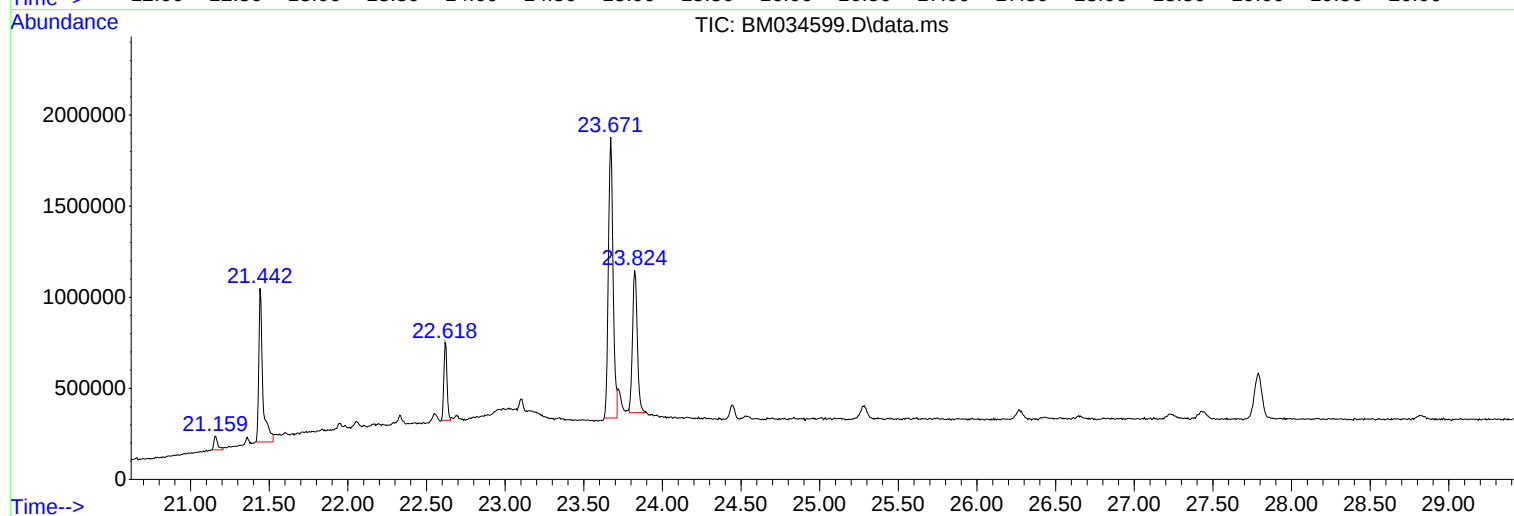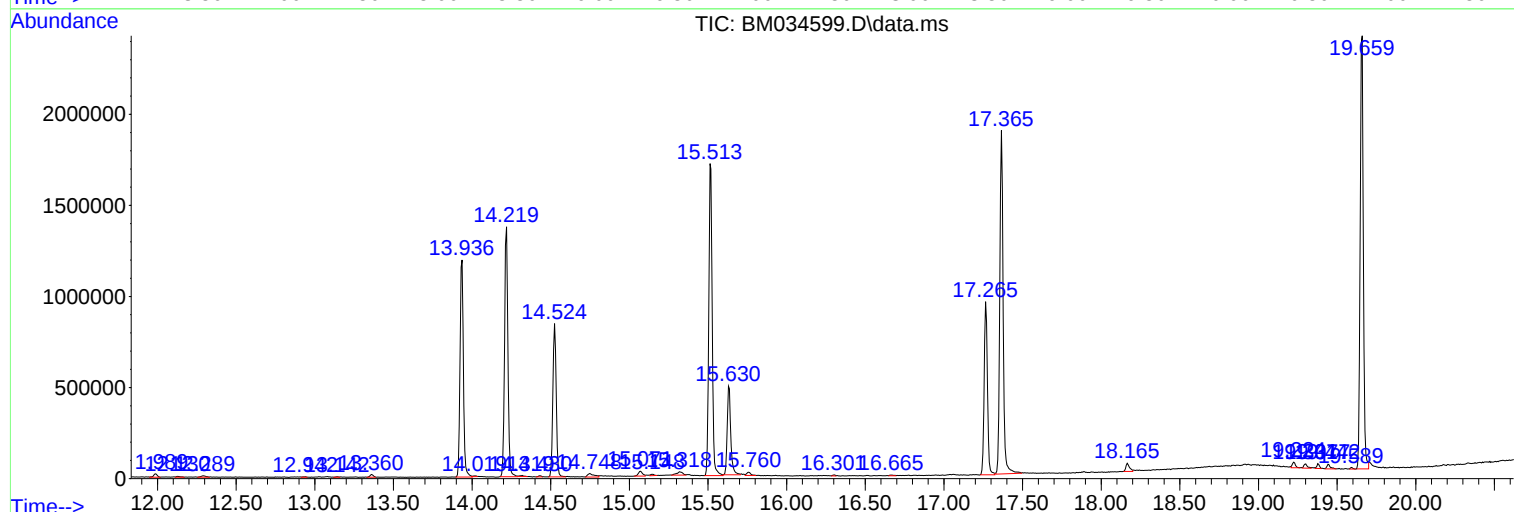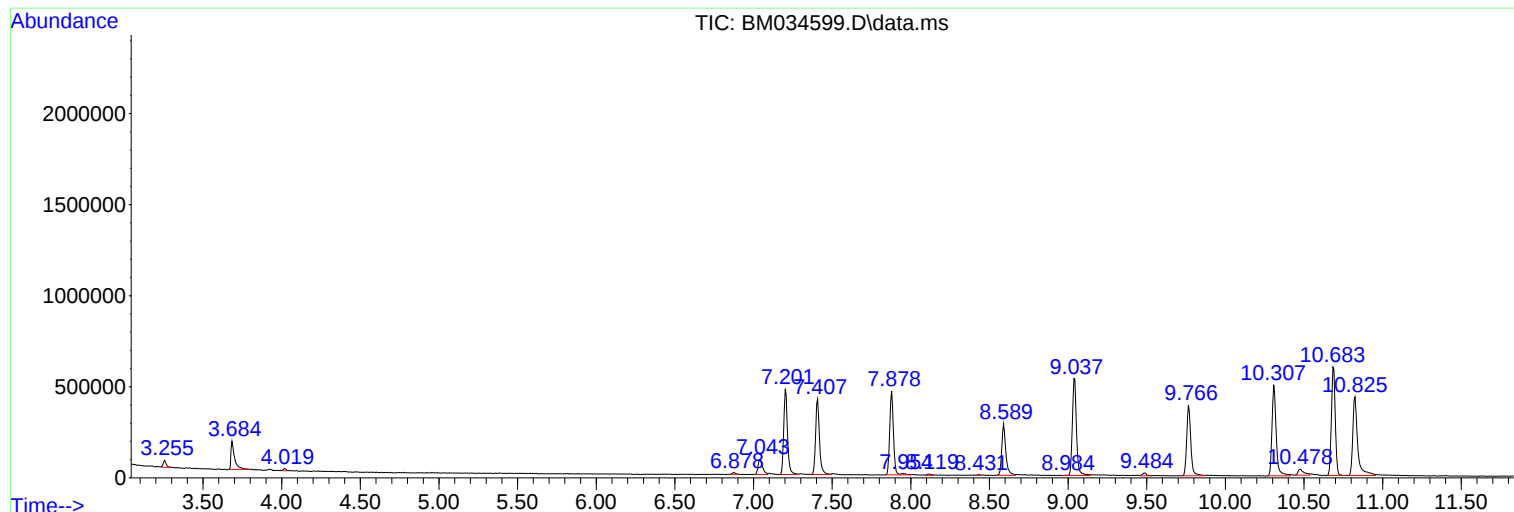

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis[2-(2-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.618	8.14 ng/ul	604946	Chrysene-d12	21.442

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis[2-(2-butox...	434	C22H42O8	000141-17-3	91
2			1-Decanamine	157	C10H23N	002016-57-1	22
3			Propane, 1,1'-[ethylidenebis(oxy...	174	C10H22O2	005669-09-0	22
4			Butane, 1,1'-[oxybis(2,1-ethaned...	218	C12H26O3	000112-73-2	16
5			2-(2-Butoxyethoxy)ethyl heptanoate	274	C15H30O4	1000367-04-4	16

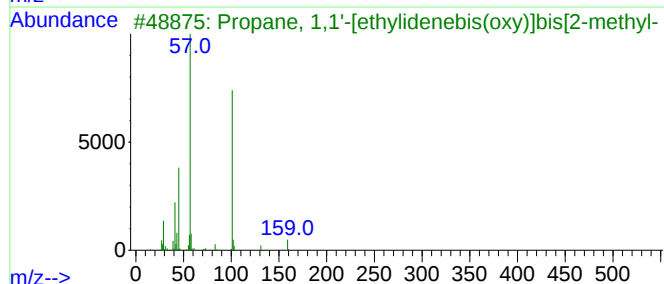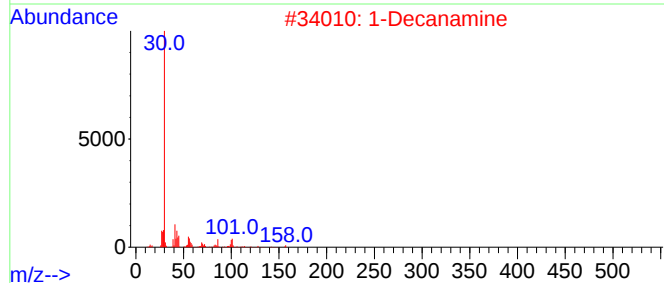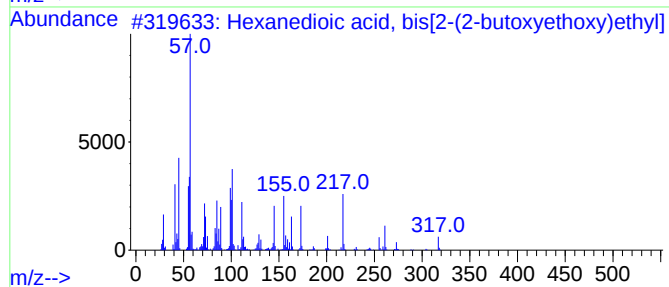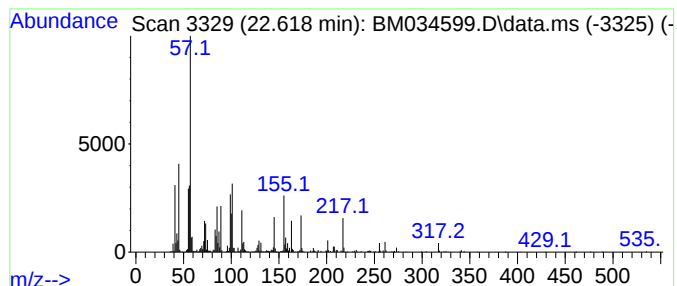

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040922\
Data File : BM034599.D
Acq On : 09 Apr 2022 15:08
Operator : CG/JU
Sample : N2266-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	22.618	8.1	ng/ul	604946	5	21.442	1487040	20.0