

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019864.D
 Acq On : 10 Apr 2019 15:21
 Operator : JU/SJ
 Sample : K2303-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A2

Quant Time: Apr 11 03:22:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	116845	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	500100	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	268445	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	576984	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	556549	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	589988	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	20653	6.92	ng/uL	0.00
5) Phenol-d5	6.75	99	217220	20.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	141697	20.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	181042	22.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	177456	22.72	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	82128	23.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	94011	23.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	153180	20.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	228566	25.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	520576	24.03	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	647909	23.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	58539	17.24	ng/ul	0.03
58) Fluorene-d10	15.22	176	432806	23.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	53004	13.89	ng/ul	0.00
71) Anthracene-d10	17.07	188	667233	24.10	ng/ul	0.00
79) Pyrene-d10	19.39	212	709538	27.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	727791	23.27	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.69	163	88052	4.052 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019864.D
Acq On : 10 Apr 2019 15:21
Operator : JU/SJ
Sample : K2303-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF8A2

Quant Time: Apr 11 03:22:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

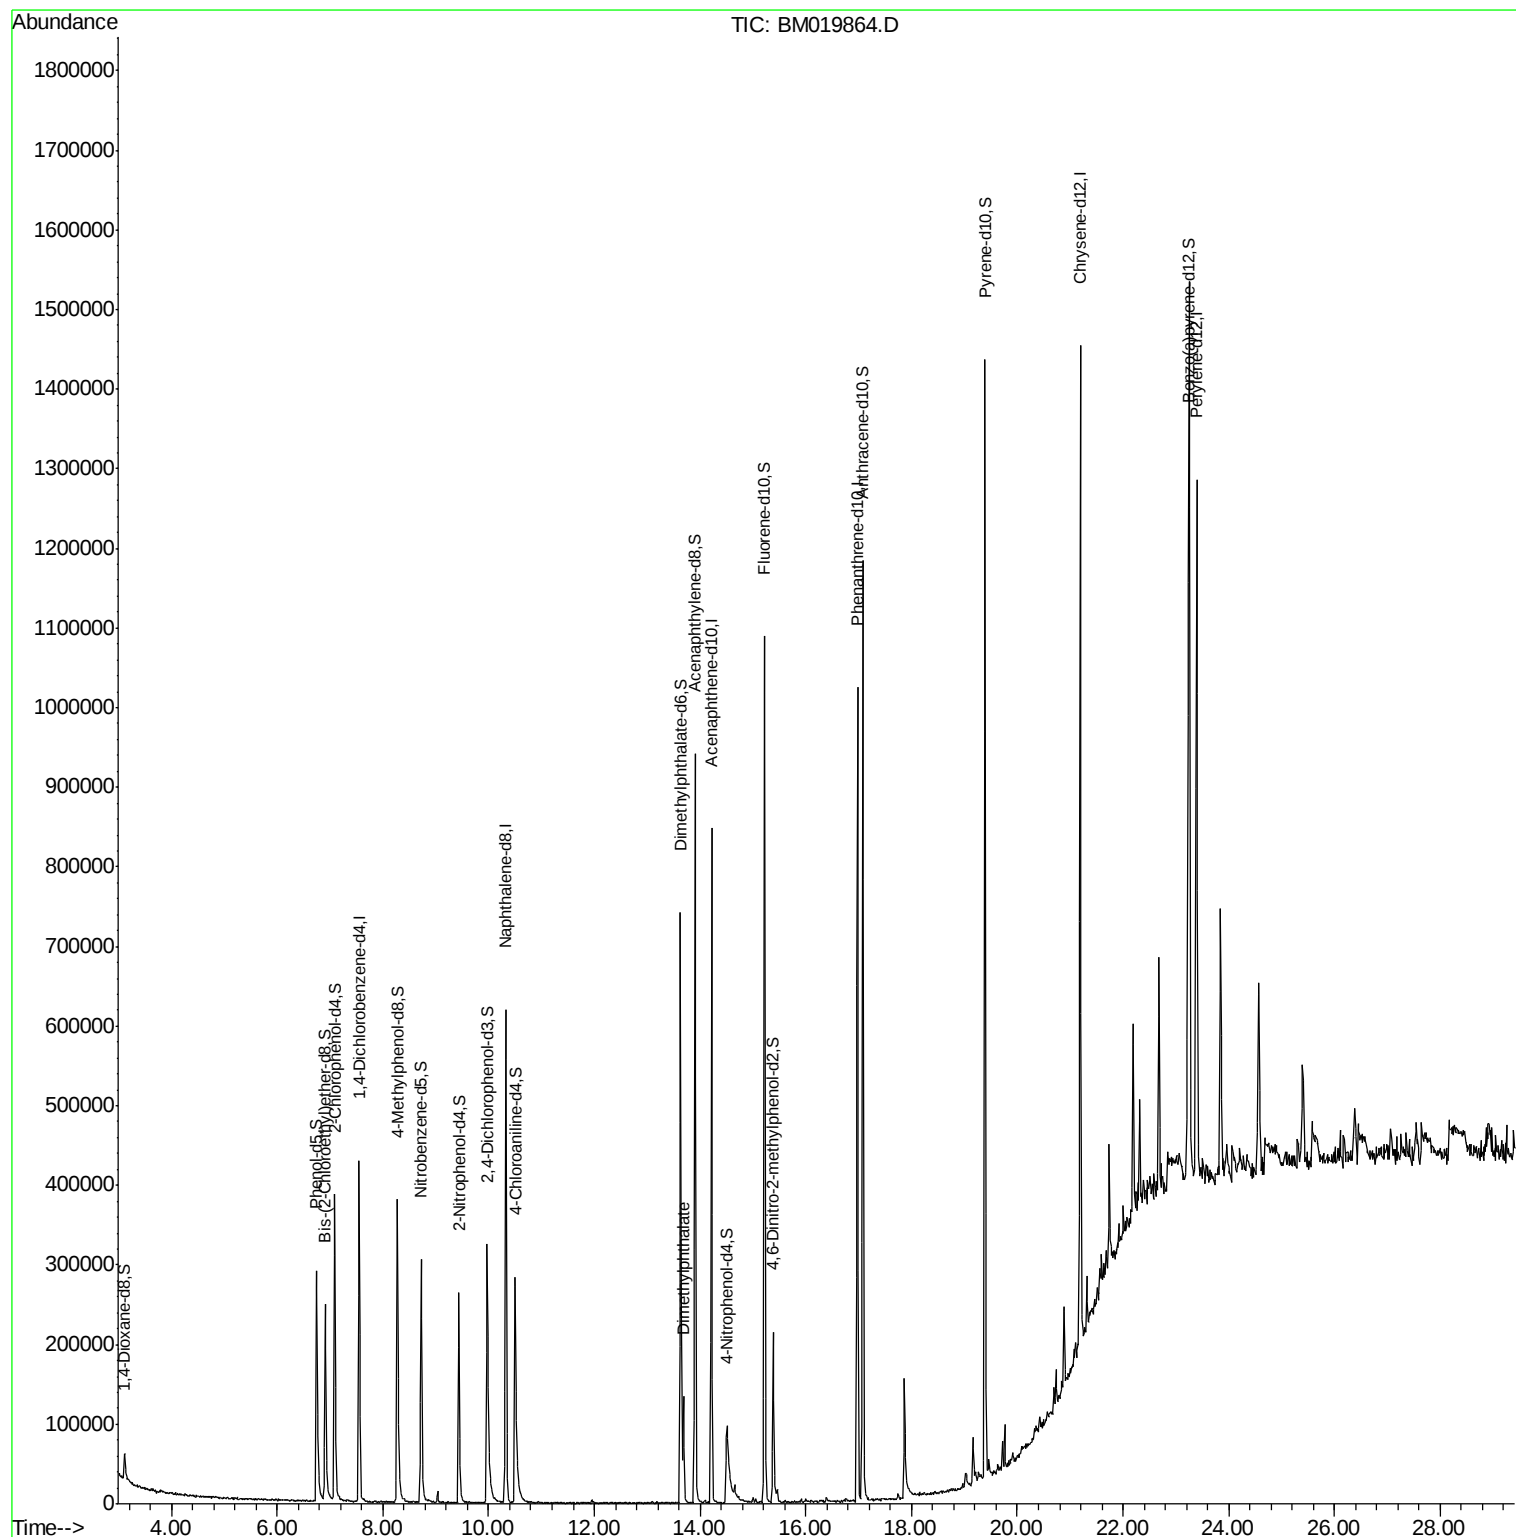

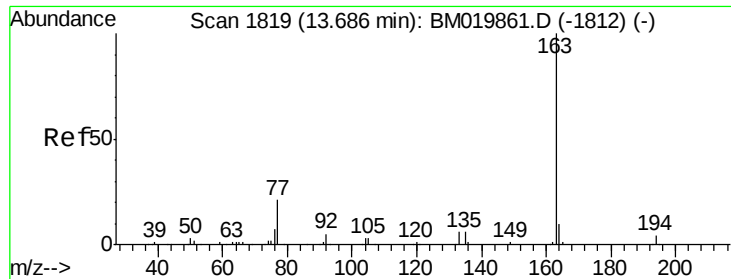

#45

Dimethylphthalate

Concen: 4.052 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM019864.D

Acq: 10 Apr 2019 15:21

Instrument :

BNA_M

ClientSampleId :

BF8A2


Tgt Ion:163 Resp: 88052

Ion Ratio Lower Upper

163 100

194 3.4 4.0 6.0#

164 10.4 8.4 12.6

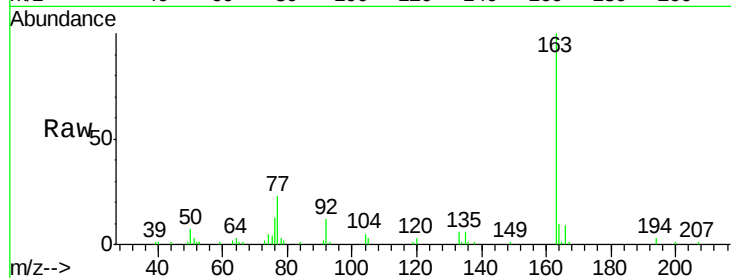

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

