

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019873.D
 Acq On : 10 Apr 2019 20:54
 Operator : JU/SJ
 Sample : K2303-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF883

Quant Time: Apr 11 03:23:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	117927	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	482959	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	252279	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	515187	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	474821	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	549736	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	20262	6.73	ng/uL	0.00
5) Phenol-d5	6.75	99	195054	18.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	136675	19.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	162407	20.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	144381	18.32	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	73687	21.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	84354	22.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	122275	16.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	183566	21.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	463358	22.76	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	519130	20.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	36509	11.44	ng/ul	0.04
58) Fluorene-d10	15.22	176	362627	20.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	42728	12.54	ng/ul	0.00
71) Anthracene-d10	17.07	188	525618	21.26	ng/ul	0.00
79) Pyrene-d10	19.39	212	534774	24.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	595350	20.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	98376	4.817	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019873.D
Acq On : 10 Apr 2019 20:54
Operator : JU/SJ
Sample : K2303-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF883

Quant Time: Apr 11 03:23:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

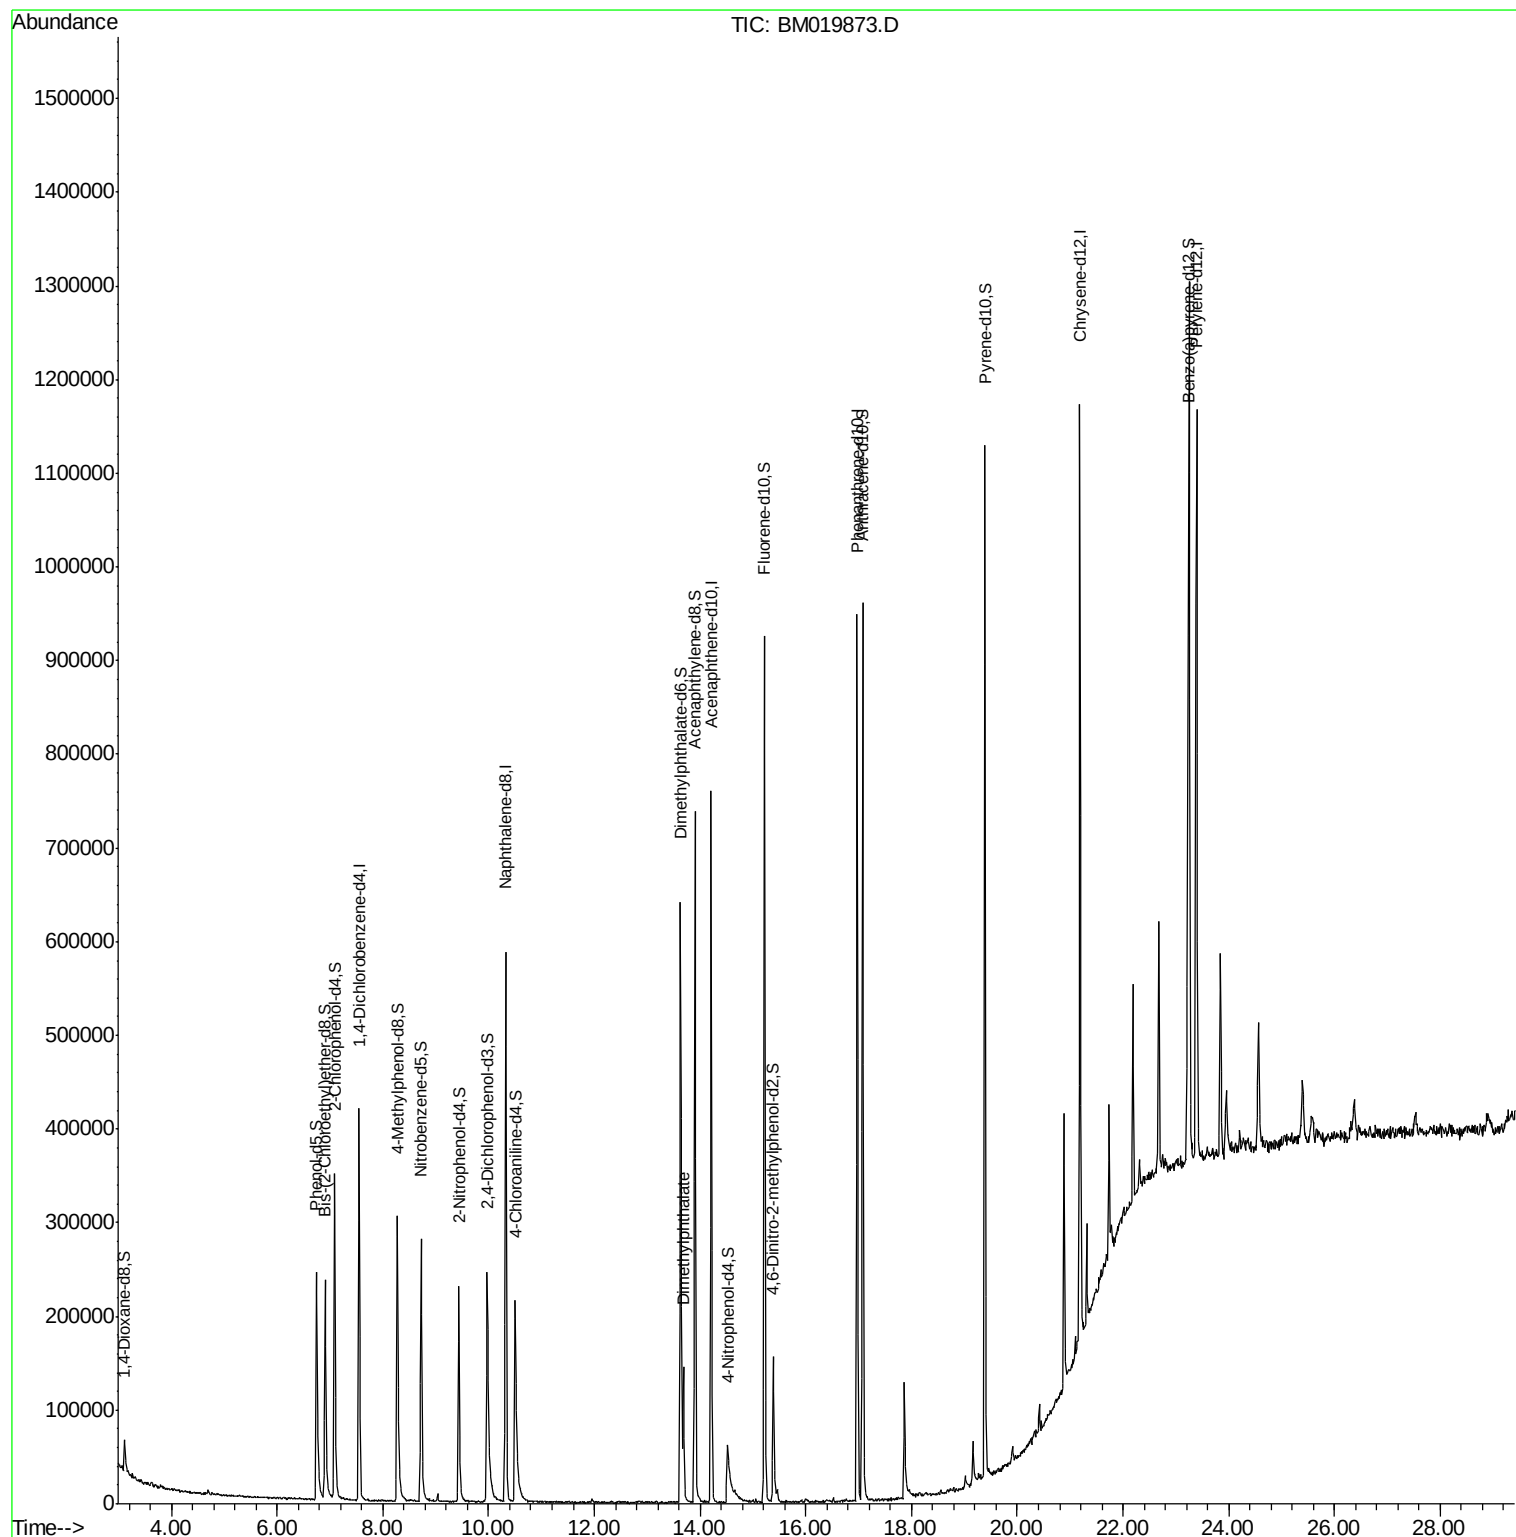

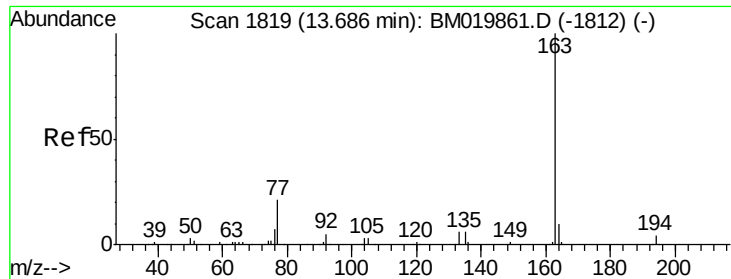

#45

Dimethylphthalate

Concen: 4.817 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM019873.D

Acq: 10 Apr 2019 20:54

Instrument :

BNA_M

ClientSampleId :

BF883


Tgt Ion:163 Resp: 98376

Ion Ratio Lower Upper

163 100

194 3.2 4.0 6.0#

164 9.3 8.4 12.6

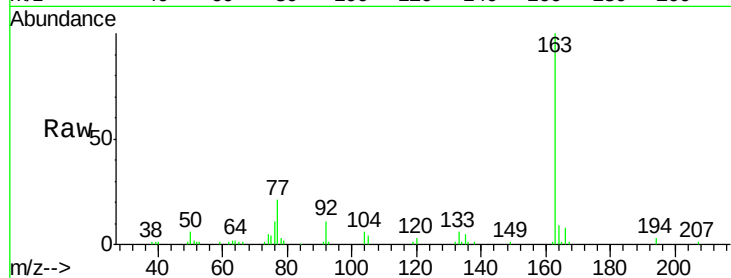

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

