

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019875.D
 Acq On : 10 Apr 2019 22:08
 Operator : JU/SJ
 Sample : K2303-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A4

Quant Time: Apr 11 03:23:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	118736	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	503559	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	273651	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	562685	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	497960	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	530087	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	20682	6.82	ng/uL	0.00
5) Phenol-d5	6.75	99	174372	16.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	121132	17.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	149577	18.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	137381	17.31	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	71237	19.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	77946	19.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	119077	15.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	162693	17.96	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	452092	20.47	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	521989	18.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	36500	10.55	ng/ul	0.04
58) Fluorene-d10	15.22	176	366978	19.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	40101	10.78	ng/ul	0.00
71) Anthracene-d10	17.07	188	545379	20.20	ng/ul	0.00
79) Pyrene-d10	19.39	212	572522	24.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	552551	19.66	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	84765	3.826	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019875.D
Acq On : 10 Apr 2019 22:08
Operator : JU/SJ
Sample : K2303-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF8A4

Quant Time: Apr 11 03:23:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

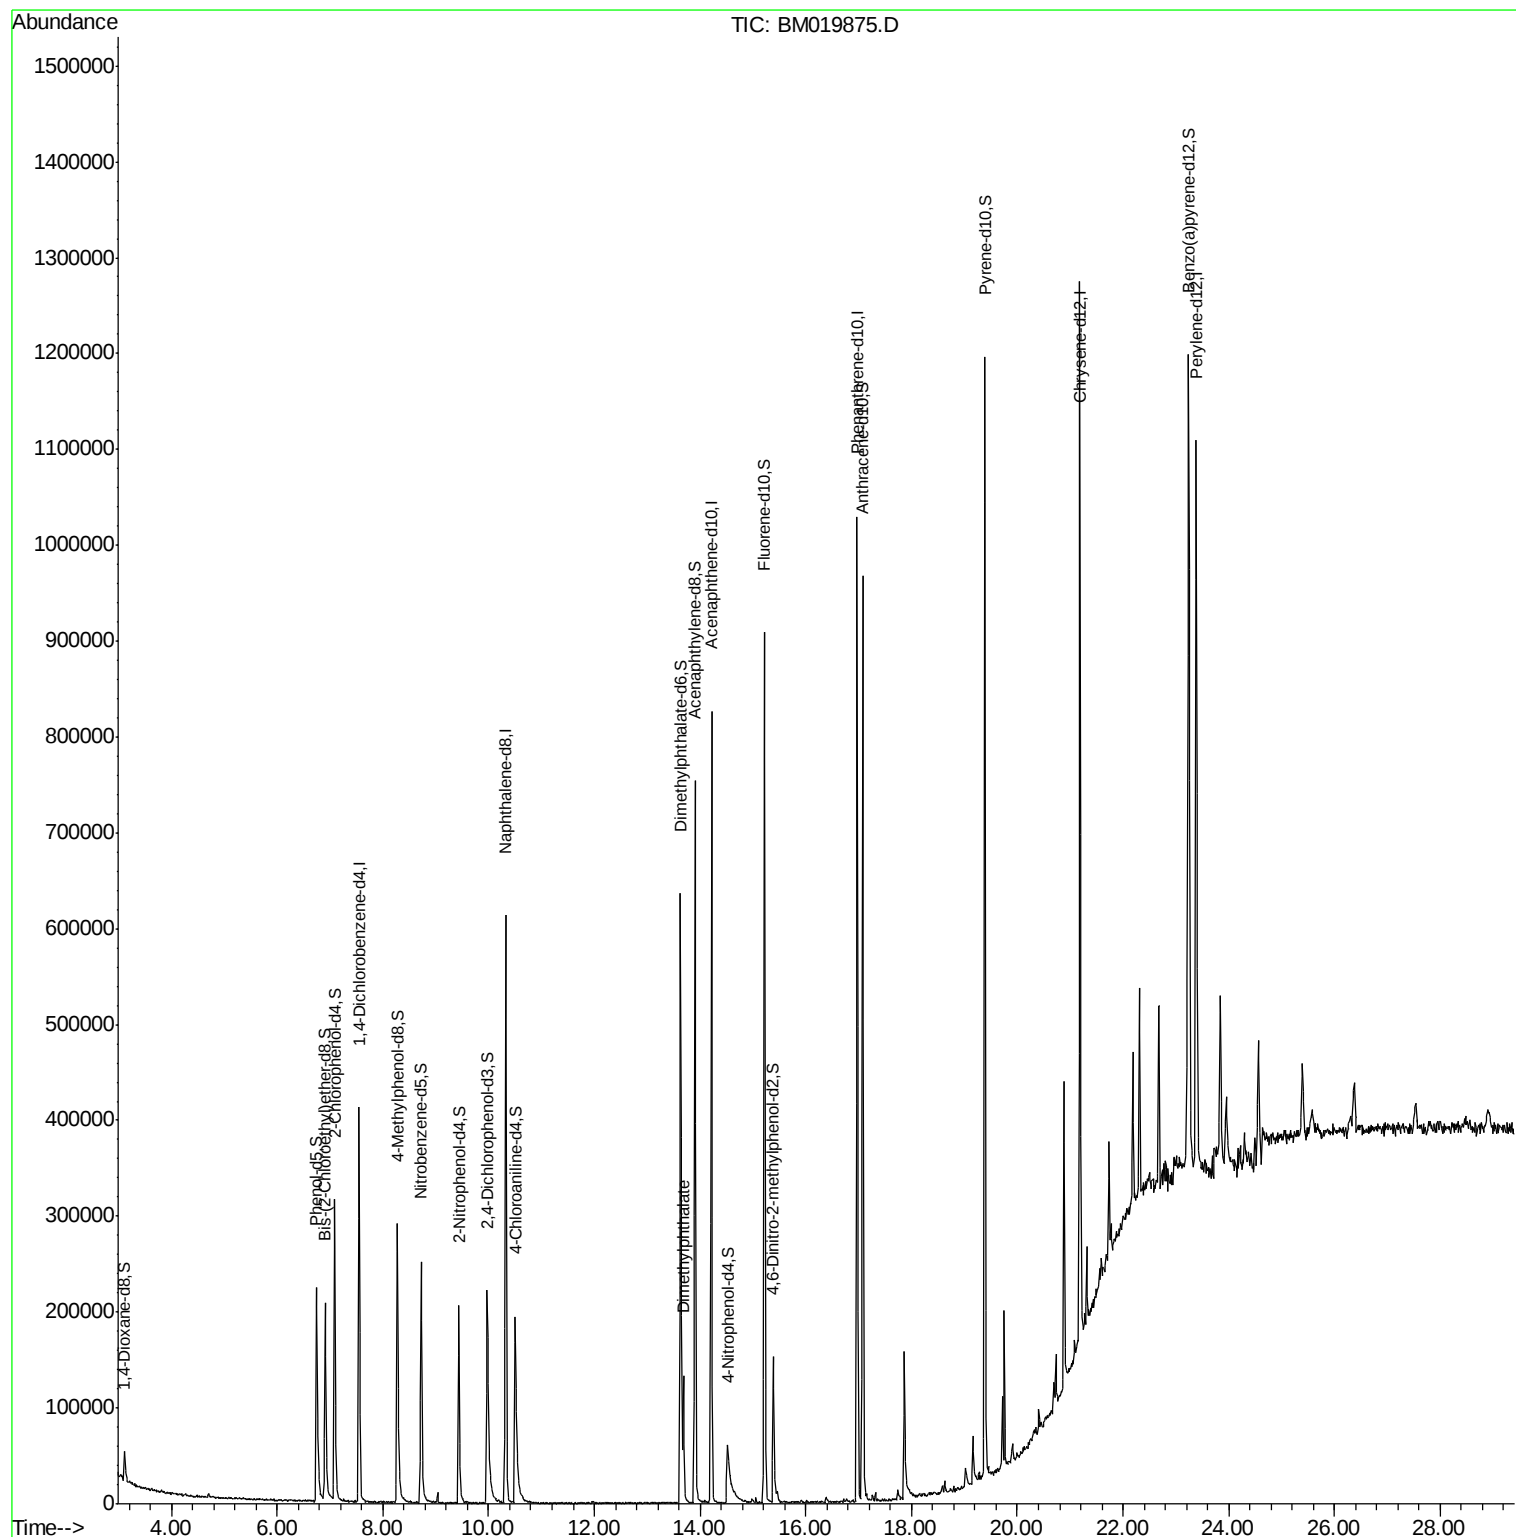

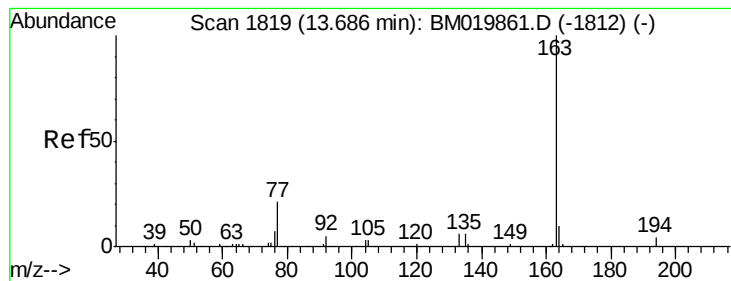

#45
 Dimethylphthalate
 Concen: 3.826 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. -0.00 min
 Lab File: BM019875.D
 Acq: 10 Apr 2019 22:08

Instrument :
 BNA_M
 ClientSampleId :
 BF8A4

Tgt Ion:	163	Resp:	84765
Ion	Ratio	Lower	Upper
163	100		
194	4.4	4.0	6.0
164	9.5	8.4	12.6

