

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019863.D
Acq On : 10 Apr 2019 14:45
Operator : JU/SJ
Sample : K2393-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF8A1

Quant Time: Apr 11 03:51:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/12/2019 5:17:55 PM

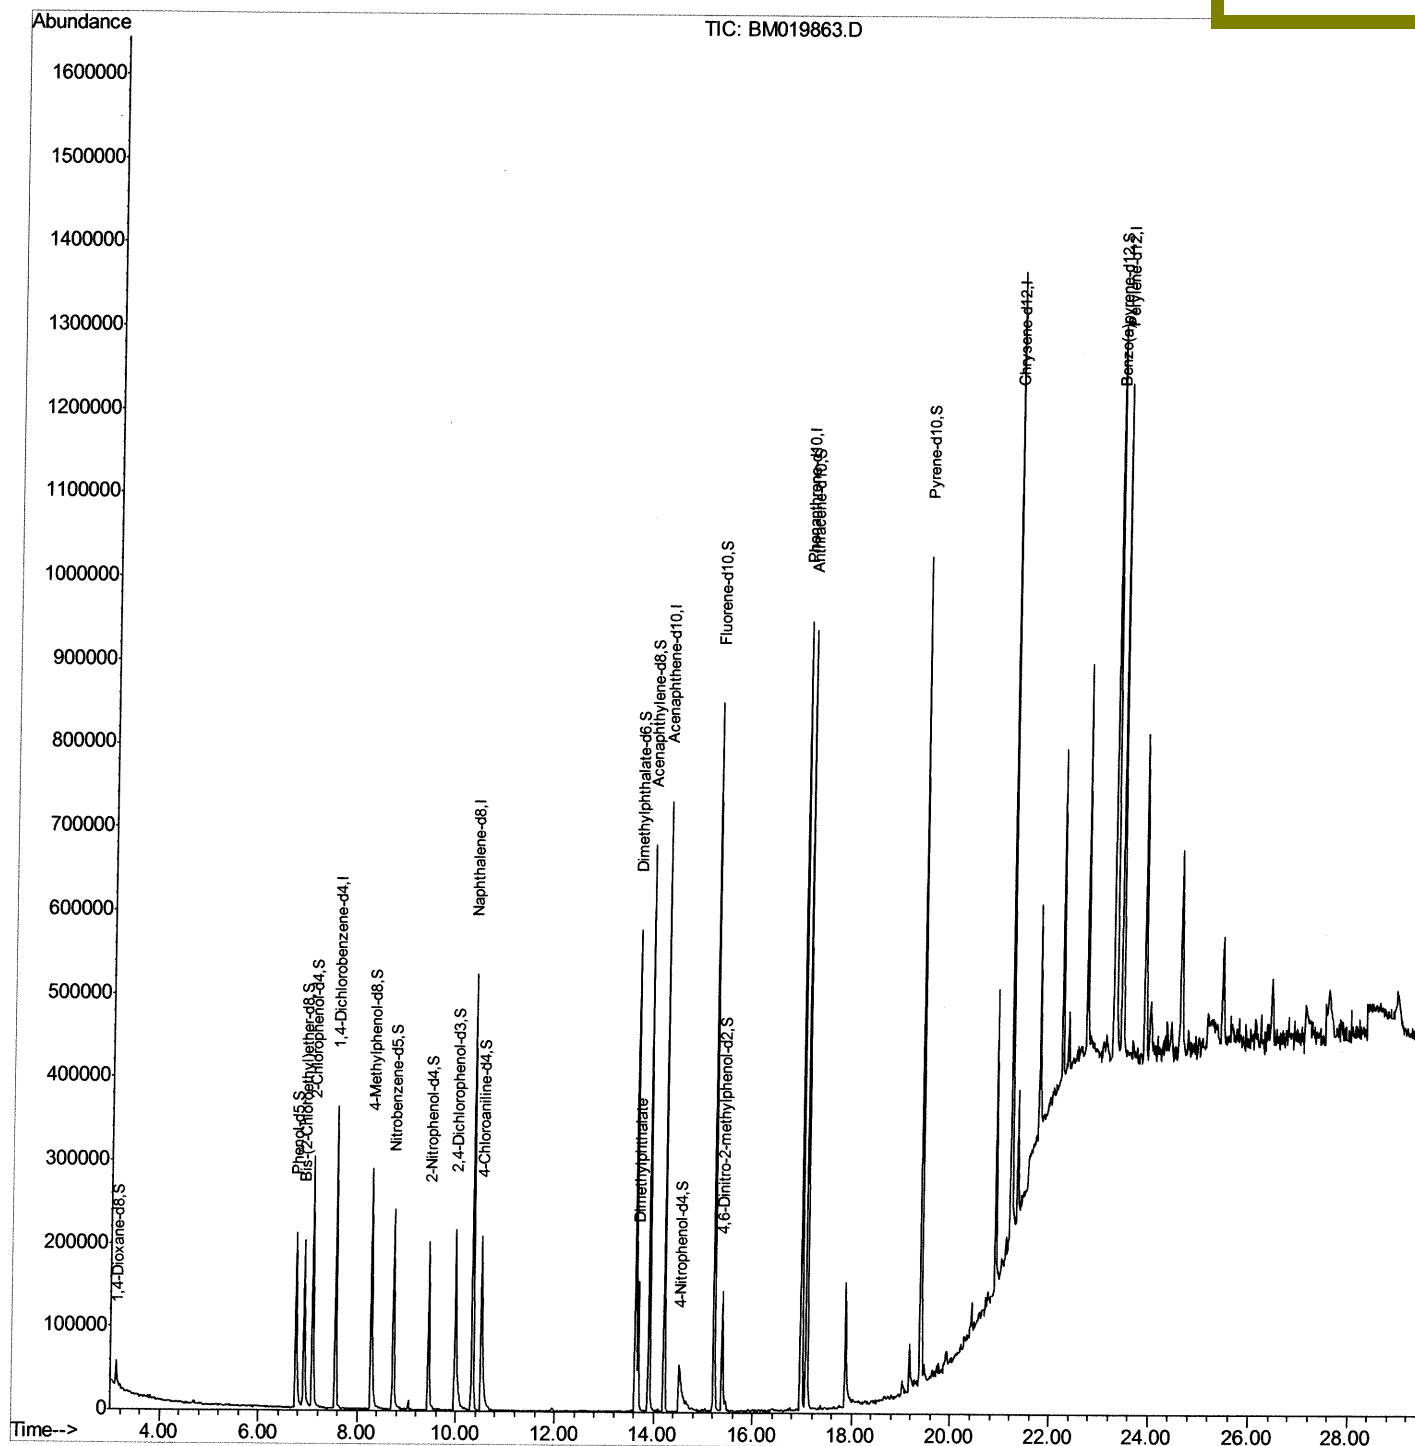

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019863.D
 Acq On : 10 Apr 2019 14:45
 Operator : JU/SJ
 Sample : K2393-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A1

Quant Time: Apr 11 03:22:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:17:55 PM

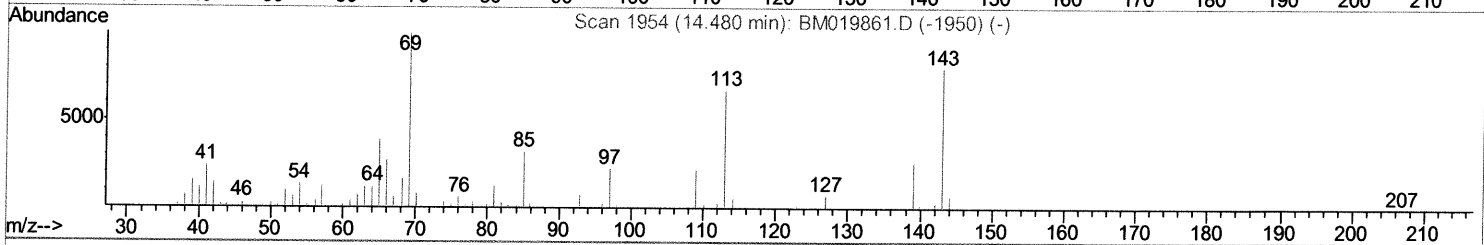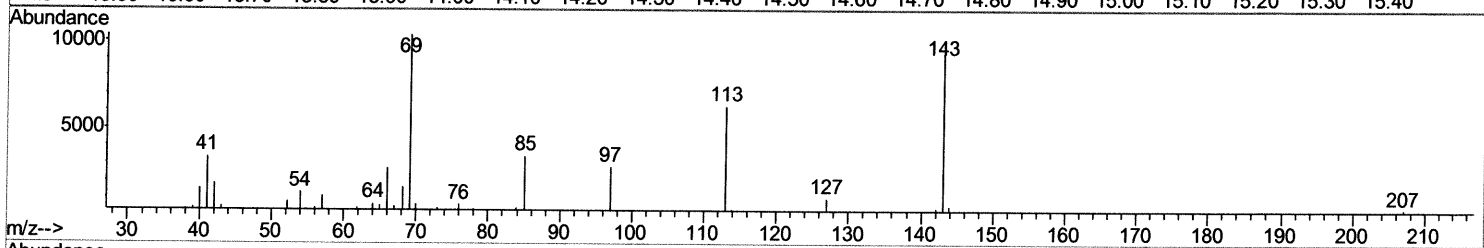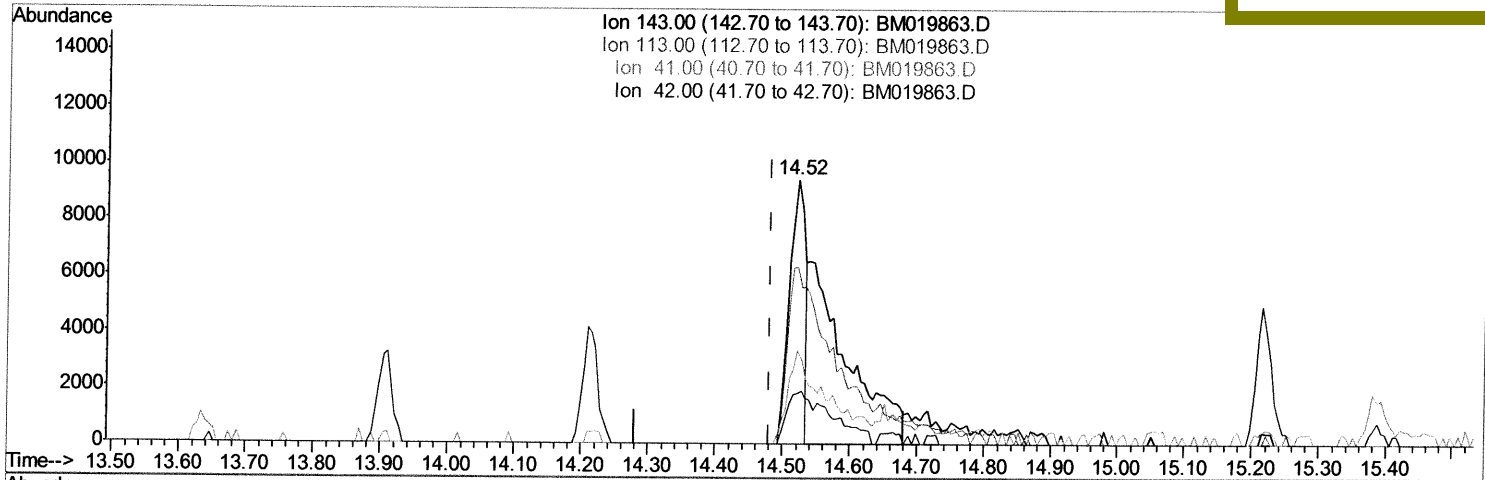

TIC: BM019863.D

(52) 4-Nitrophenol-d4 (S)

14.521min (+0.041) 5.21ng/ul

response 15506

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	67.01
41.00	32.60	35.52
42.00	22.30	19.16

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019863.D
 Acq On : 10 Apr 2019 14:45
 Operator : JU/SJ
 Sample : K2393-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A1

Quant Time: Apr 11 03:22:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:17:55 PM

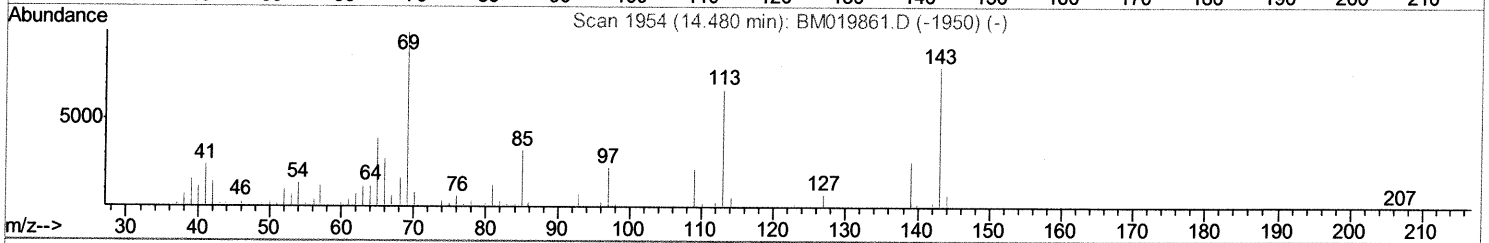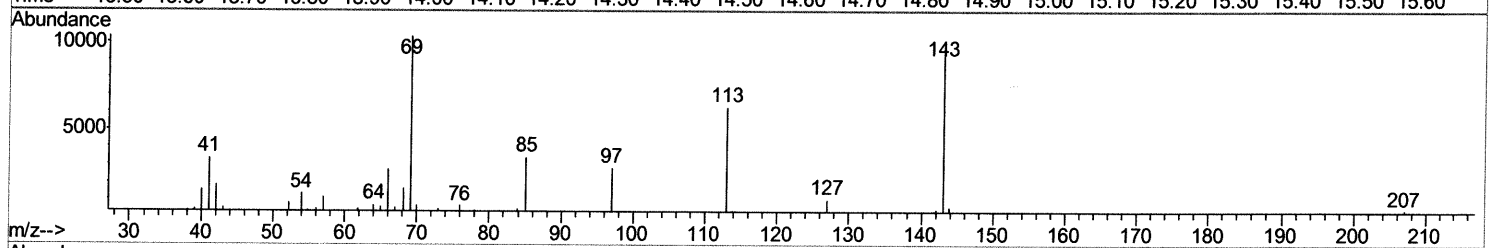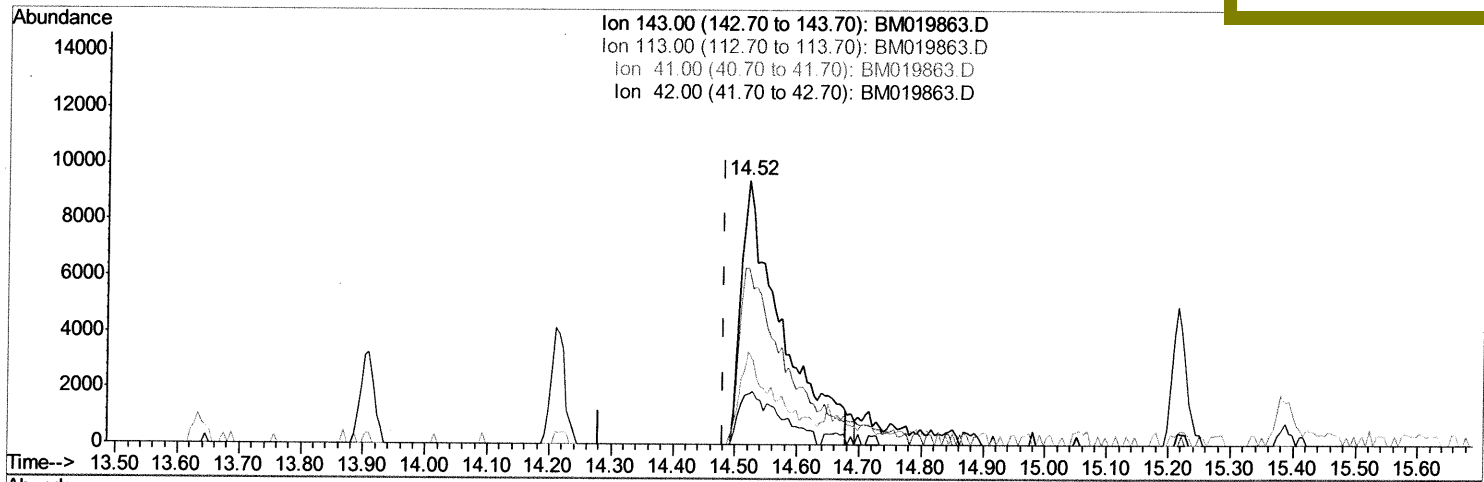

TIC: BM019863.D

(52) 4-Nitrophenol-d4 (S)

14.521min (+0.041) 14.38ng/ul m

response 42774

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	67.01
41.00	32.60	35.52
42.00	22.30	19.16

SJ 26/16/19

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019863.D
 Acq On : 10 Apr 2019 14:45
 Operator : JU/SJ
 Sample : K2393-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A1

Quant Time: Apr 11 03:51:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:17:55 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	100360	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	426005	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	235167	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	522544	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	517499	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	542470	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.12	96	21233	8.28	ng/uL	0.00
5) Phenol-d5	6.75	99	173424	19.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	115084	19.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	144540	21.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	139725	20.83	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	67979	22.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	75291	22.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	118586	18.58	ng/ul	0.01
29) 4-Chloroaniline-d4	10.50	131	166854	21.77	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	426892	22.50	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	483705	20.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	42774m	14.38	ng/ul	0.04
58) Fluorene-d10	15.22	176	348515	21.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	40321	11.67	ng/ul	0.00
71) Anthracene-d10	17.08	188	530884	21.17	ng/ul	0.00
79) Pyrene-d10	19.39	212	519084	21.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	527120	18.33	ng/ul	0.00

SJ
 04/16/19

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	104410	5.484	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed