

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019865.D
 Acq On : 10 Apr 2019 15:58
 Operator : JU/SJ
 Sample : K2303-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A3

Quant Time: Apr 11 03:55:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:00 PM

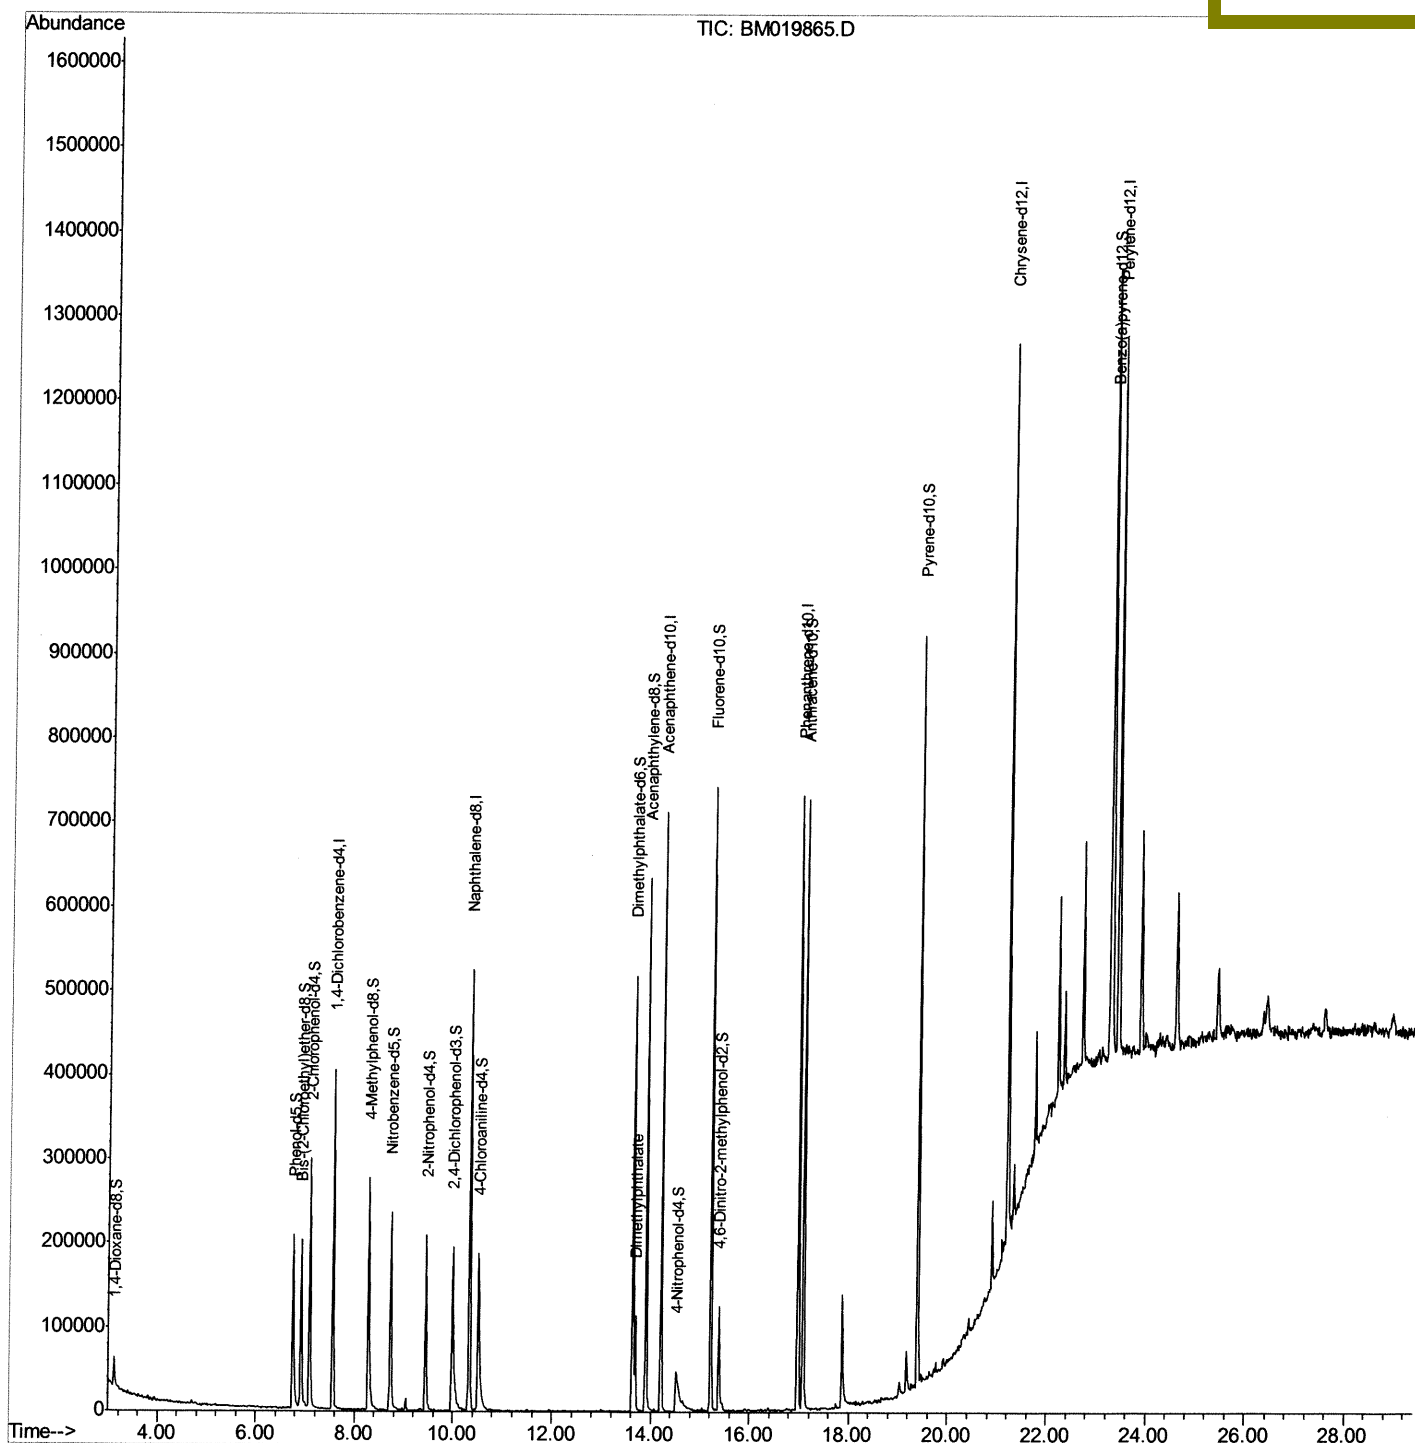

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019865.D
 Acq On : 10 Apr 2019 15:58
 Operator : JU/SJ
 Sample : K2303-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A3

Quant Time: Apr 11 03:23:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:00 PM

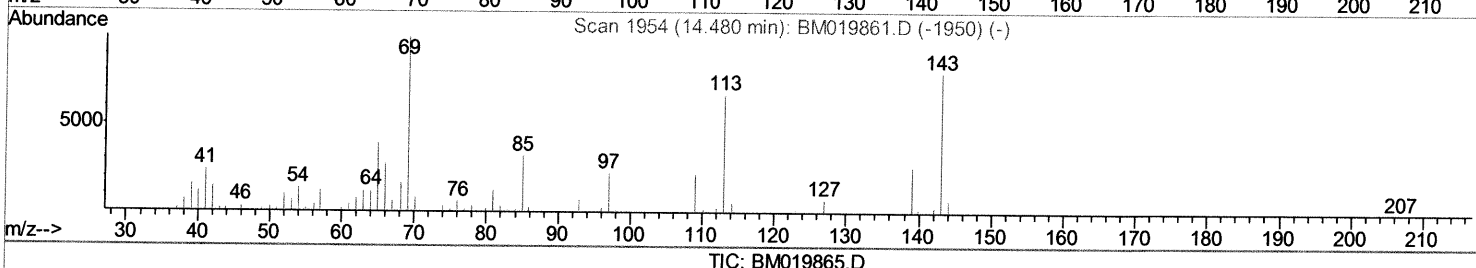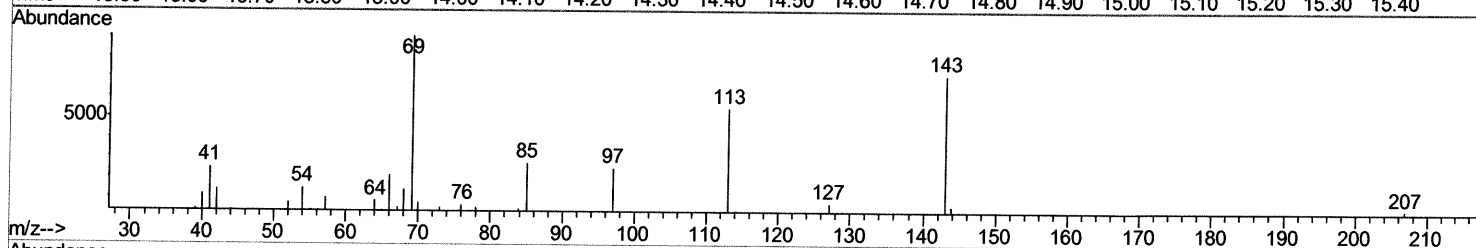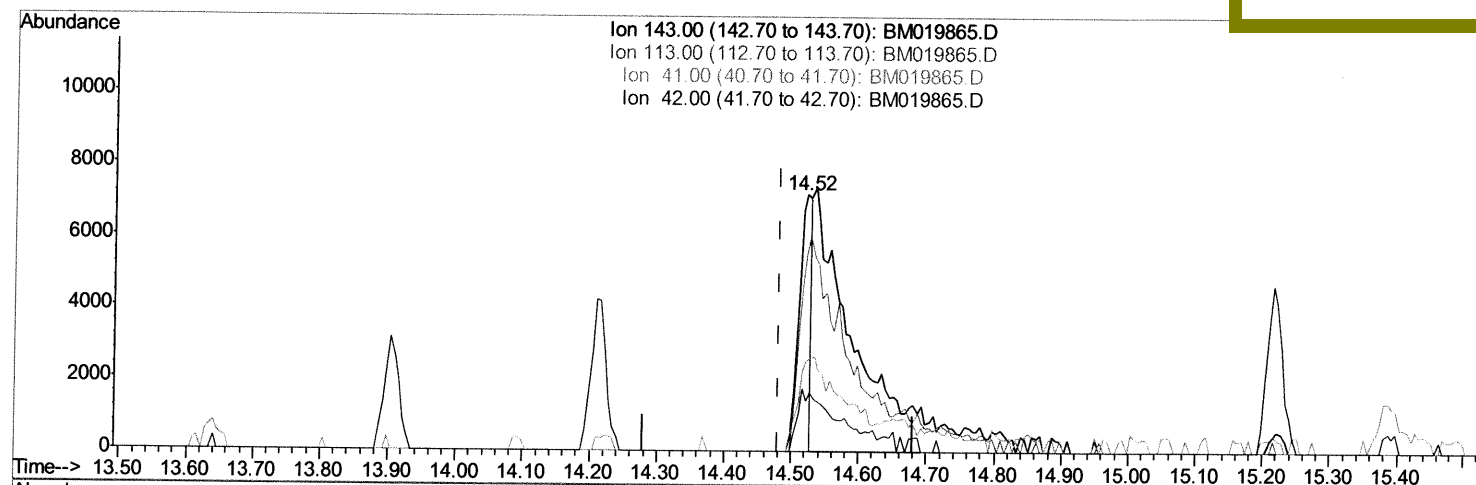

TIC: BM019865.D

(52) 4-Nitrophenol-d4 (S)

14.521min (+0.041) 3.36ng/ul

response 9611

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	76.81
41.00	32.60	34.97
42.00	22.30	19.63

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019865.D
 Acq On : 10 Apr 2019 15:58
 Operator : JU/SJ
 Sample : K2303-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A3

Quant Time: Apr 11 03:23:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:00 PM

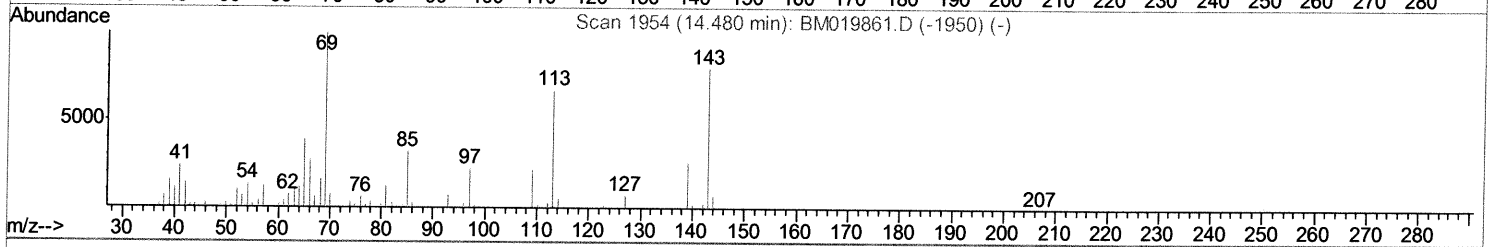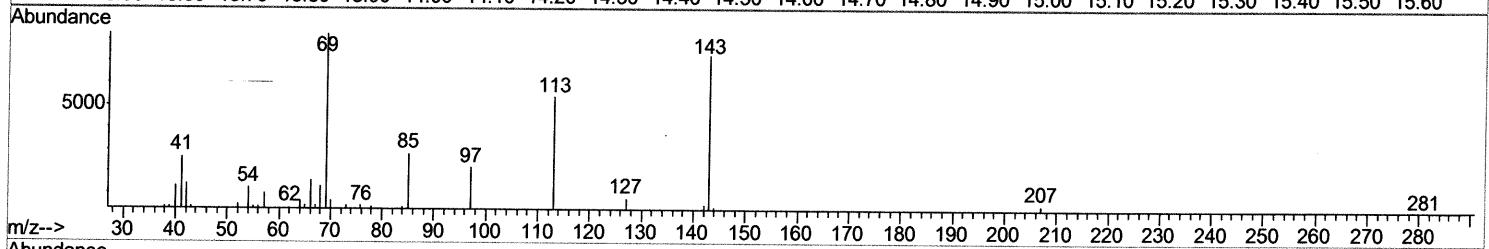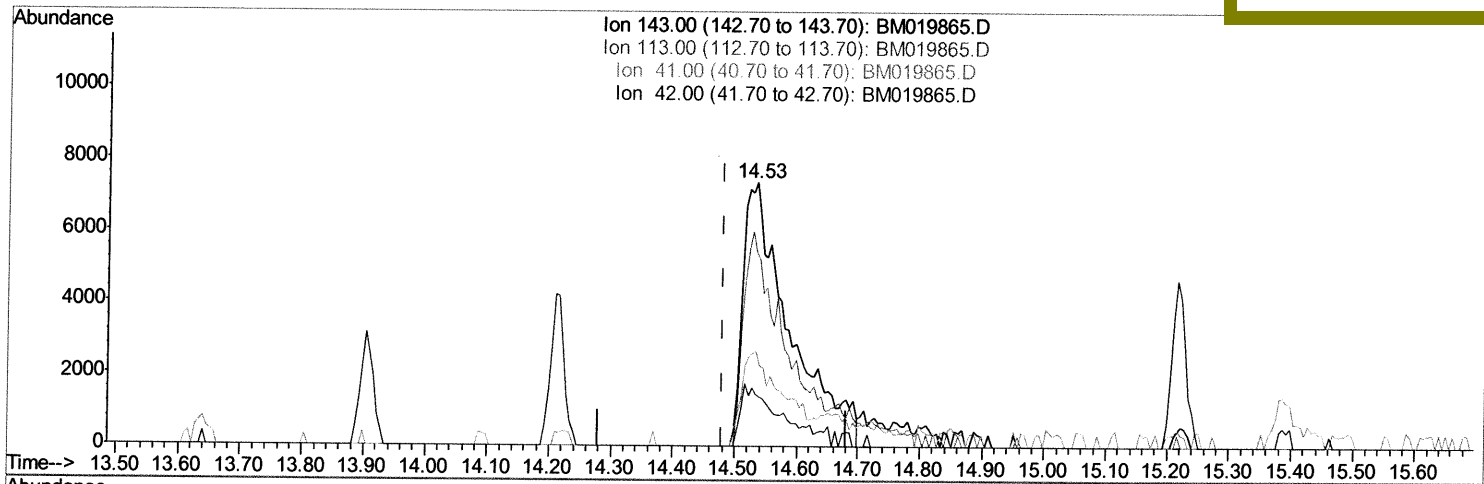

TIC: BM019865.D

(52) 4-Nitrophenol-d4 (S)

14.533min (+0.053) 13.52ng/ul m

response 38650

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	73.52
41.00	32.60	36.06
42.00	22.30	19.55

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019865.D
 Acq On : 10 Apr 2019 15:58
 Operator : JU/SJ
 Sample : K2303-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8A3

Quant Time: Apr 11 03:55:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:00 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	111429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	427819	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	225950	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	427963	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	479642	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	575993	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	21554	7.57	ng/uL	0.00
5) Phenol-d5	6.75	99	171228	17.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	118228	17.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	141113	18.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	135061	18.13	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	64951	21.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	76902	22.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	112439	17.54	ng/ul	0.01
29) 4-Chloroaniline-d4	10.51	131	159398	20.71	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	384382	21.08	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	463625	20.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	38650m	13.52	ng/ul	0.05
58) Fluorene-d10	15.22	176	311666	19.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	33788	11.94	ng/ul	0.00
71) Anthracene-d10	17.08	188	433039	21.09	ng/ul	0.00
79) Pyrene-d10	19.39	212	456710	20.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	579621	18.98	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	70479	3.853	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed